

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040419\
 Data File : BF113589.D
 Acq On : 4 Apr 2019 18:10
 Operator : JU/SJ
 Sample : K2221-04
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S2B(2-10)COMP

Quant Time: Apr 05 04:33:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	109203	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	405977	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	201163	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	441045	20.00	ng	-0.02
76) Chrysene-d12	13.82	240	434763	20.00	ng	-0.03
87) Perylene-d12	15.22	264	406259	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	759542	118.60	ng	0.00
7) Phenol-d6	6.33	99	870295	110.26	ng	-0.01
23) Nitrobenzene-d5	7.25	82	679506	98.04	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	391070	161.84	ng	-0.02
45) 2-Fluorobiphenyl	9.04	172	1269857	101.63	ng	-0.01
79) Terphenyl-d14	12.77	244	1696907	79.47	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040419\
Data File : BF113589.D
Acq On : 4 Apr 2019 18:10
Operator : JU/SJ
Sample : K2221-04
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S2B(2-10)COMP

Quant Time: Apr 05 04:33:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

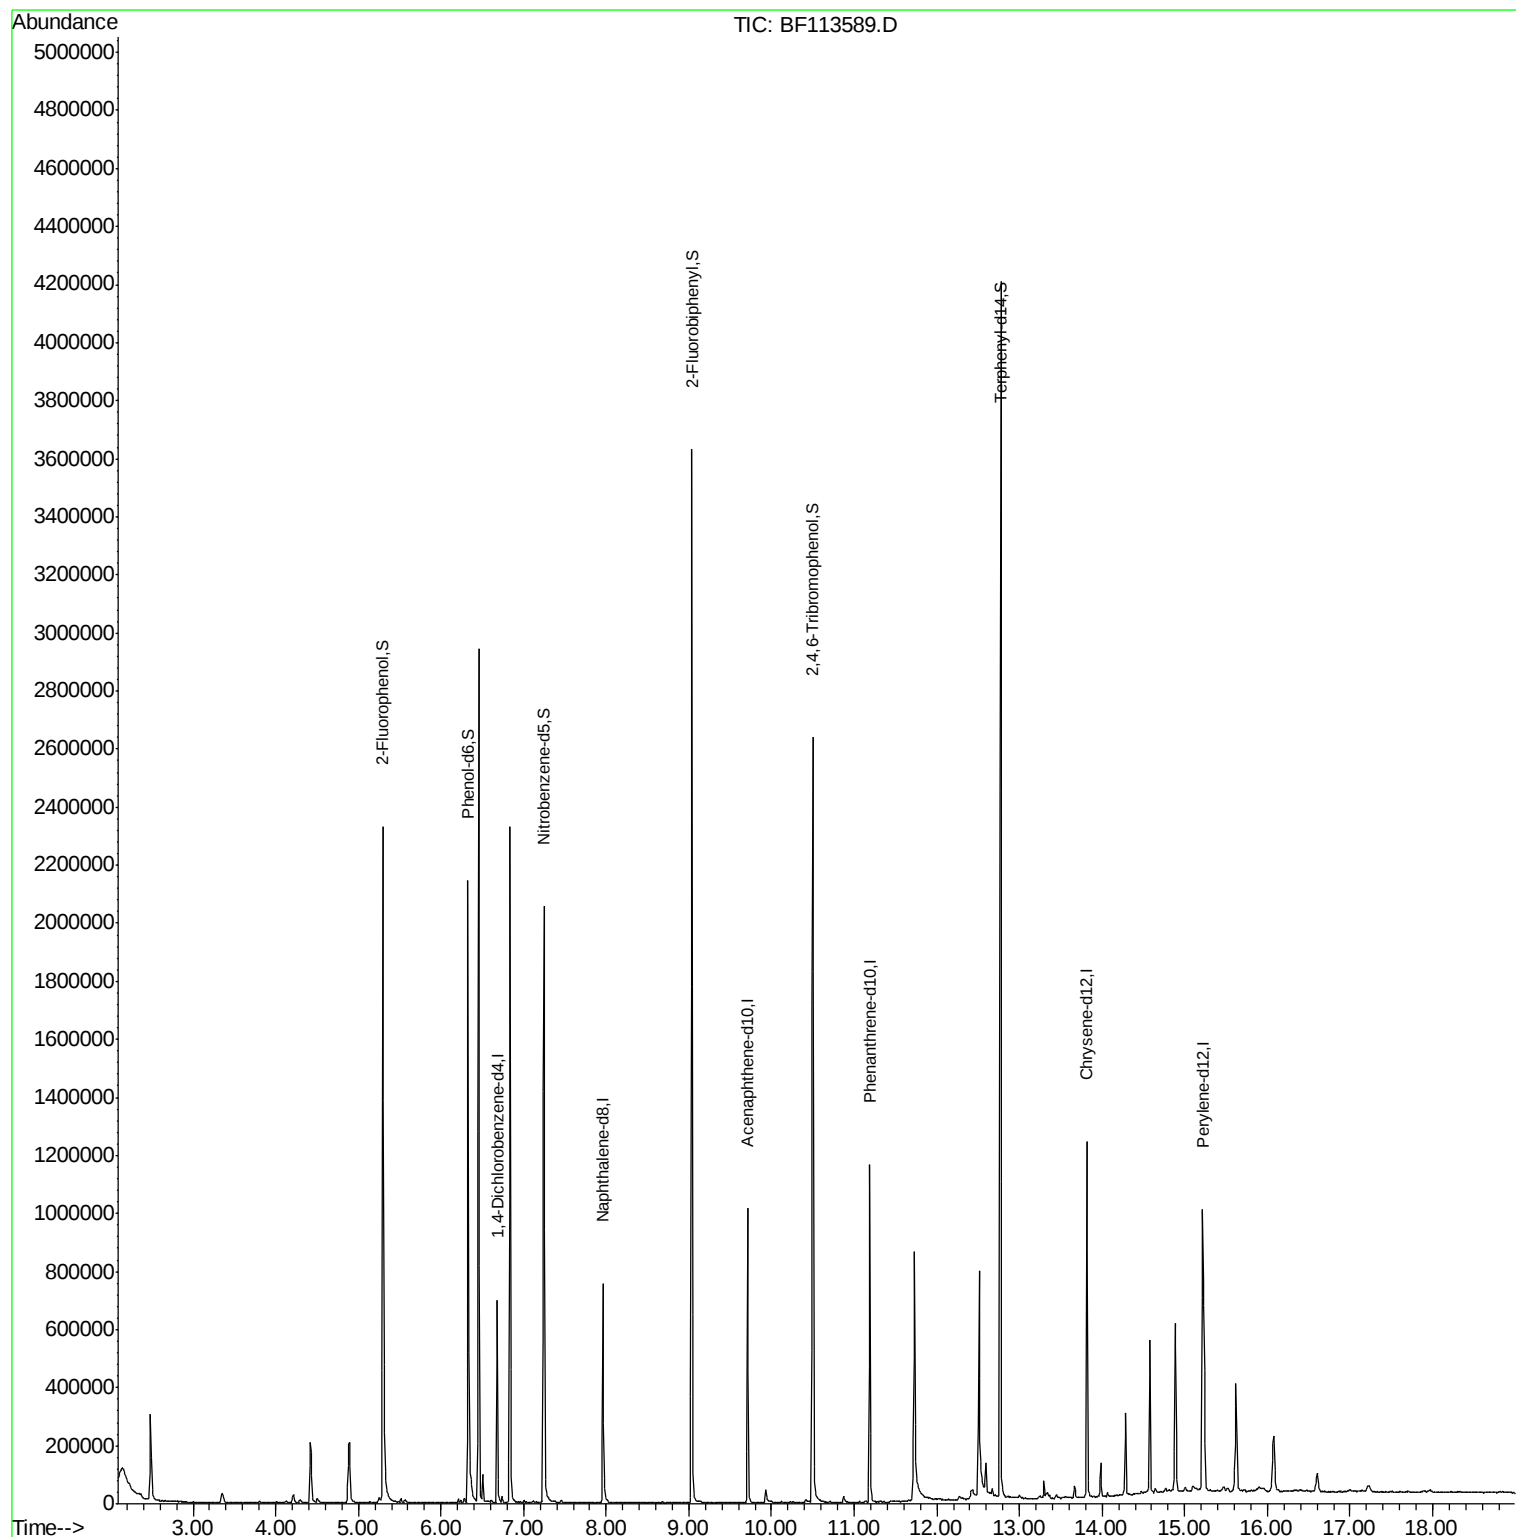

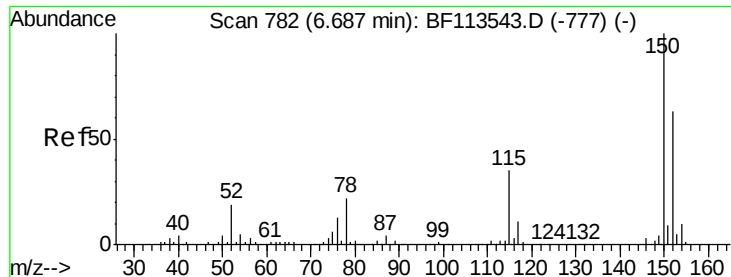


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.68 min Scan# 781
Delta R.T. -0.01 min
Lab File: BF113589.D
Acq: 4 Apr 2019 18:10

Instrument :
BNA_F
ClientSampleId :
S2B(2-10)COMP

Tgt Ion:152 Resp: 109203
Ion Ratio Lower Upper
152 100
150 154.3 124.7 187.1
115 53.6 46.0 69.0

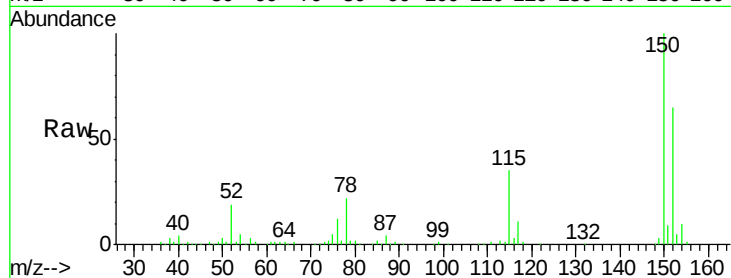


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

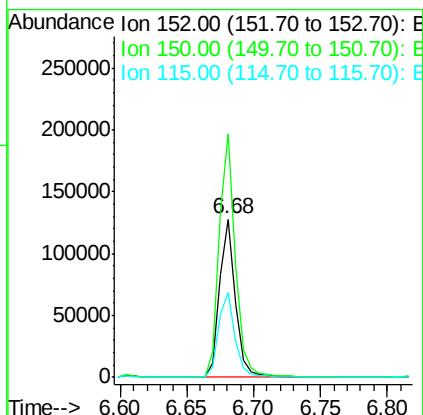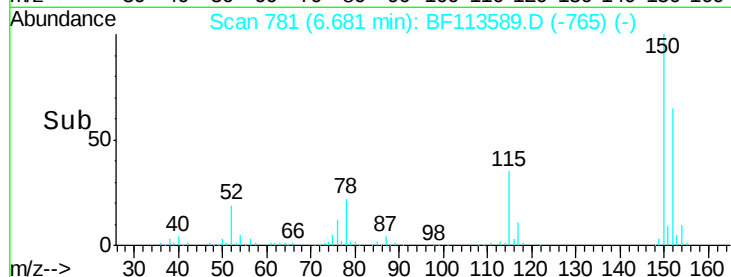



#5


2-Fluorophenol
Concen: 118.604 ng
RT: 5.30 min Scan# 546
Delta R.T. 0.00 min
Lab File: BF113589.D
Acq: 4 Apr 2019 18:10

Tgt Ion:112 Resp: 759542
Ion Ratio Lower Upper
112 100
64 58.7 49.2 73.8
63 30.0 24.9 37.3

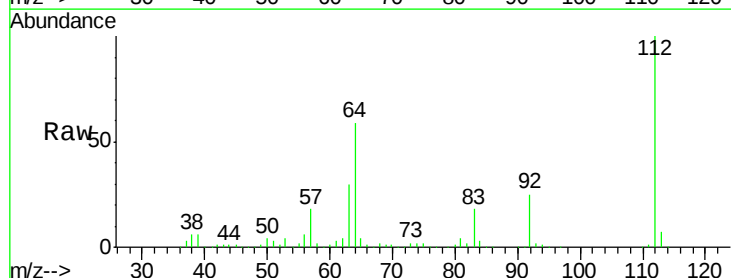

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

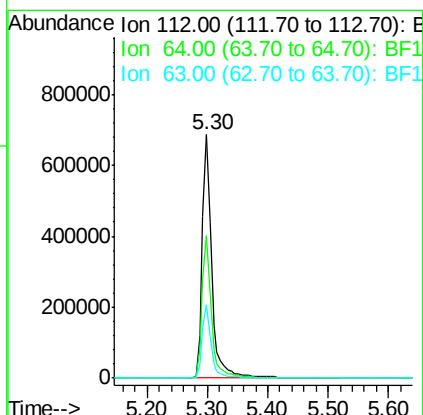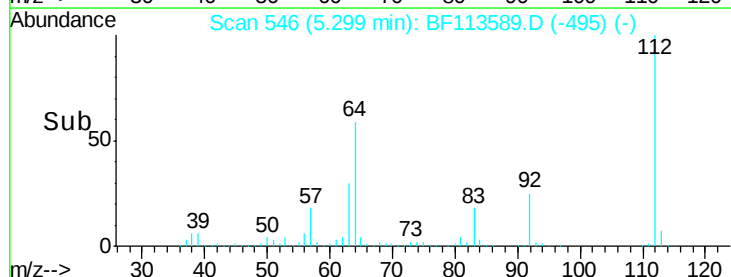

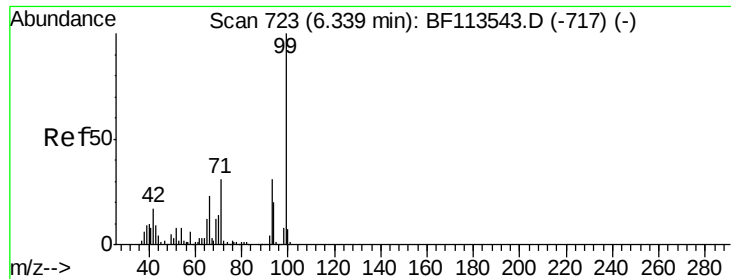

#7

Phenol-d6

Concen: 110.262 ng

RT: 6.33 min Scan# 721

Delta R.T. -0.01 min

Lab File: BF113589.D

Acq: 4 Apr 2019 18:10

Instrument :

BNA_F

ClientSampleId :

S2B(2-10)COMP





Tgt Ion: 99 Resp: 870295

Ion Ratio Lower Upper

99 100

42 18.2 14.8 22.2

71 31.2 24.9 37.3

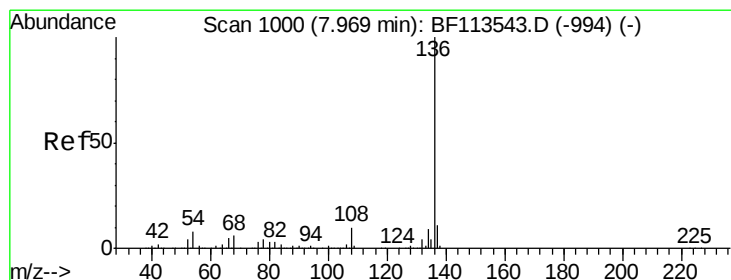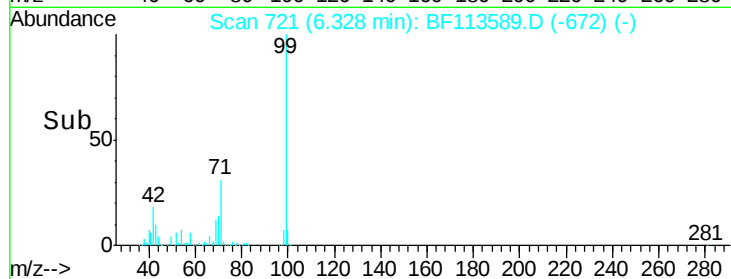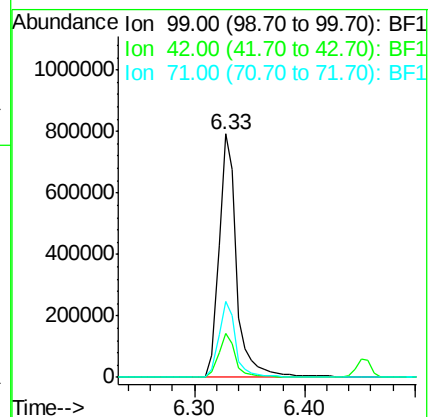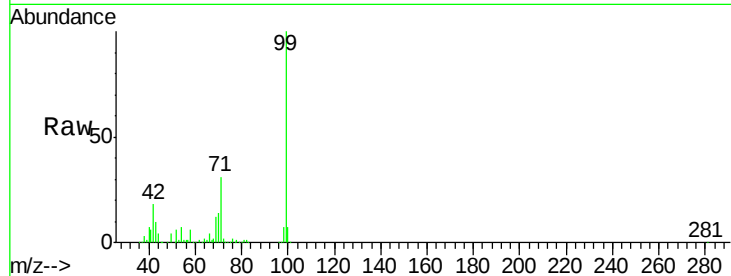

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 999

Delta R.T. -0.01 min

Lab File: BF113589.D

Acq: 4 Apr 2019 18:10

Tgt Ion: 136 Resp: 405977




Ion Ratio Lower Upper

136 100

137 10.6 8.9 13.3

54 7.1 7.0 10.6

68 5.3 4.8 7.2

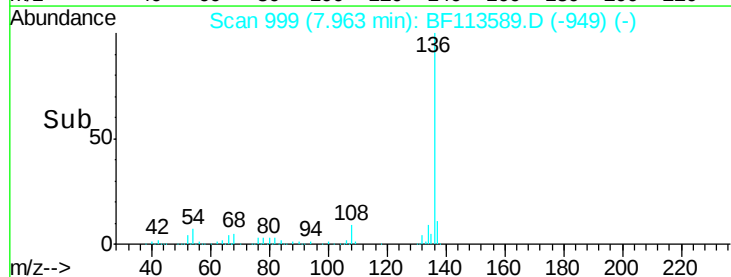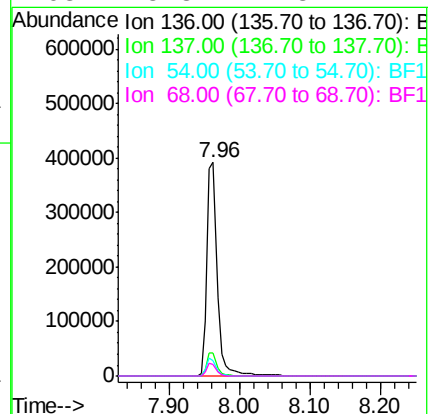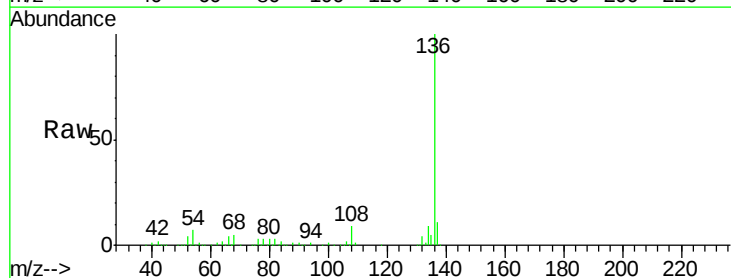







#23
Nitrobenzene-d5
Concen: 98.041 ng
RT: 7.25 min Scan# 877
Delta R.T. -0.01 min
Lab File: BF113589.D
Acq: 4 Apr 2019 18:10

Instrument :
BNA_F
ClientSampleId :
S2B(2-10)COMP

Tgt Ion: 82 Resp: 679506
Ion Ratio Lower Upper
82 100
128 47.1 36.5 54.7
54 51.4 42.2 63.2

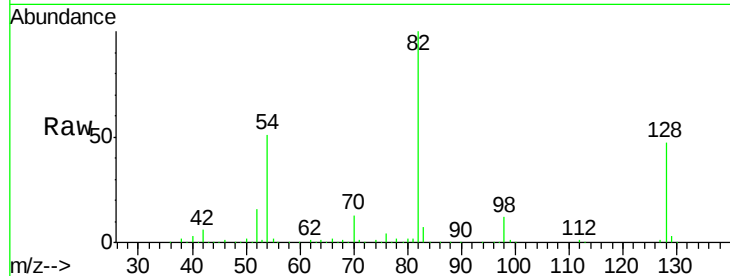


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

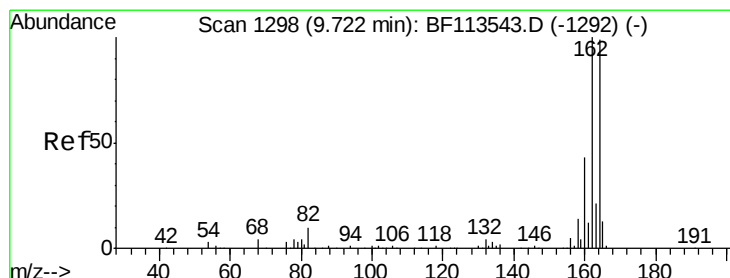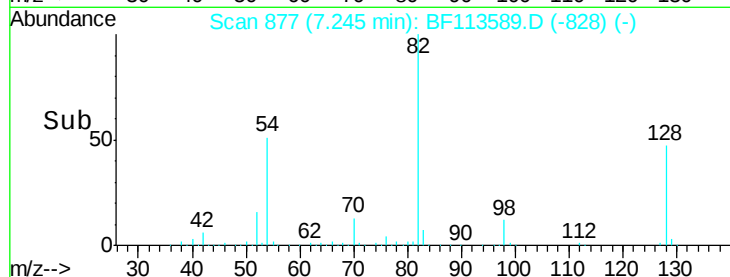
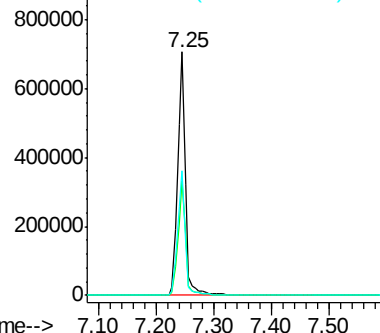


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.71 min Scan# 1296
Delta R.T. -0.01 min
Lab File: BF113589.D
Acq: 4 Apr 2019 18:10

Tgt Ion: 164 Resp: 201163
Ion Ratio Lower Upper
164 100
162 101.6 81.8 122.6
160 44.7 36.4 54.6

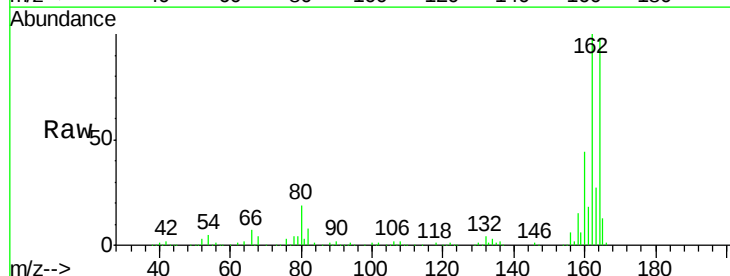

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

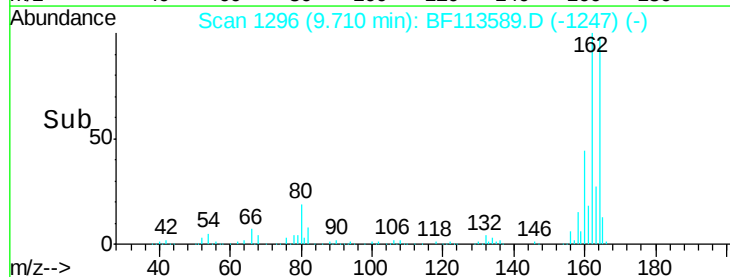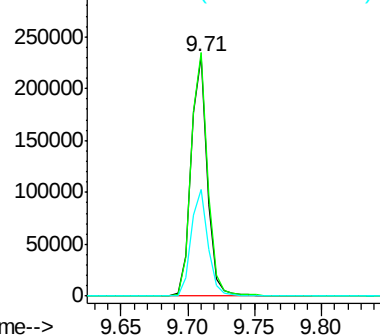







#42
 2,4,6-Tribromophenol
 Concen: 161.836 ng
 RT: 10.50 min Scan# 1430
 Delta R.T. -0.02 min
 Lab File: BF113589.D
 Acq: 4 Apr 2019 18:10

Instrument :
 BNA_F
 ClientSampleId :
 S2B(2-10)COMP

Tgt Ion:330 Resp: 391070
 Ion Ratio Lower Upper
 330 100
 332 95.4 77.8 116.6
 141 27.3 22.7 34.1

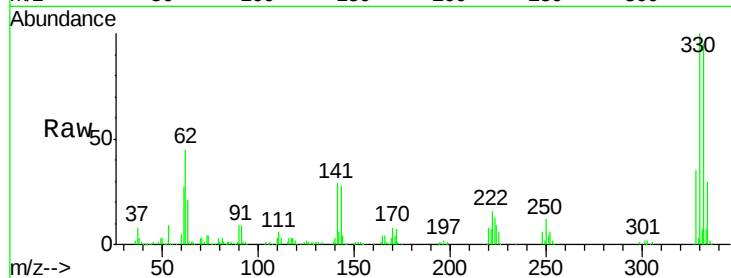


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

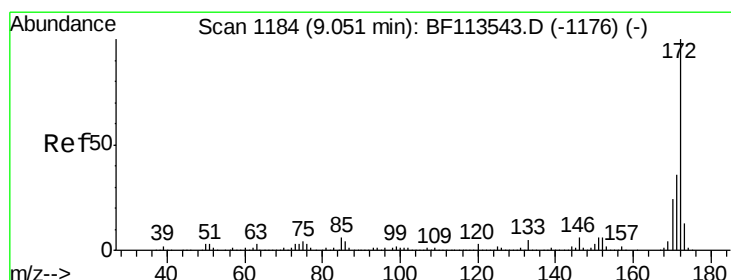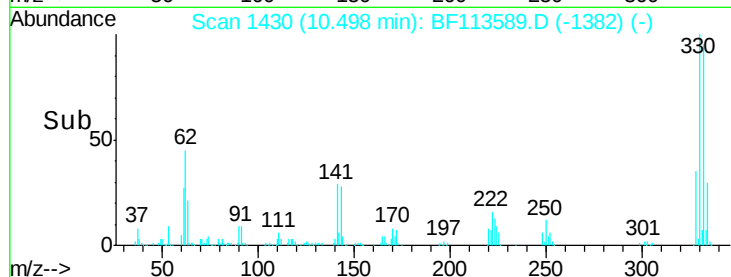
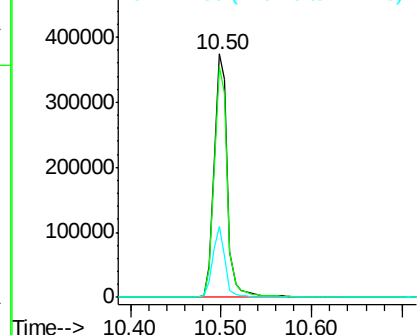



#45
 2-Fluorobiphenyl
 Concen: 101.626 ng
 RT: 9.04 min Scan# 1182
 Delta R.T. -0.01 min
 Lab File: BF113589.D
 Acq: 4 Apr 2019 18:10

Tgt Ion:172 Resp: 1269857
 Ion Ratio Lower Upper
 172 100
 171 35.2 29.0 43.6
 170 24.0 19.5 29.3

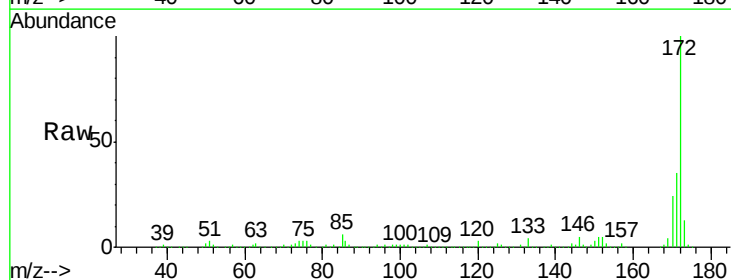

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



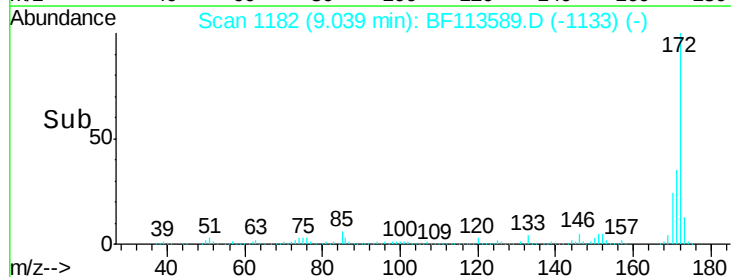
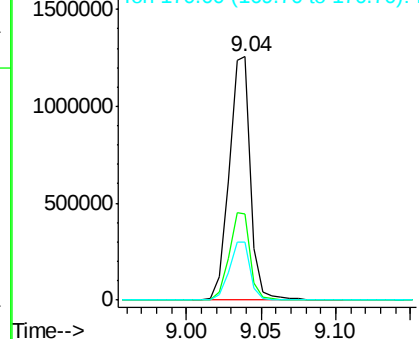


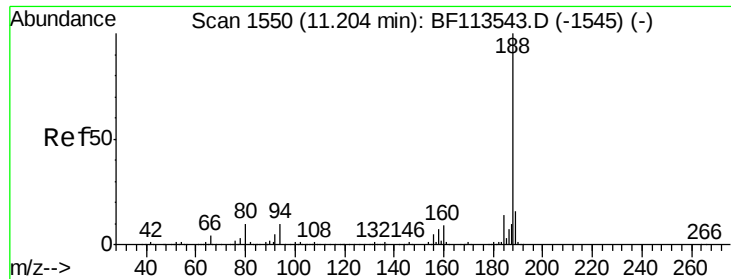

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.19 min Scan# 1547
Delta R.T. -0.02 min
Lab File: BF113589.D
Acq: 4 Apr 2019 18:10




Instrument :
BNA_F
ClientSampleId :
S2B(2-10)COMP


Tgt Ion:188 Resp: 441045
Ion Ratio Lower Upper
188 100
94 10.0 7.0 10.6
80 10.1 7.7 11.5

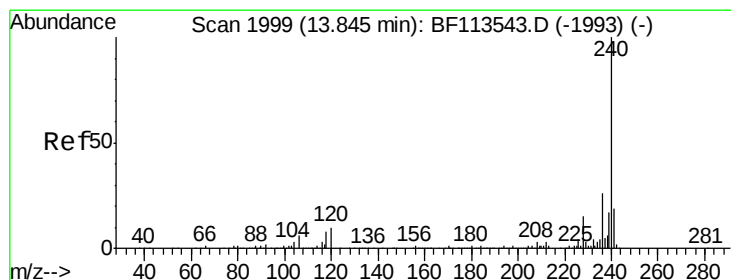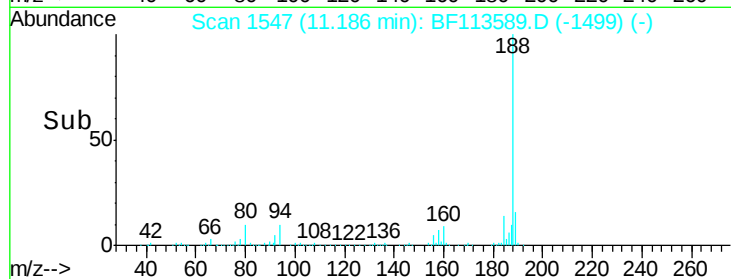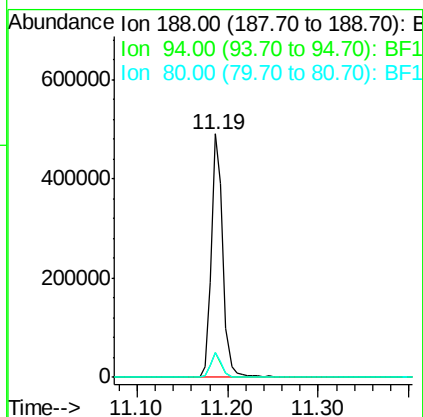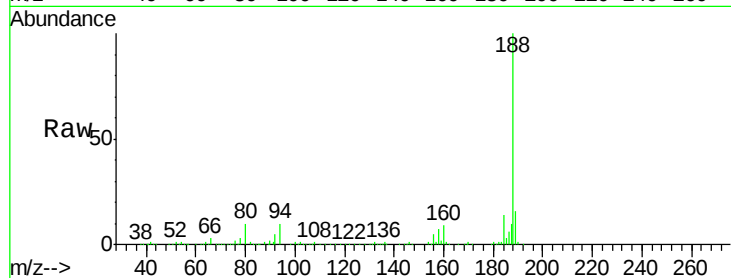

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.82 min Scan# 1994
Delta R.T. -0.03 min
Lab File: BF113589.D
Acq: 4 Apr 2019 18:10

Tgt Ion:240 Resp: 434763
Ion Ratio Lower Upper
240 100
120 11.0 8.8 13.2
236 25.6 20.9 31.3

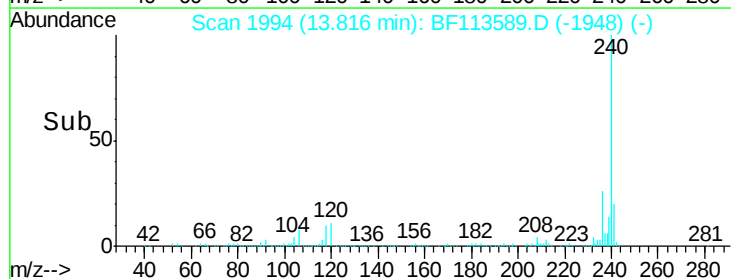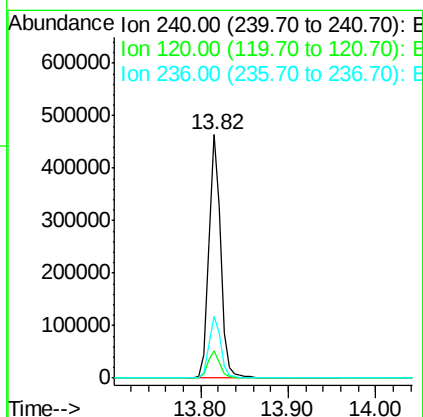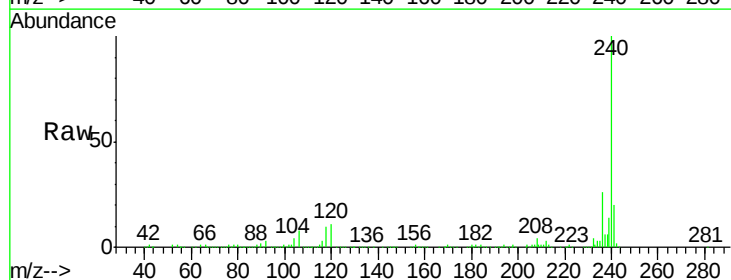

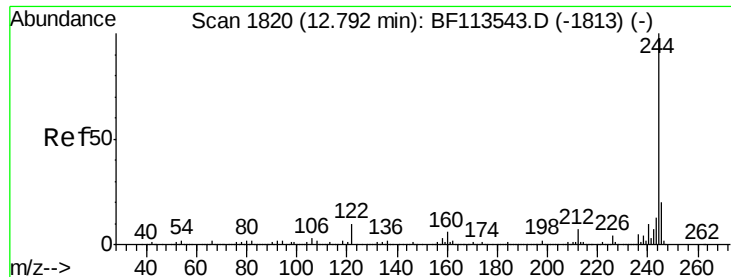

#79

Terphenyl-d14

Concen: 79.467 ng

RT: 12.77 min Scan# 1817

Delta R.T. -0.02 min

Lab File: BF113589.D

Acq: 4 Apr 2019 18:10

Instrument :

BNA_F

ClientSampleId :

S2B(2-10)COMP


Tgt Ion:244 Resp: 1696907

Ion Ratio Lower Upper

244 100

212 6.6 5.5 8.3




122 10.7 8.6 13.0

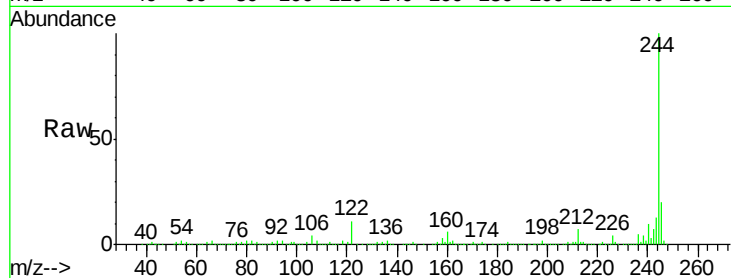

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

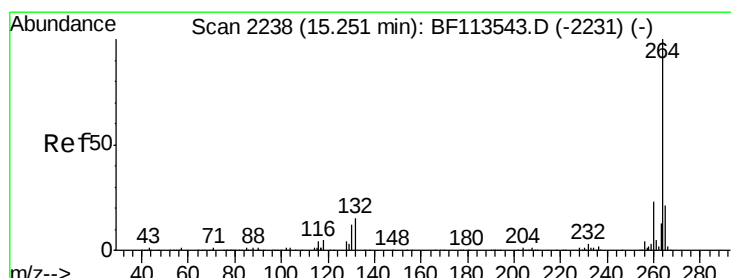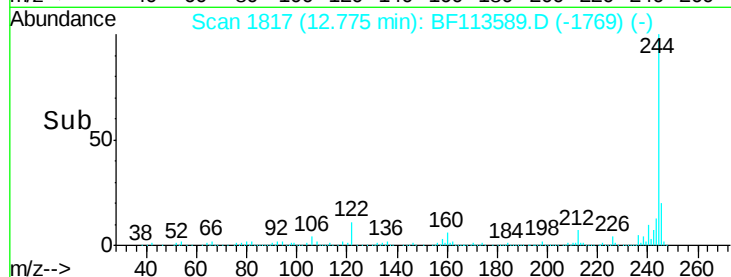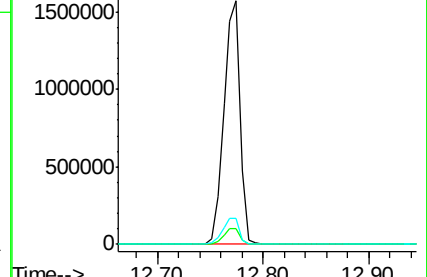

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.22 min Scan# 2232

Delta R.T. -0.04 min

Lab File: BF113589.D

Acq: 4 Apr 2019 18:10


Tgt Ion:264 Resp: 406259

Ion Ratio Lower Upper

264 100

260 23.9 19.1 28.7

265 21.8 17.1 25.7

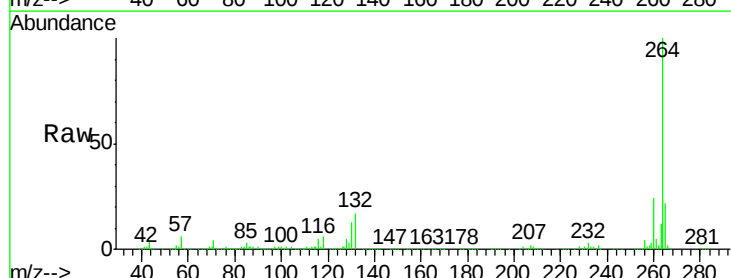

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

