

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040419\
 Data File : BF113596.D
 Acq On : 4 Apr 2019 21:34
 Operator : JU/SJ
 Sample : K2257-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-1-A

Quant Time: Apr 05 05:11:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	137365	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	520993	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	260939	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	555945	20.00	ng	-0.02
76) Chrysene-d12	13.82	240	482095	20.00	ng	-0.03
87) Perylene-d12	15.22	264	380834	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	759964	94.34	ng	0.00
7) Phenol-d6	6.33	99	1006103	101.34	ng	-0.01
23) Nitrobenzene-d5	7.25	82	600643	67.53	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	313350	99.97	ng	-0.02
45) 2-Fluorobiphenyl	9.03	172	1150958	71.01	ng	-0.02
79) Terphenyl-d14	12.77	244	1380103	58.29	ng	-0.02
Target Compounds						
50) Dimethylphthalate	9.43	163	145138	7.546	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040419\
Data File : BF113596.D
Acq On : 4 Apr 2019 21:34
Operator : JU/SJ
Sample : K2257-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-1-A

Quant Time: Apr 05 05:11:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

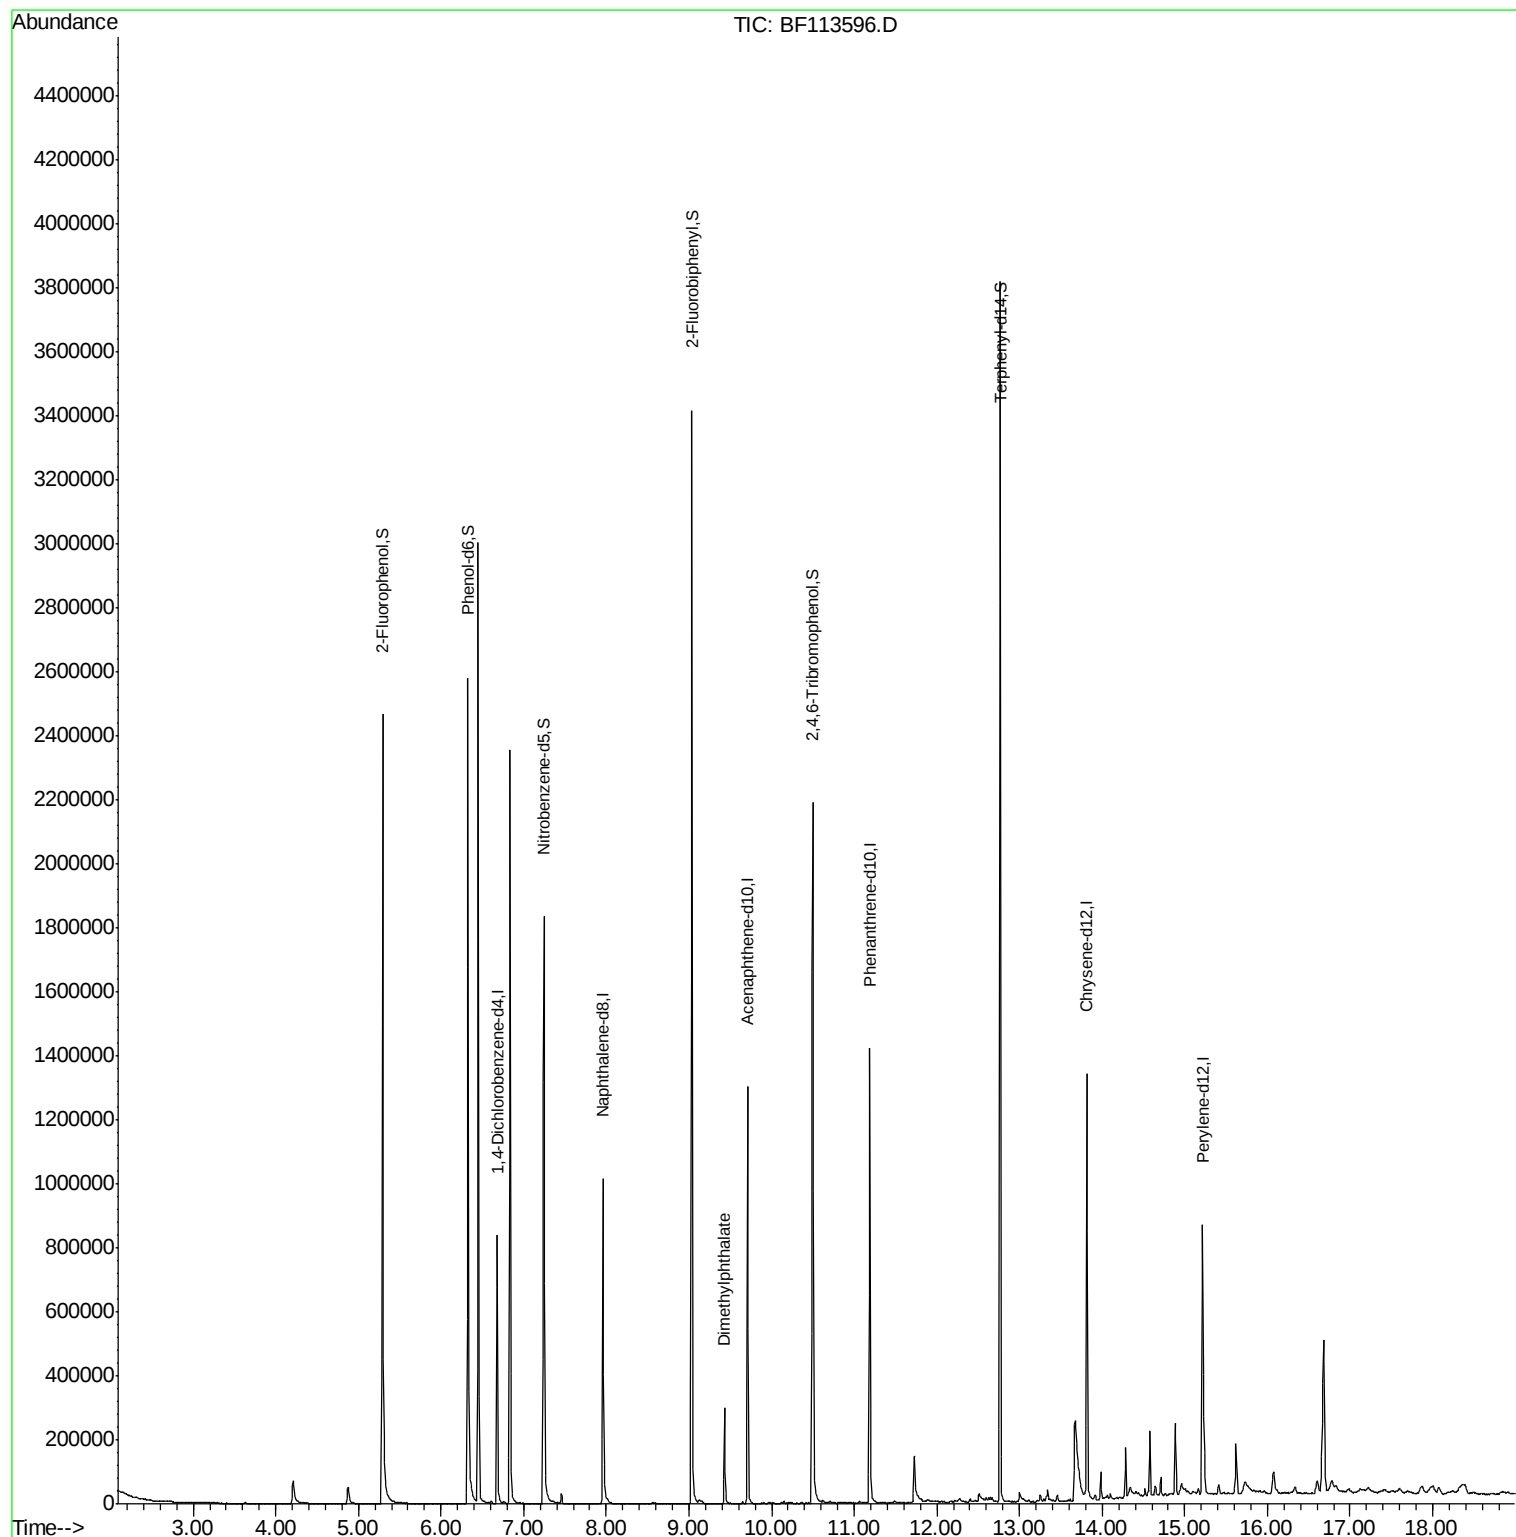

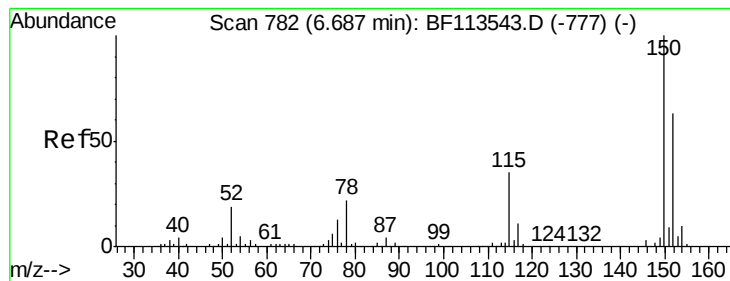


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.68 min Scan# 781
Delta R.T. -0.01 min
Lab File: BF113596.D
Acq: 4 Apr 2019 21:34

Instrument :
BNA_F
ClientSampled :
SP-1-A

Tgt Ion:152 Resp: 137365
Ion Ratio Lower Upper
152 100
150 151.9 124.7 187.1
115 53.8 46.0 69.0

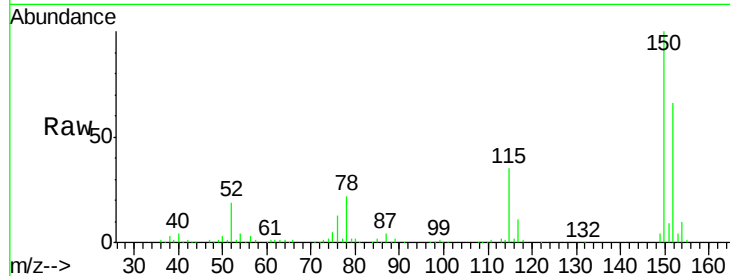


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

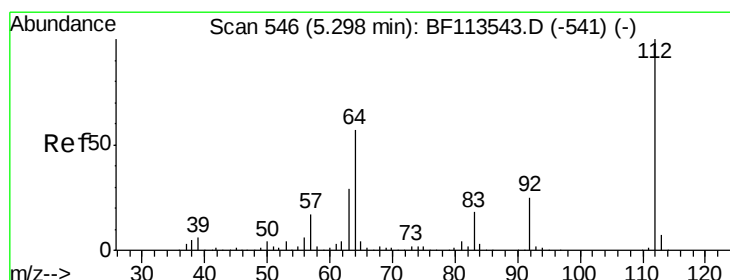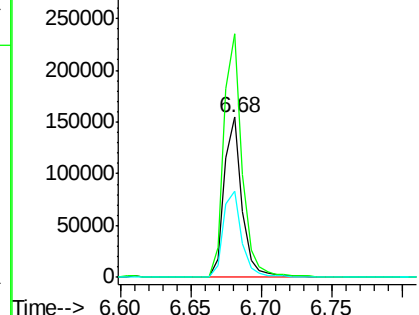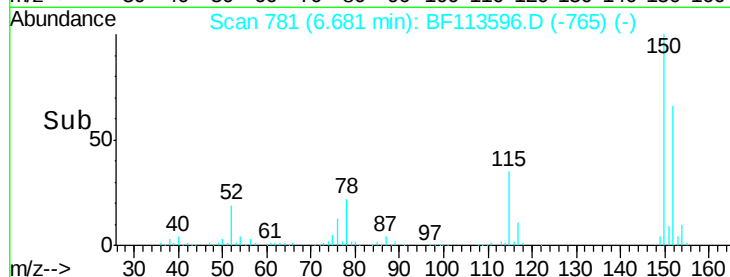



#5


2-Fluorophenol
Concen: 94.341 ng
RT: 5.29 min Scan# 545
Delta R.T. -0.01 min
Lab File: BF113596.D
Acq: 4 Apr 2019 21:34

Tgt Ion:112 Resp: 759964
Ion Ratio Lower Upper
112 100
64 60.1 49.2 73.8
63 30.3 24.9 37.3

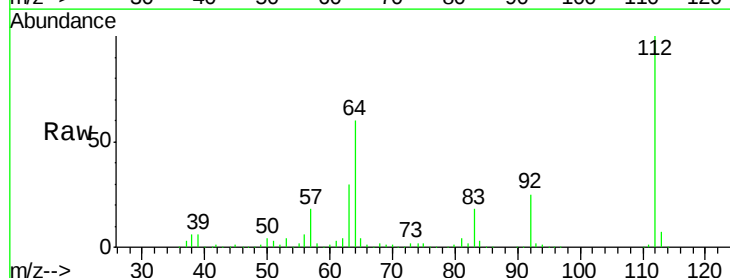

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

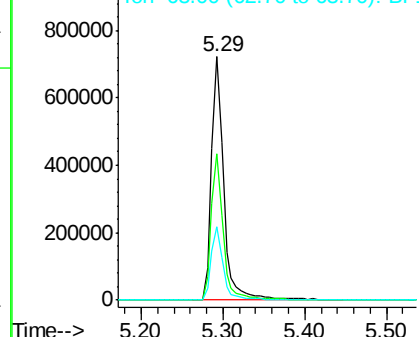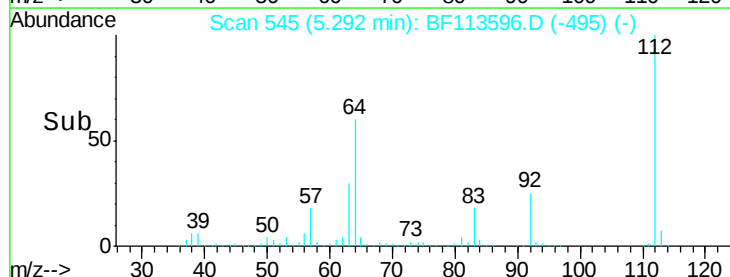

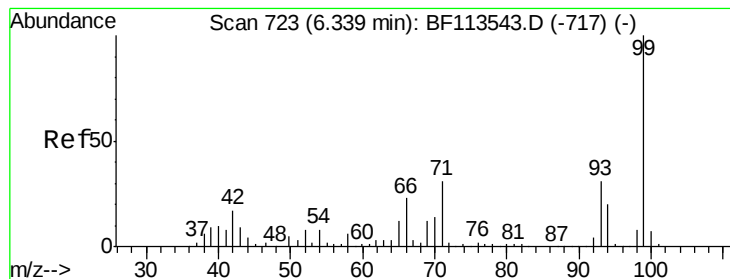

#7

Phenol-d6

Concen: 101.335 ng

RT: 6.33 min Scan# 721

Delta R.T. -0.01 min

Lab File: BF113596.D

Acq: 4 Apr 2019 21:34

Instrument :

BNA_F

ClientSampleId :

SP-1-A


Tgt Ion: 99 Resp: 1006103

Ion Ratio Lower Upper

99 100

42 18.2 14.8 22.2




71 31.3 24.9 37.3

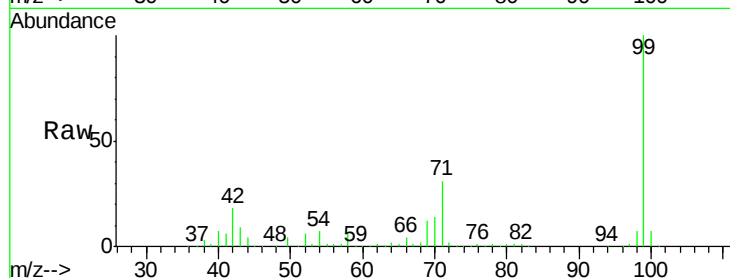

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

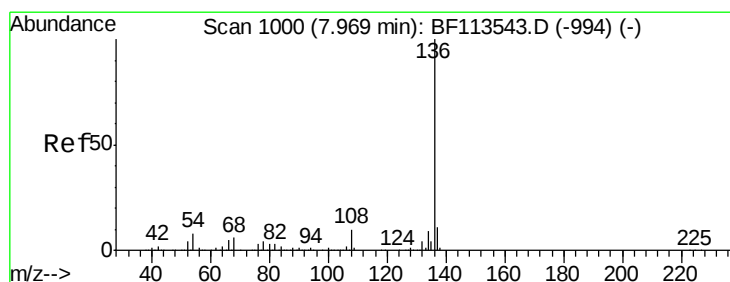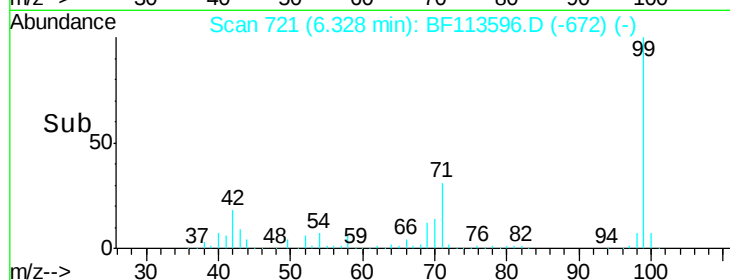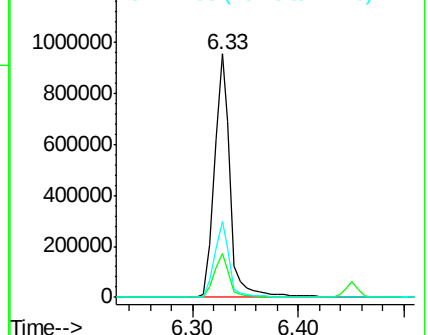

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 999

Delta R.T. -0.01 min

Lab File: BF113596.D

Acq: 4 Apr 2019 21:34

Tgt Ion: 136 Resp: 520993


Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 7.2 7.0 10.6

68 5.7 4.8 7.2


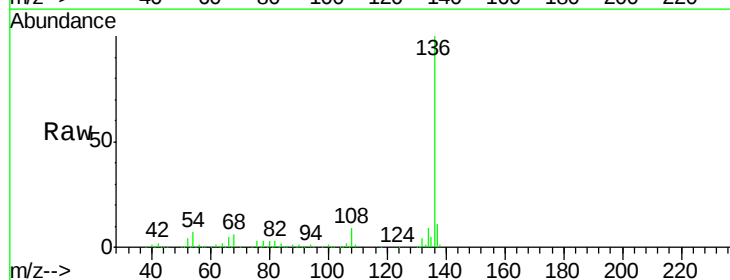


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

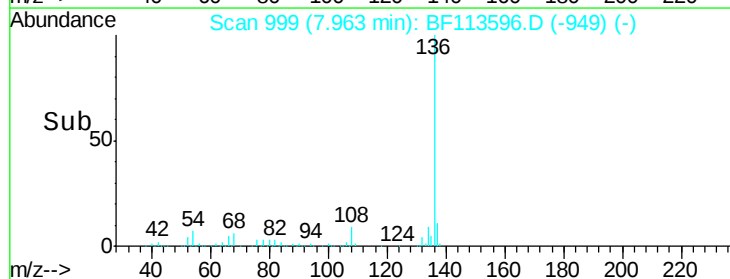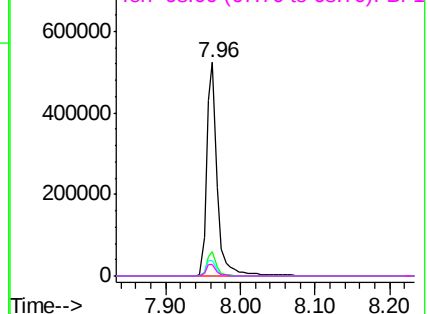







#23
 Nitrobenzene-d5
 Concen: 67.530 ng
 RT: 7.25 min Scan# 877
 Delta R.T. -0.01 min
 Lab File: BF113596.D
 Acq: 4 Apr 2019 21:34

Instrument :
 BNA_F
 ClientSampleId :
 SP-1-A

Tgt Ion: 82 Resp: 600643
 Ion Ratio Lower Upper
 82 100
 128 47.5 36.5 54.7
 54 51.1 42.2 63.2

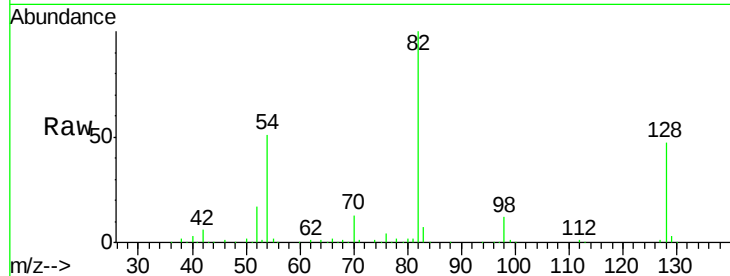


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF1

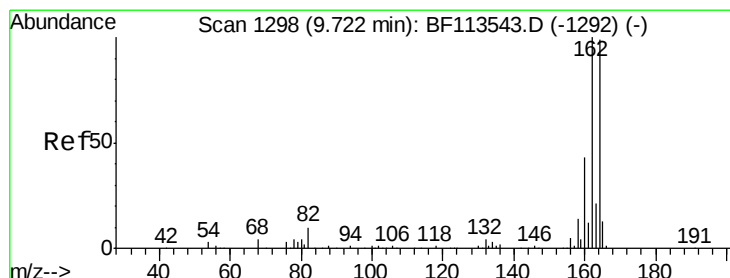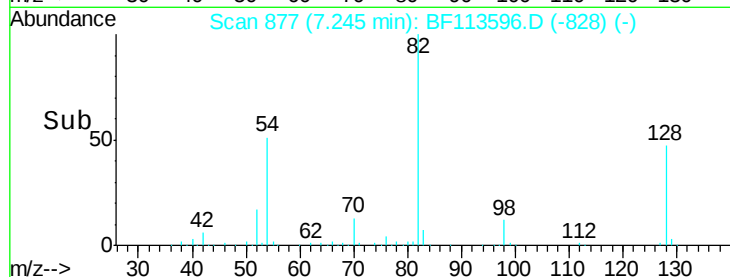
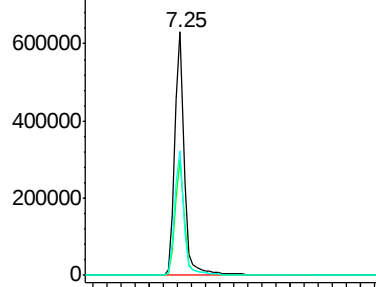


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.71 min Scan# 1296
 Delta R.T. -0.01 min
 Lab File: BF113596.D
 Acq: 4 Apr 2019 21:34

Tgt Ion: 164 Resp: 260939
 Ion Ratio Lower Upper
 164 100
 162 99.0 81.8 122.6
 160 44.2 36.4 54.6

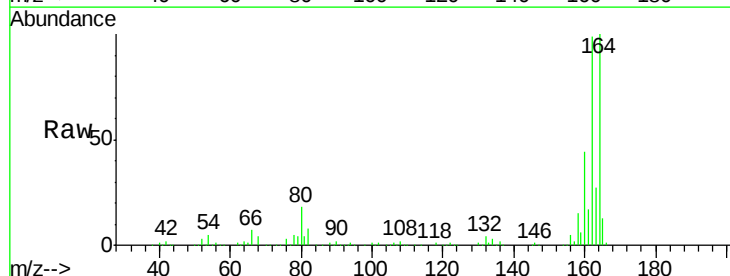

Abundance Ion 164.00 (163.70 to 164.70): B
 Ion 162.00 (161.70 to 162.70): B
 Ion 160.00 (159.70 to 160.70): B

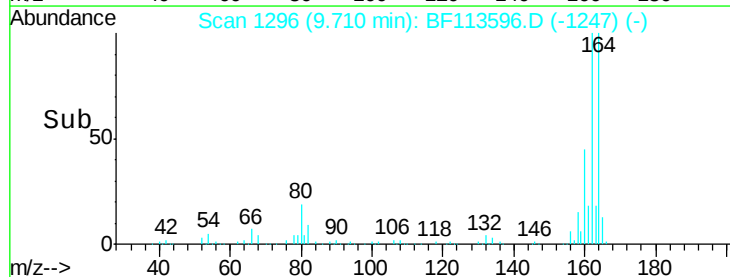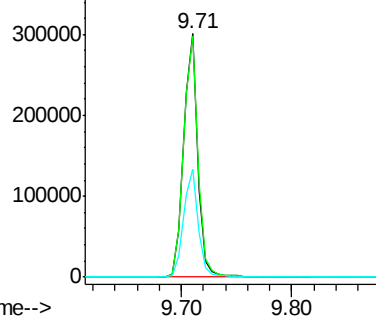







#42
 2,4,6-Tribromophenol
 Concen: 99.968 ng
 RT: 10.50 min Scan# 1430
 Delta R.T. -0.02 min
 Lab File: BF113596.D
 Acq: 4 Apr 2019 21:34

Instrument :
 BNA_F
 ClientSampleId :
 SP-1-A

Tgt Ion:330 Resp: 313350
 Ion Ratio Lower Upper
 330 100
 332 96.8 77.8 116.6
 141 27.5 22.7 34.1

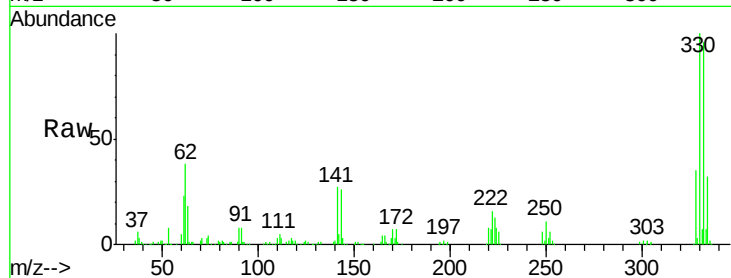


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

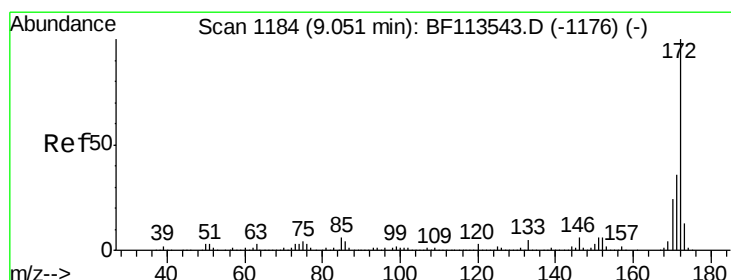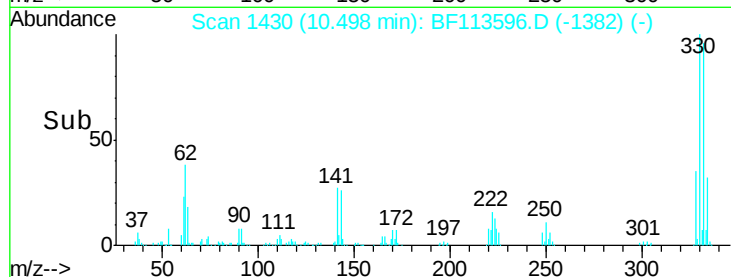
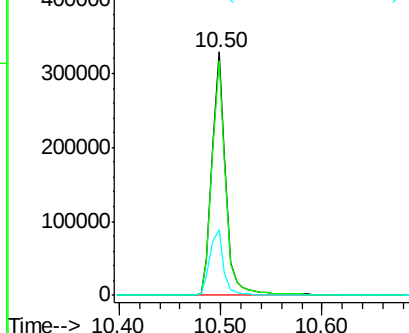


#45
 2-Fluorobiphenyl
 Concen: 71.010 ng
 RT: 9.03 min Scan# 1181
 Delta R.T. -0.02 min
 Lab File: BF113596.D
 Acq: 4 Apr 2019 21:34

Tgt Ion:172 Resp: 1150958
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.0 43.6
 170 24.3 19.5 29.3

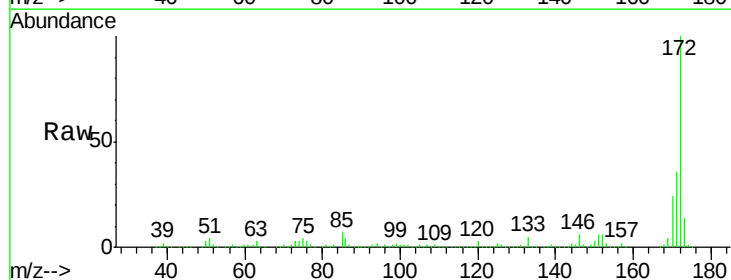

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

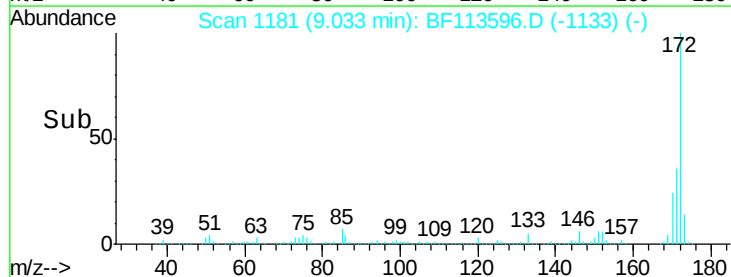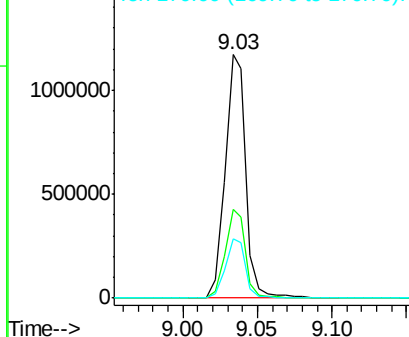







#50
Dimethylphthalate
Concen: 7.546 ng
RT: 9.43 min Scan# 1249
Delta R.T. -0.02 min
Lab File: BF113596.D
Acq: 4 Apr 2019 21:34

Instrument :
BNA_F
ClientSampleId :
SP-1-A

Tgt Ion:163 Resp: 145138
Ion Ratio Lower Upper
163 100
194 3.8 3.0 4.6
164 9.8 8.1 12.1

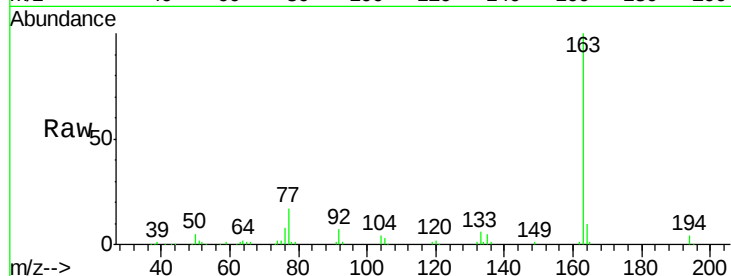


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

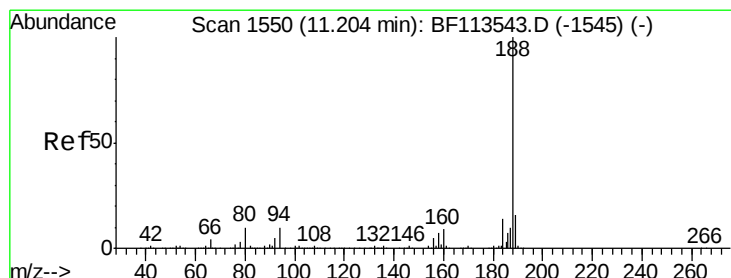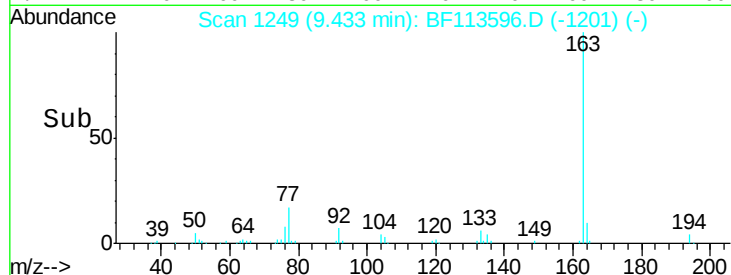
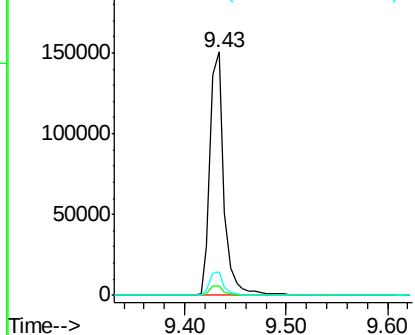



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.19 min Scan# 1547
Delta R.T. -0.02 min
Lab File: BF113596.D
Acq: 4 Apr 2019 21:34

Tgt Ion:188 Resp: 555945
Ion Ratio Lower Upper
188 100
94 9.6 7.0 10.6
80 10.0 7.7 11.5

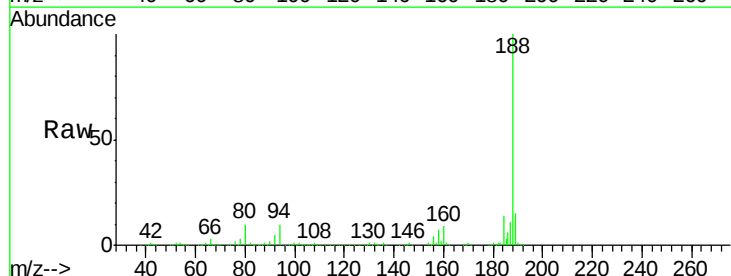

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

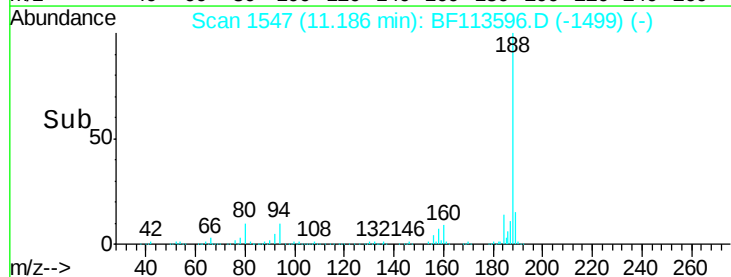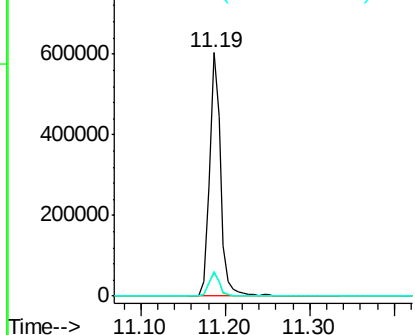

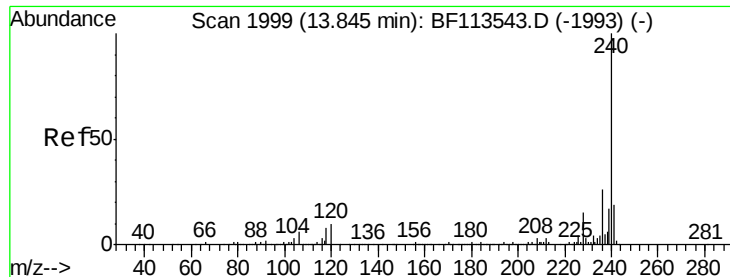

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.82 min Scan# 1994

Delta R.T. -0.03 min

Lab File: BF113596.D

Acq: 4 Apr 2019 21:34

Instrument :

BNA_F

ClientSampleId :

SP-1-A


Tgt Ion:240 Resp: 482095

Ion Ratio Lower Upper

240 100

120 10.6 8.8 13.2




236 26.1 20.9 31.3

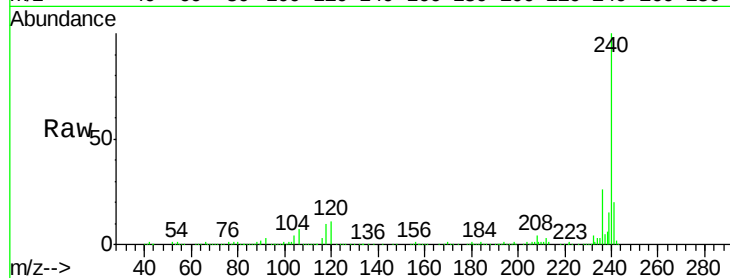

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

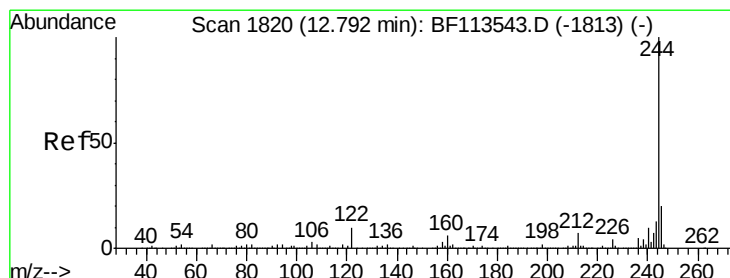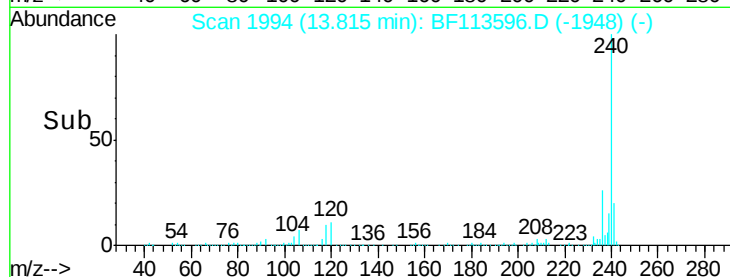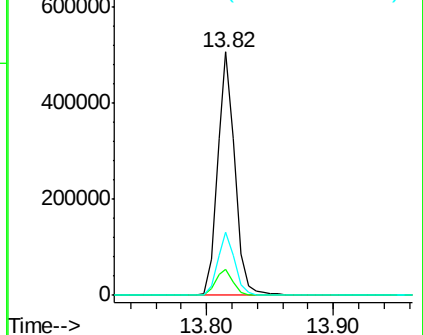

#79

Terphenyl-d14

Concen: 58.285 ng

RT: 12.77 min Scan# 1816

Delta R.T. -0.02 min

Lab File: BF113596.D

Acq: 4 Apr 2019 21:34


Tgt Ion:244 Resp: 1380103

Ion Ratio Lower Upper

244 100

212 6.6 5.5 8.3



122 10.9 8.6 13.0

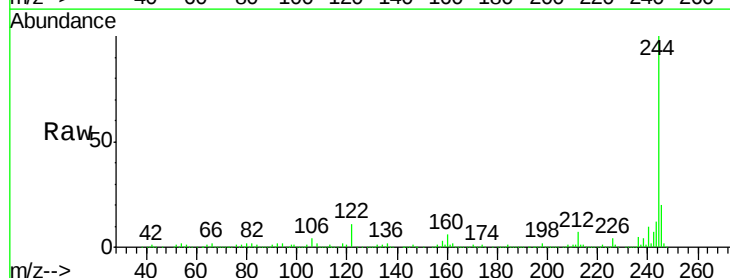


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

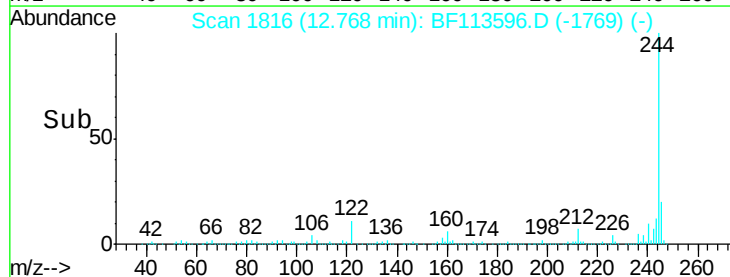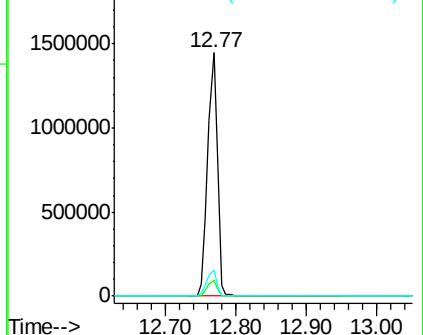


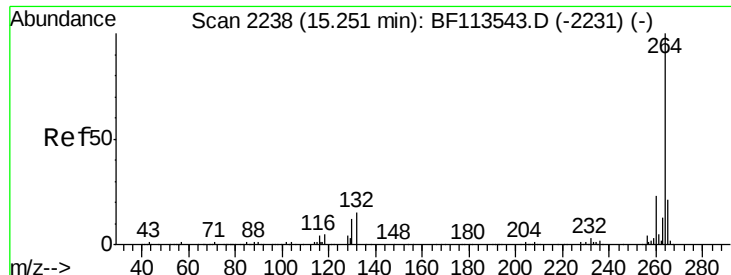

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.22 min Scan# 2232
Delta R.T. -0.04 min
Lab File: BF113596.D
Acq: 4 Apr 2019 21:34

Instrument :
BNA_F
ClientSampleId :
SP-1-A

Tgt Ion: 264 Resp: 380834
Ion Ratio Lower Upper
264 100
260 24.0 19.1 28.7
265 21.8 17.1 25.7

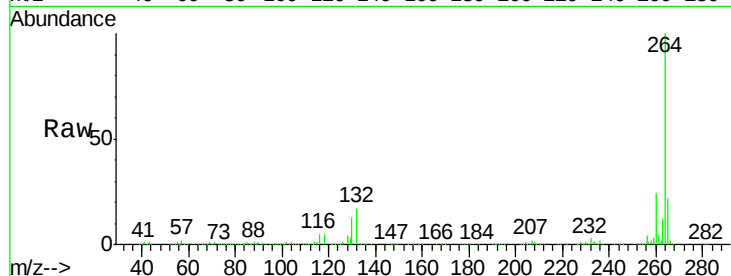

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

