


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040419\
 Data File : BF113580.D
 Acq On : 4 Apr 2019 13:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

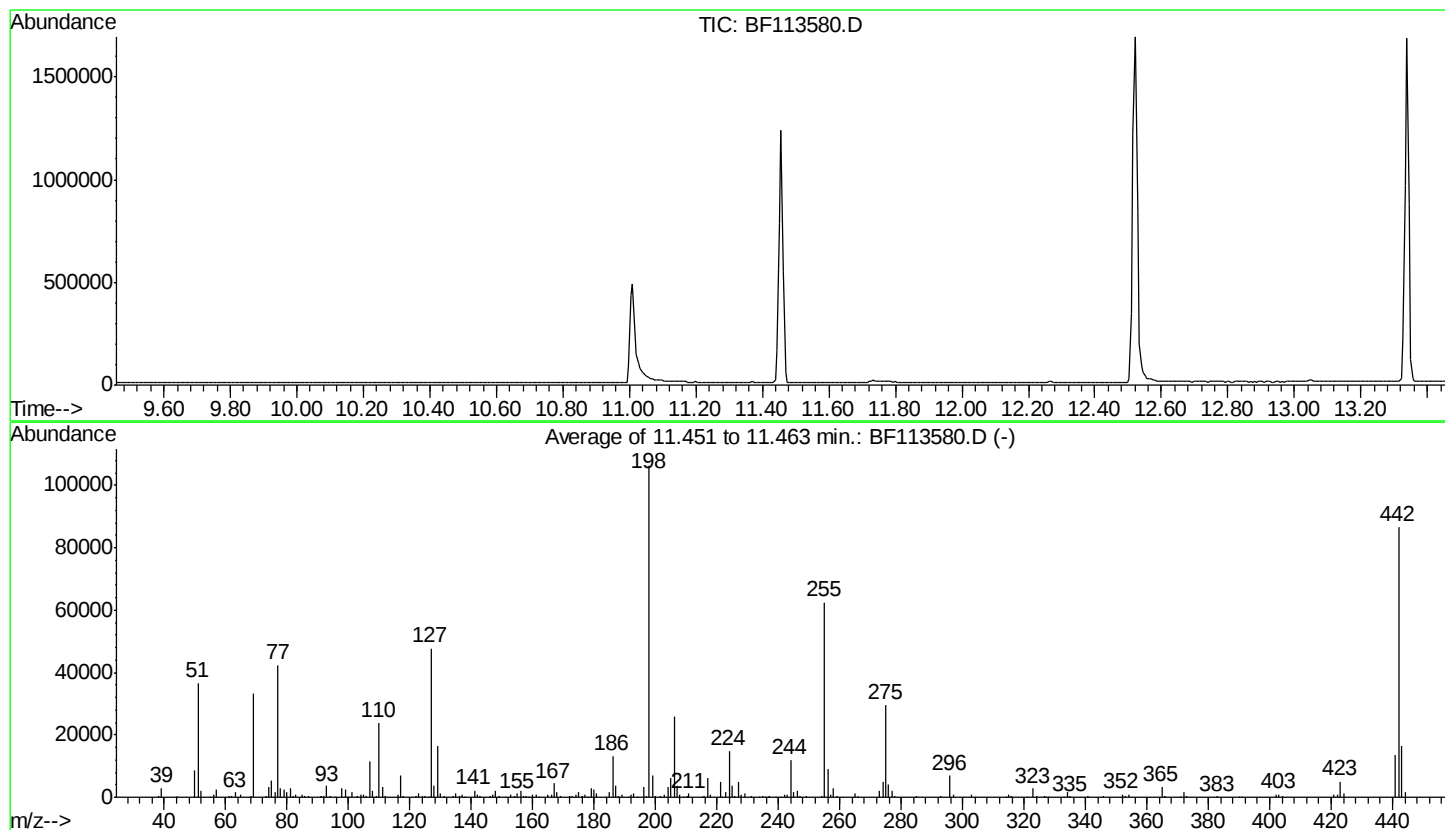

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	36668	PASS
68	69	0.00	2	1.2	384	PASS
69	198	0.00	100	31.3	33286	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	47701	PASS
197	198	0.00	2	0.6	593	PASS
198	198	100	100	100.0	106274	PASS
199	198	5	9	6.7	7076	PASS
275	198	10	60	27.9	29666	PASS
365	198	1	100	3.2	3373	PASS
441	198	0.01	100	12.8	13599	PASS
442	198	50	100	81.6	86701	PASS
443	442	15	24	18.9	16353	PASS