
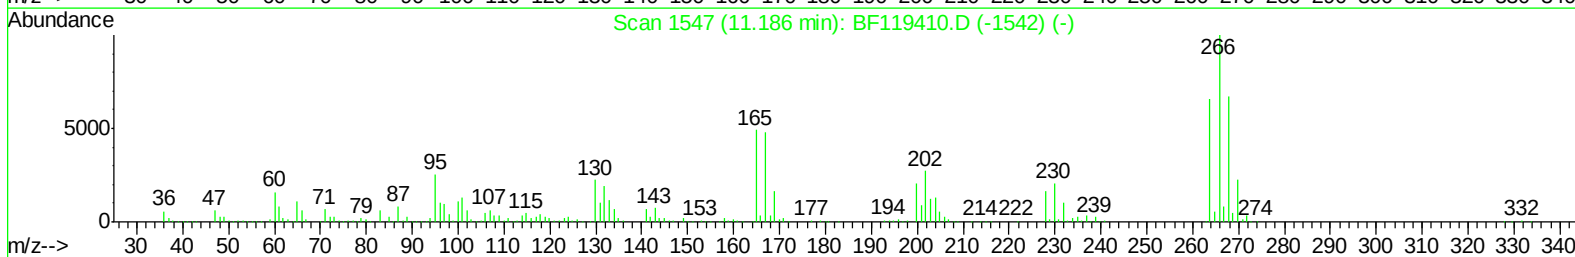
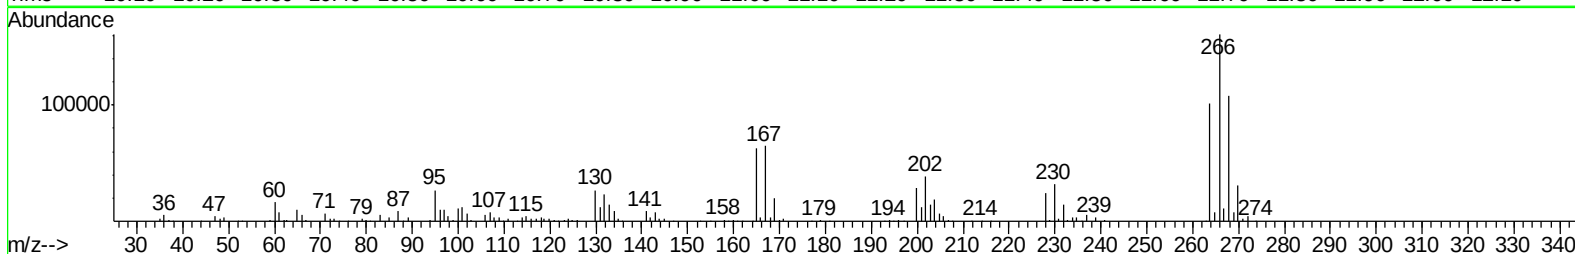


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040620\
Data File : BF119800.D
Acq On : 7 Apr 2020 4:54
Operator : MA/SJ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 05:28:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 06 11:15:16 2020
Response via : Initial Calibration

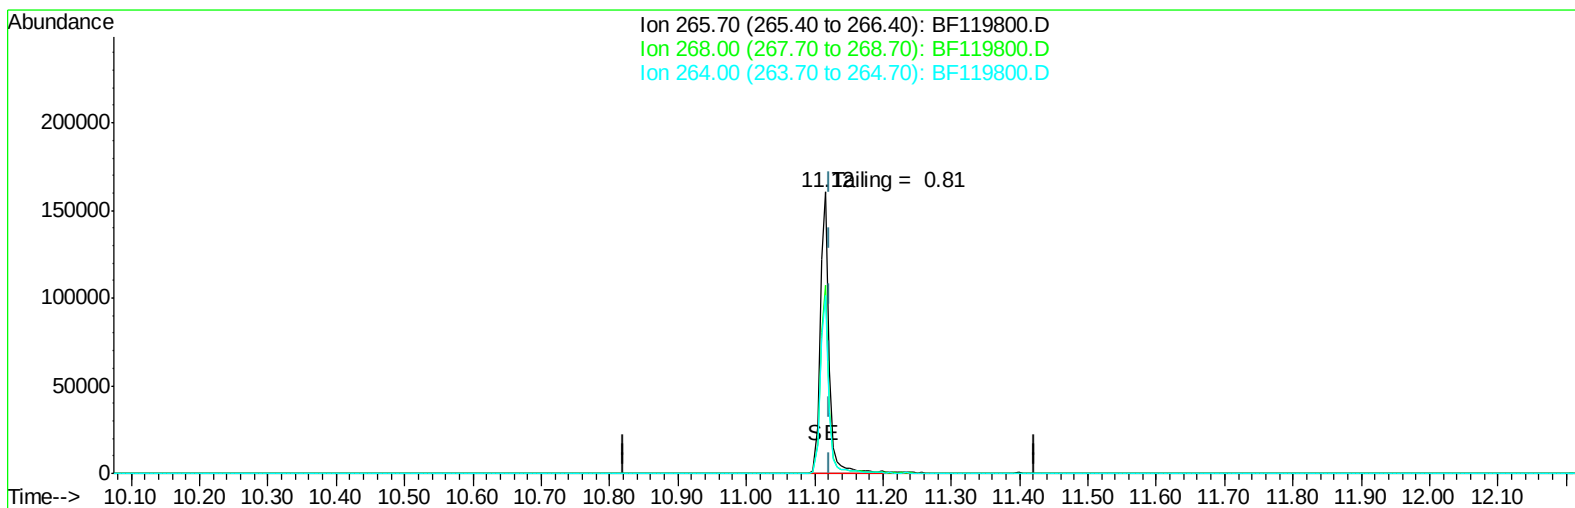

TIC: BF119800.D

(70) Pentachlorophenol (C)




11.116min (-0.006) 73394.91ng

response 145973

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.95
264.00	61.20	63.07
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040620\
 Data File : BF119800.D
 Acq On : 7 Apr 2020 4:54
 Operator : MA/SJ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 05:28:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 06 11:15:16 2020
 Response via : Initial Calibration

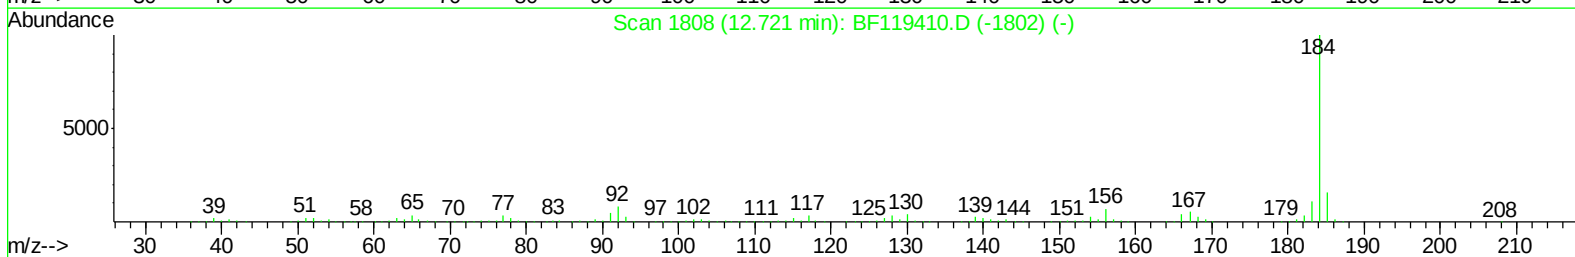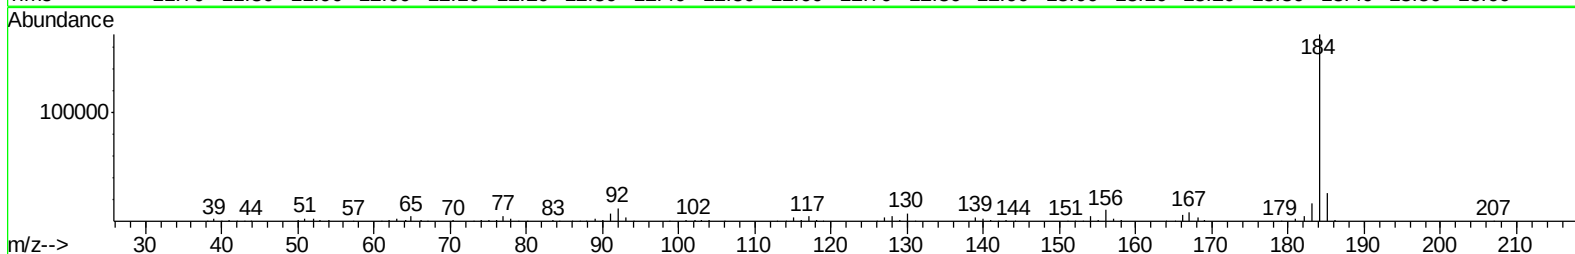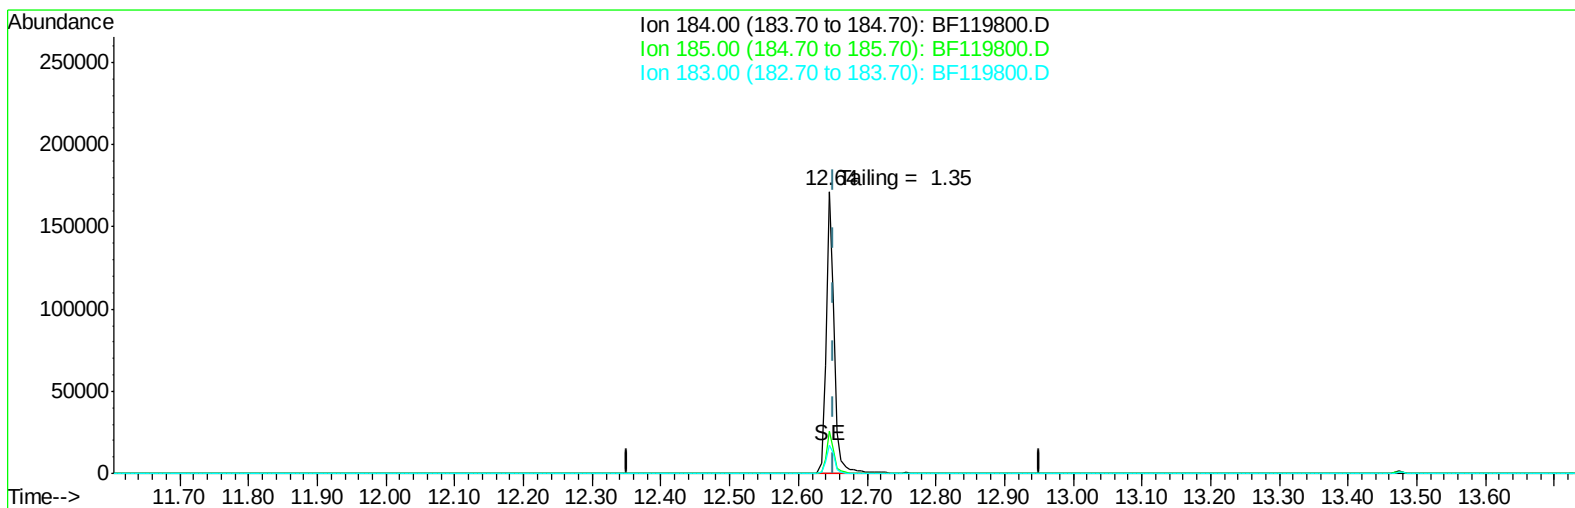

TIC: BF119800.D

(77) Benzidine

12.645min (-0.006) 0.00ng

response 140233

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.91
183.00	11.30	9.91
0.00	0.00	0.00