

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040620\
 Data File : BF119763.D
 Acq On : 6 Apr 2020 11:25
 Operator : MA/SJ
 Sample : PB128003BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128003BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	493	498	505	rBV	55167	78687	1.18%	0.177%
2	5.404	558	564	567	rBV	5648692	5698394	85.32%	12.836%
3	6.416	730	736	739	rBV	4906353	5559430	83.24%	12.523%
4	6.781	794	798	802	rBV	1154303	930054	13.93%	2.095%
5	6.939	820	825	828	rBV	4801751	4356398	65.23%	9.813%
6	7.345	888	894	897	rBV	3188447	3618921	54.19%	8.152%
7	8.069	1012	1017	1020	rBV	1282111	1221520	18.29%	2.752%
8	9.151	1194	1201	1204	rBV	6018828	6325430	94.71%	14.249%
9	9.827	1310	1316	1319	rBV	1351788	1316310	19.71%	2.965%
10	10.616	1443	1450	1453	rBV	4428631	4484458	67.14%	10.102%
11	11.310	1563	1568	1572	rBV	1791949	1525626	22.84%	3.437%
12	12.910	1832	1840	1843	rBV	6473429	6678783	100.00%	15.045%
13	13.951	2013	2017	2021	rBV	1443981	1283675	19.22%	2.892%
14	15.398	2257	2263	2267	rBV	1066560	1315419	19.70%	2.963%


Sum of corrected areas: 44393105

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040620\
Data File : BF119763.D
Acq On : 6 Apr 2020 11:25
Operator : MA/SJ
Sample : PB128003BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128003BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

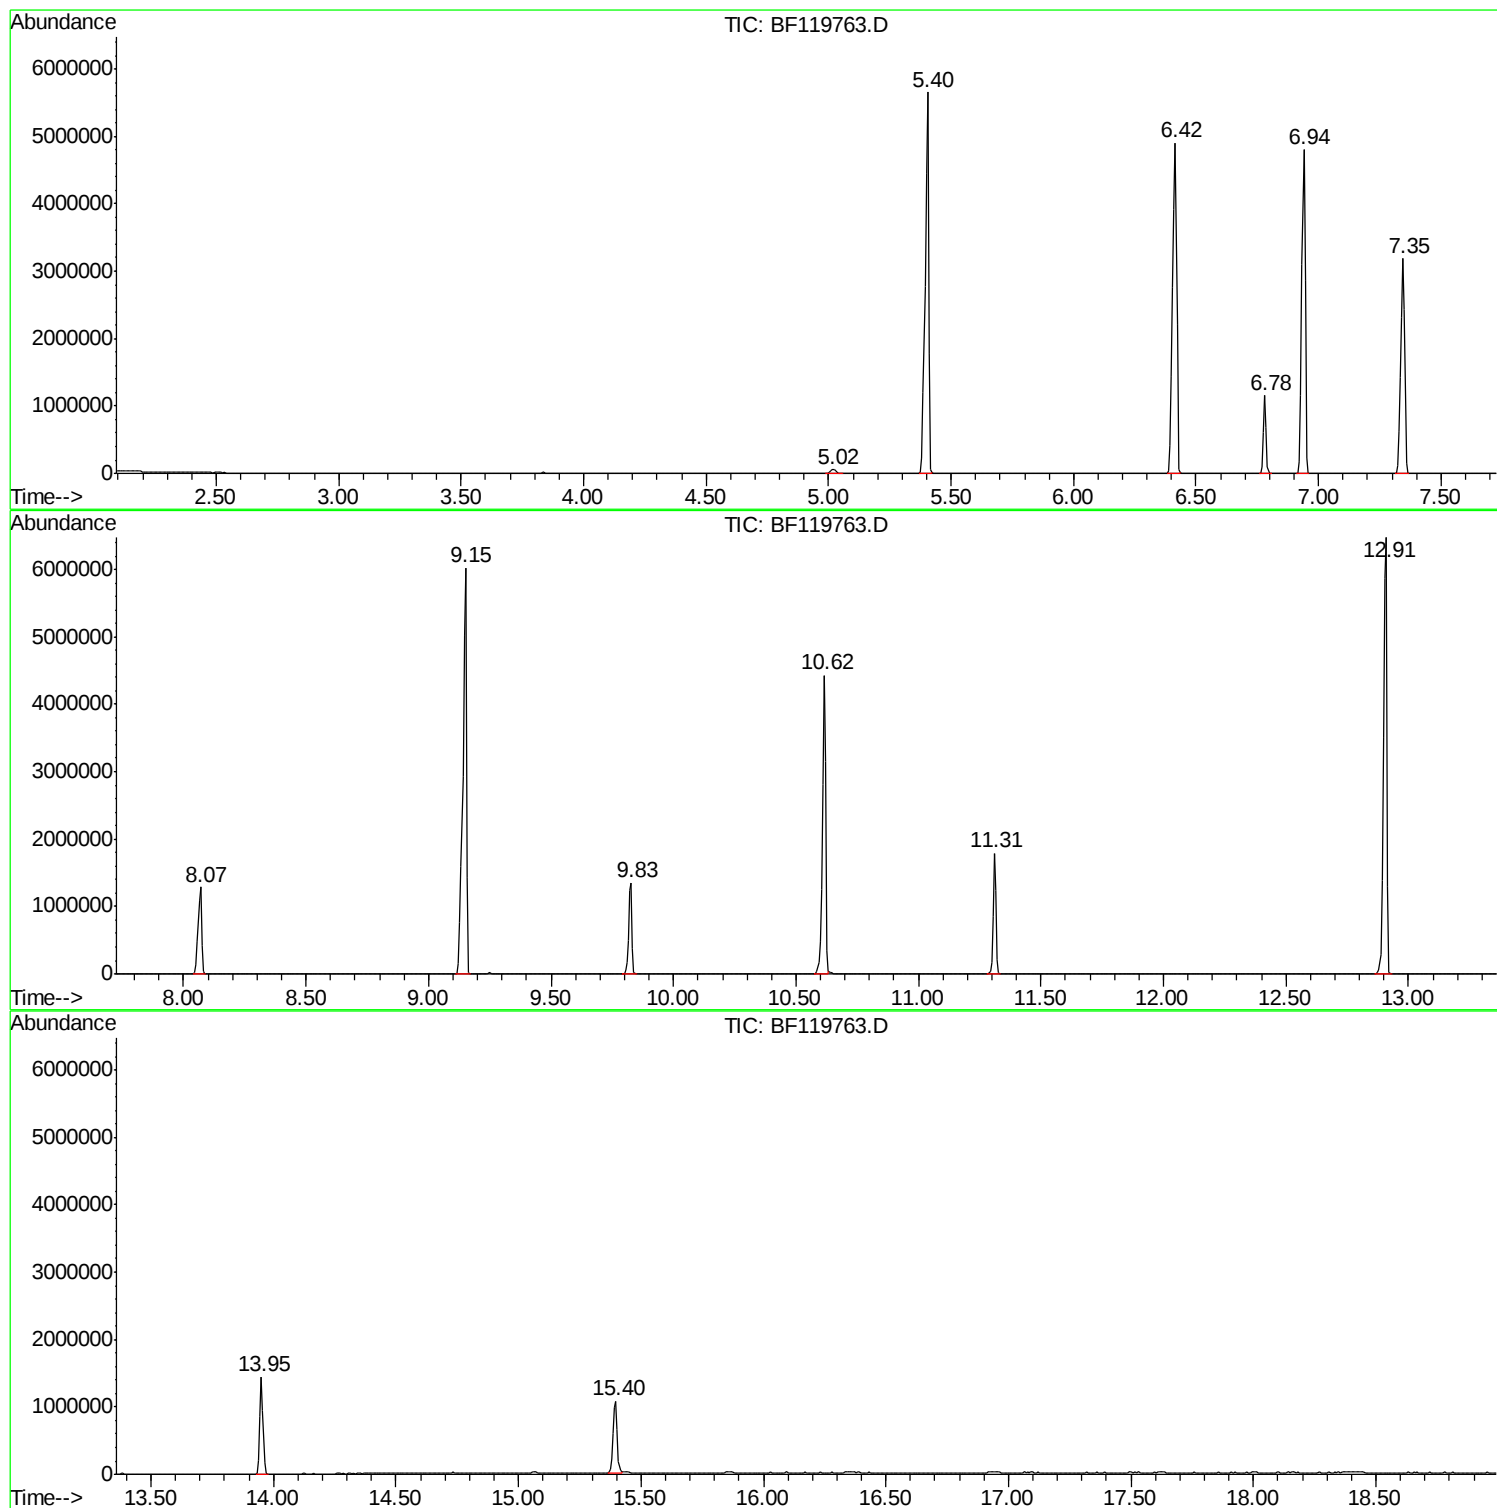

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040620\
Data_File : BF119763.D
Acq_On : 6 Apr 2020 11:255
Operator : MA/SJJ
Sample : PB128003BLL
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB128003BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
