

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040620\
 Data File : BF119764.D
 Acq On : 6 Apr 2020 11:52
 Operator : MA/SJ
 Sample : PB128016BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128016BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.004	493	496	503	rBV	50847	68090	1.11%	0.163%
2	5.398	558	563	566	rBV	4802942	5201774	84.47%	12.424%
3	6.416	730	736	738	rBV	4306373	5071499	82.35%	12.113%
4	6.781	794	798	801	rBV	1248669	986249	16.01%	2.356%
5	6.939	820	825	828	rBV	4657524	4120557	66.91%	9.842%
6	7.345	888	894	897	rBV	3222171	3325266	54.00%	7.942%
7	8.063	1011	1016	1020	rBV	1303695	1292179	20.98%	3.086%
8	9.145	1194	1200	1203	rBV	5810800	6002263	97.46%	14.336%
9	9.822	1310	1315	1319	rBV	1592285	1452575	23.59%	3.469%
10	10.616	1443	1450	1453	rBV	4038084	3823642	62.09%	9.133%
11	11.310	1562	1568	1571	rBV	1886047	1537814	24.97%	3.673%
12	12.904	1834	1839	1842	rBV	6300444	6158389	100.00%	14.709%
13	13.951	2013	2017	2021	rBV	1574623	1398919	22.72%	3.341%
14	15.392	2257	2262	2267	rBV	1166248	1427874	23.19%	3.410%


Sum of corrected areas: 41867090

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040620\
Data File : BF119764.D
Acq On : 6 Apr 2020 11:52
Operator : MA/SJ
Sample : PB128016BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128016BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

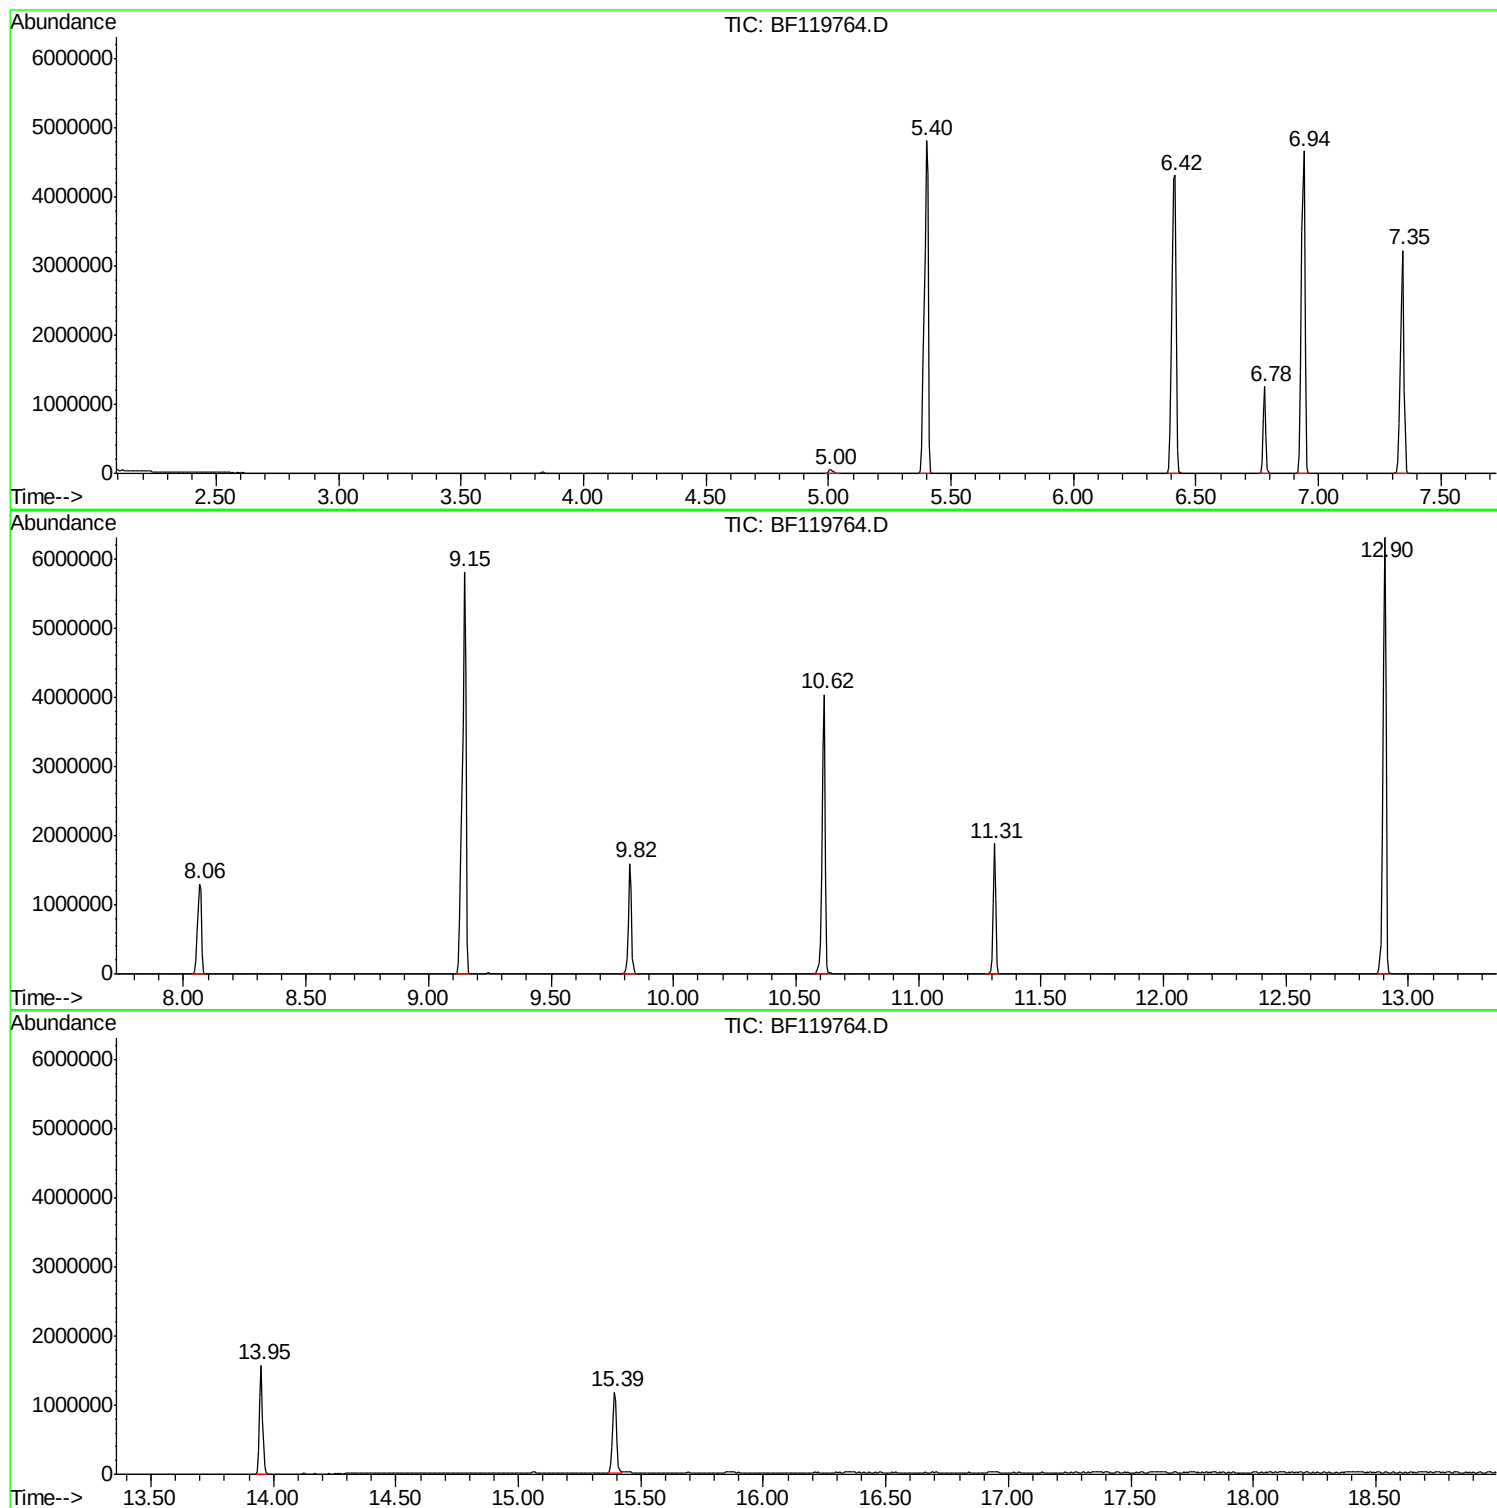

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040620\
Data_File : BF119764.D
Acq_On : 6 Apr 2020 11:522
Operator : MA/SJJ
Sample : PB128016BLL
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB128016BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
