


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040620\
 Data File : BF119760.D
 Acq On : 6 Apr 2020 9:56
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 06 11:15:16 2020

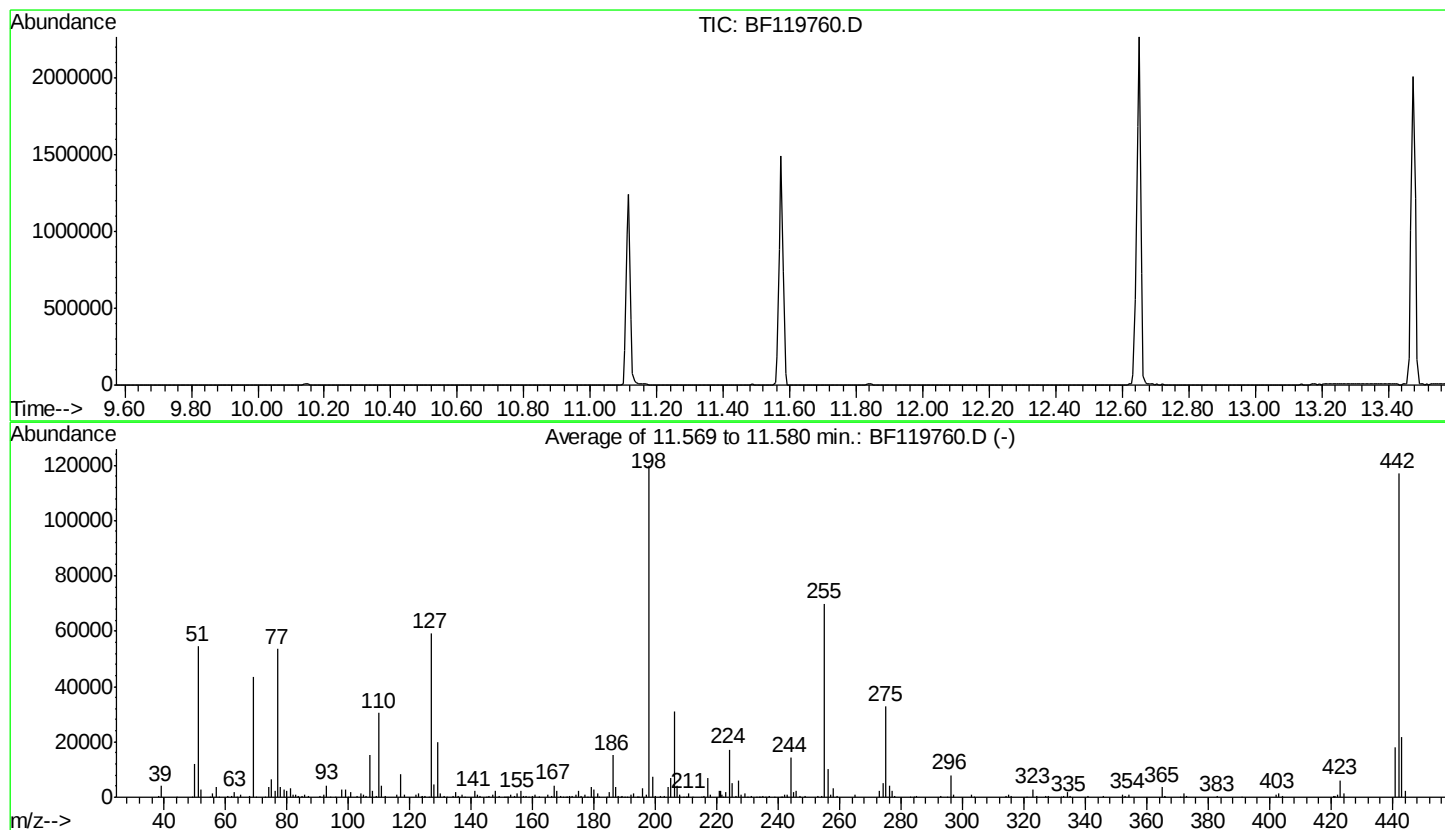

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	54463	PASS
68	69	0.00	2	1.4	618	PASS
69	198	0.00	100	36.4	43669	PASS
70	69	0.00	2	0.2	109	PASS
127	198	10	80	49.3	59104	PASS
197	198	0.00	2	0.6	758	PASS
198	198	100	100	100.0	119824	PASS
199	198	5	9	6.2	7486	PASS
275	198	10	60	27.4	32829	PASS
365	198	1	100	3.1	3689	PASS
441	198	0.01	100	15.1	18126	PASS
442	198	50	100	97.8	117168	PASS
443	442	15	24	18.7	21906	PASS