


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040620\
 Data File : BF119779.D
 Acq On : 6 Apr 2020 19:27
 Operator : MA/SJ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 06 11:15:16 2020

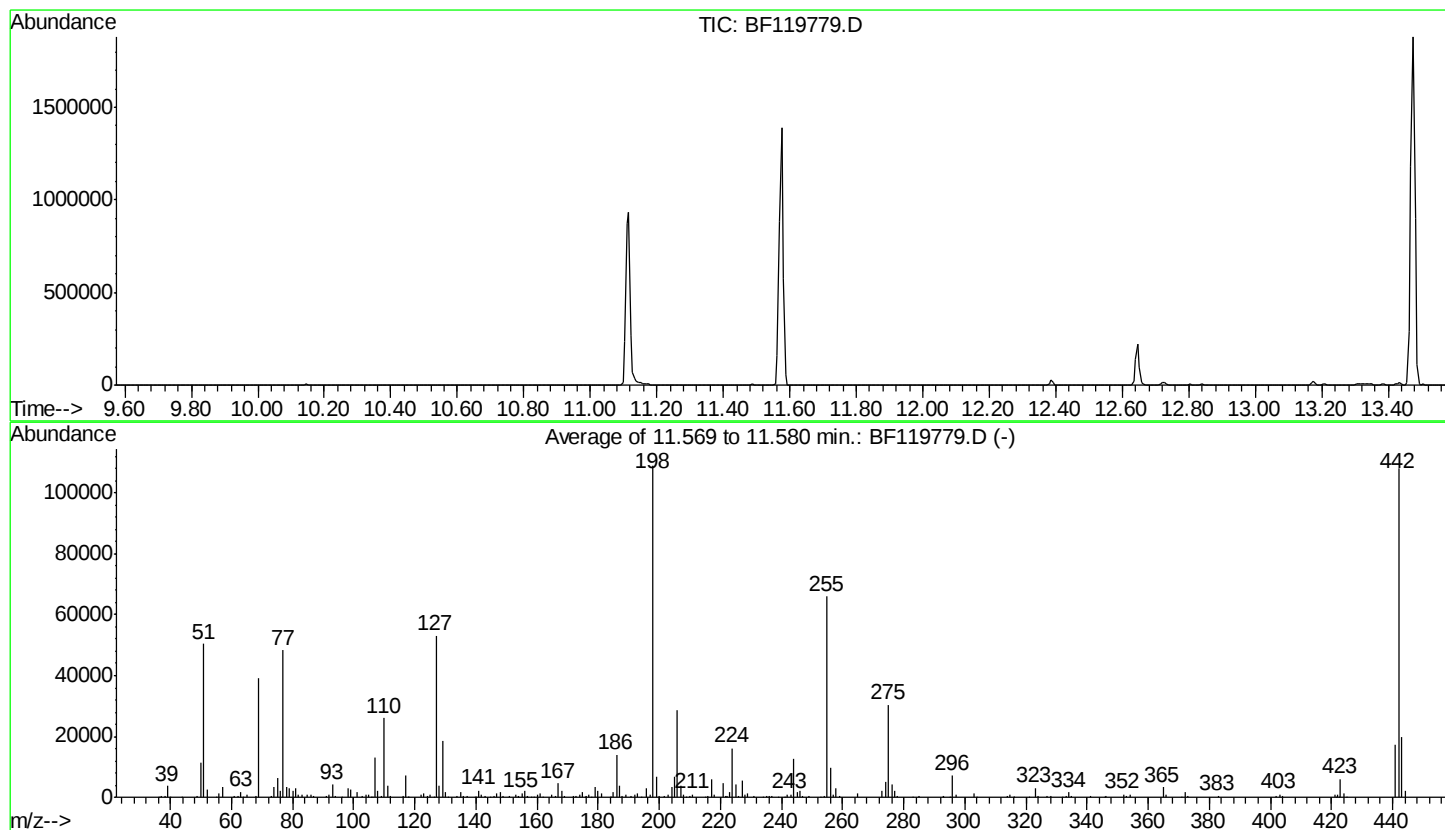

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	50485	PASS
68	69	0.00	2	1.2	468	PASS
69	198	0.00	100	36.0	39265	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	53149	PASS
197	198	0.00	2	0.8	853	PASS
198	198	100	100	100.0	109042	PASS
199	198	5	9	6.3	6903	PASS
275	198	10	60	27.9	30400	PASS
365	198	1	100	3.0	3315	PASS
441	198	0.01	100	15.8	17249	PASS
442	198	50	100	99.2	108168	PASS
443	442	15	24	18.2	19645	PASS