
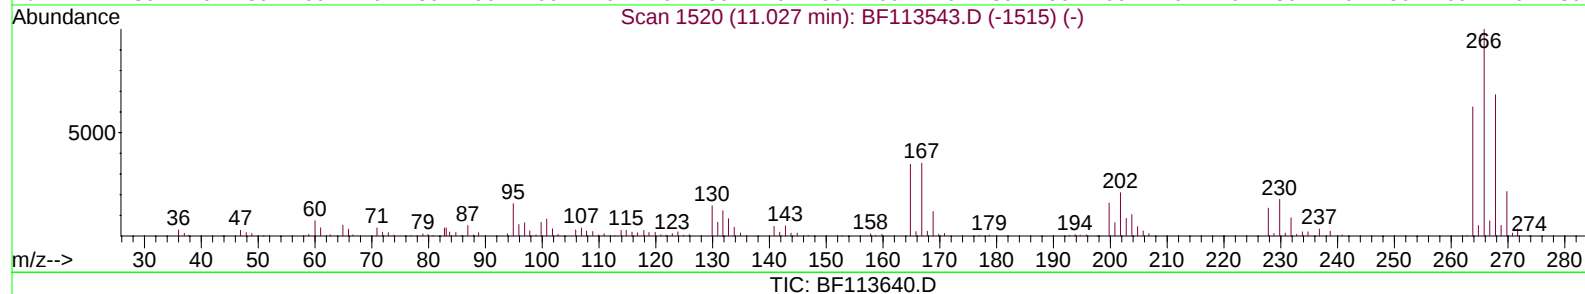
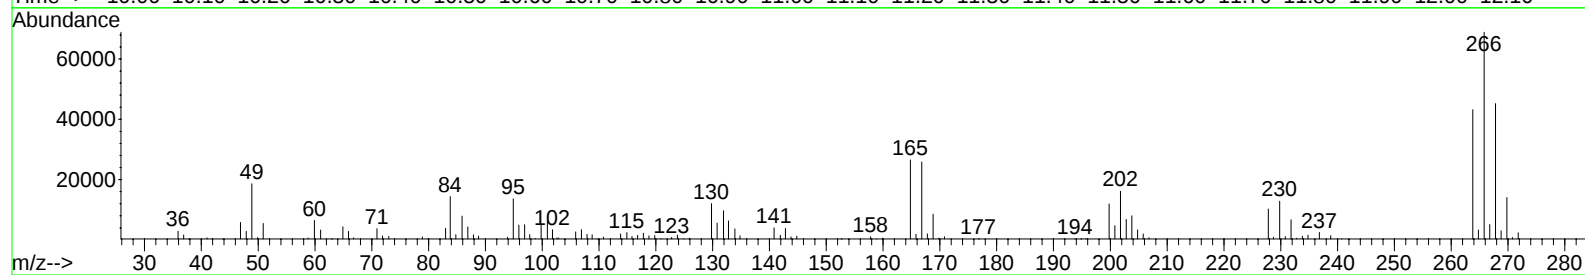


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040819\
Data File : BF113640.D
Acq On : 8 Apr 2019 15:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 19:18:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

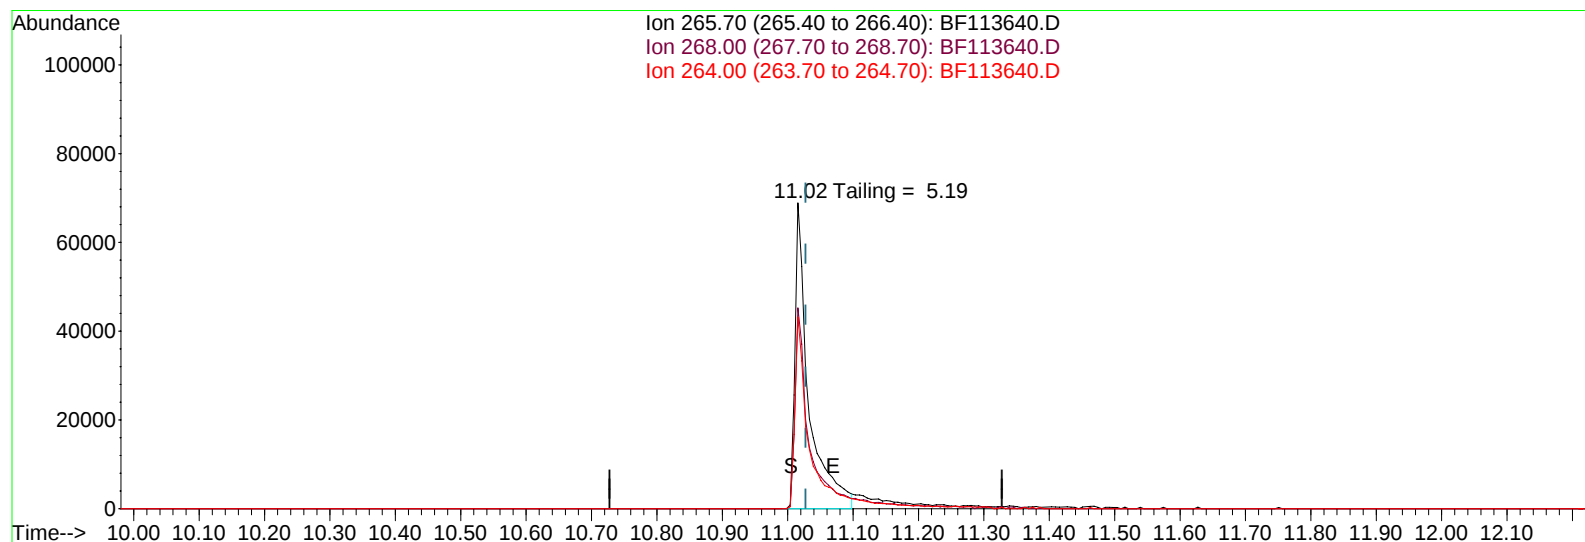

(70) Pentachlorophenol (C)




11.016min (-0.012) 40689.37ng

response 114080

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	65.66
264.00	61.50	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040819\
Data File : BF113640.D
Acq On : 8 Apr 2019 15:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 19:18:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

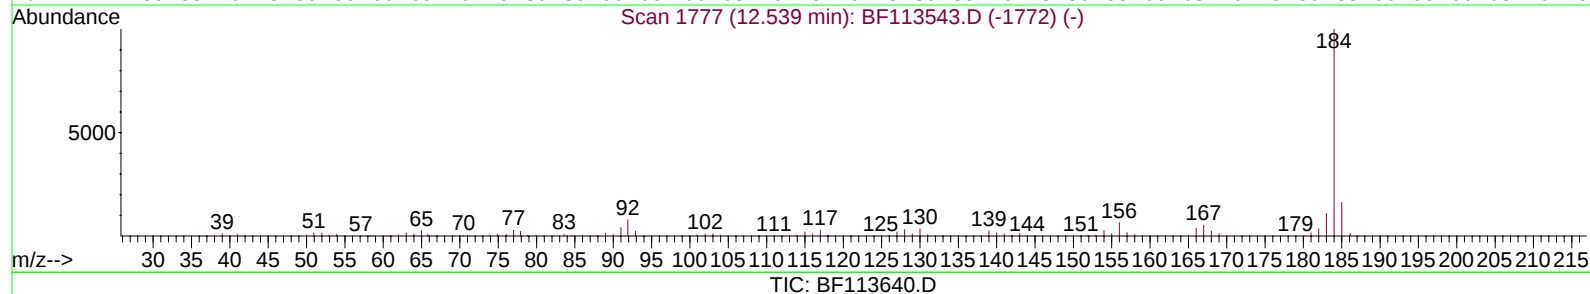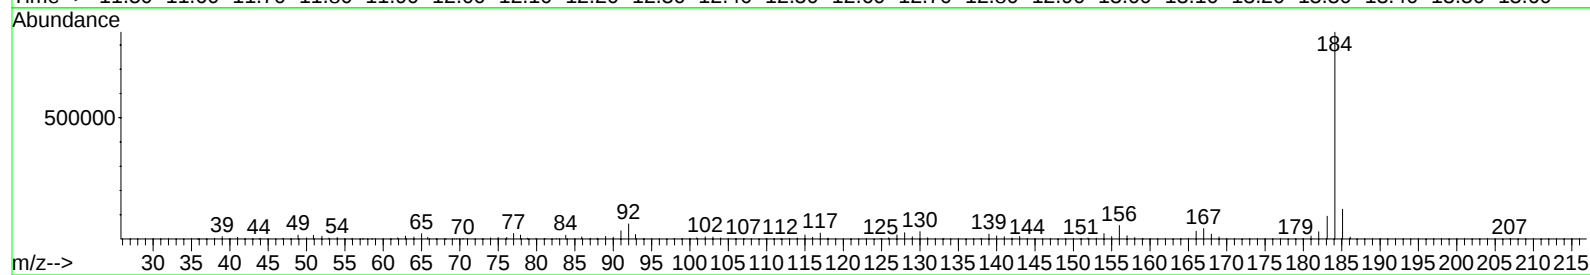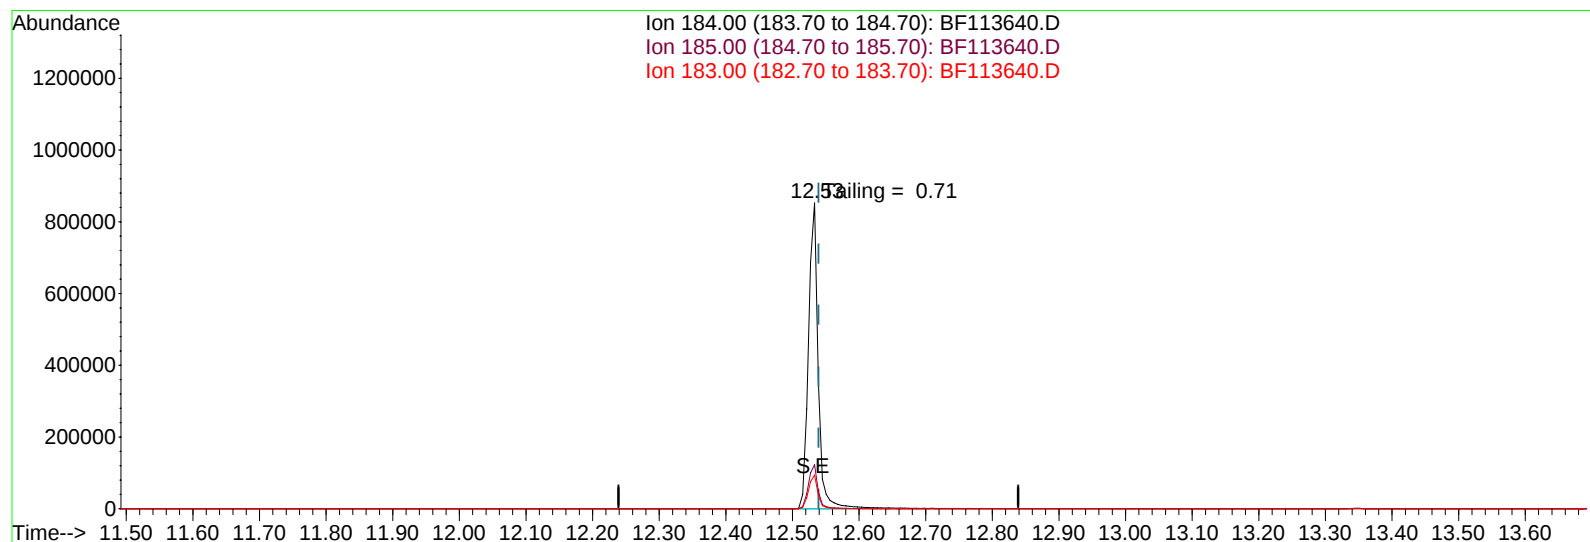

(77) Benzidine

12.533min (-0.006) 0.00ng

response 866349

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.41
183.00	11.20	11.05
0.00	0.00	0.00