

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040819\
 Data File : BF113643.D
 Acq On : 8 Apr 2019 16:52
 Operator : JU/SJ
 Sample : PB118680BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB118680BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.304	544	547	571	rBV	2070879	2473705	72.08%	9.506%
2	6.334	718	722	739	rBV	2265251	2579705	75.17%	9.914%
3	6.457	739	743	763	rVB	2822840	2605825	75.93%	10.014%
4	6.681	778	781	793	rVB	811892	712065	20.75%	2.736%
5	6.840	803	808	823	rBV	2023875	2063922	60.14%	7.932%
6	7.245	873	877	893	rBV	1605845	1638908	47.76%	6.298%
7	7.963	995	999	1016	rBV	926506	926619	27.00%	3.561%
8	9.039	1177	1182	1185	rBV	3424956	3079380	89.73%	11.834%
9	9.716	1292	1297	1308	rBV	1008290	1068646	31.14%	4.107%
10	10.504	1427	1431	1459	rBV	1955410	2092289	60.97%	8.041%
11	11.192	1545	1548	1564	rVB	1094648	1179099	34.36%	4.531%
12	12.774	1813	1817	1821	rBV	3253239	3431791	100.00%	13.188%
13	13.827	1992	1996	2006	rBV	956089	1081376	31.51%	4.156%
14	14.298	2071	2076	2079	rBV2	30684	43687	1.27%	0.168%
15	14.586	2122	2125	2128	rBV	43655	44177	1.29%	0.170%
16	14.898	2175	2178	2182	rVB	46821	47561	1.39%	0.183%
17	15.239	2231	2236	2244	rBV	645386	861009	25.09%	3.309%
18	15.639	2301	2304	2310	rBV	33860	50343	1.47%	0.193%
19	16.092	2379	2381	2389	rVB3	26316	41285	1.20%	0.159%


Sum of corrected areas: 26021392

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040819\
Data File : BF113643.D
Acq On : 8 Apr 2019 16:52
Operator : JU/SJ
Sample : PB118680BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118680BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

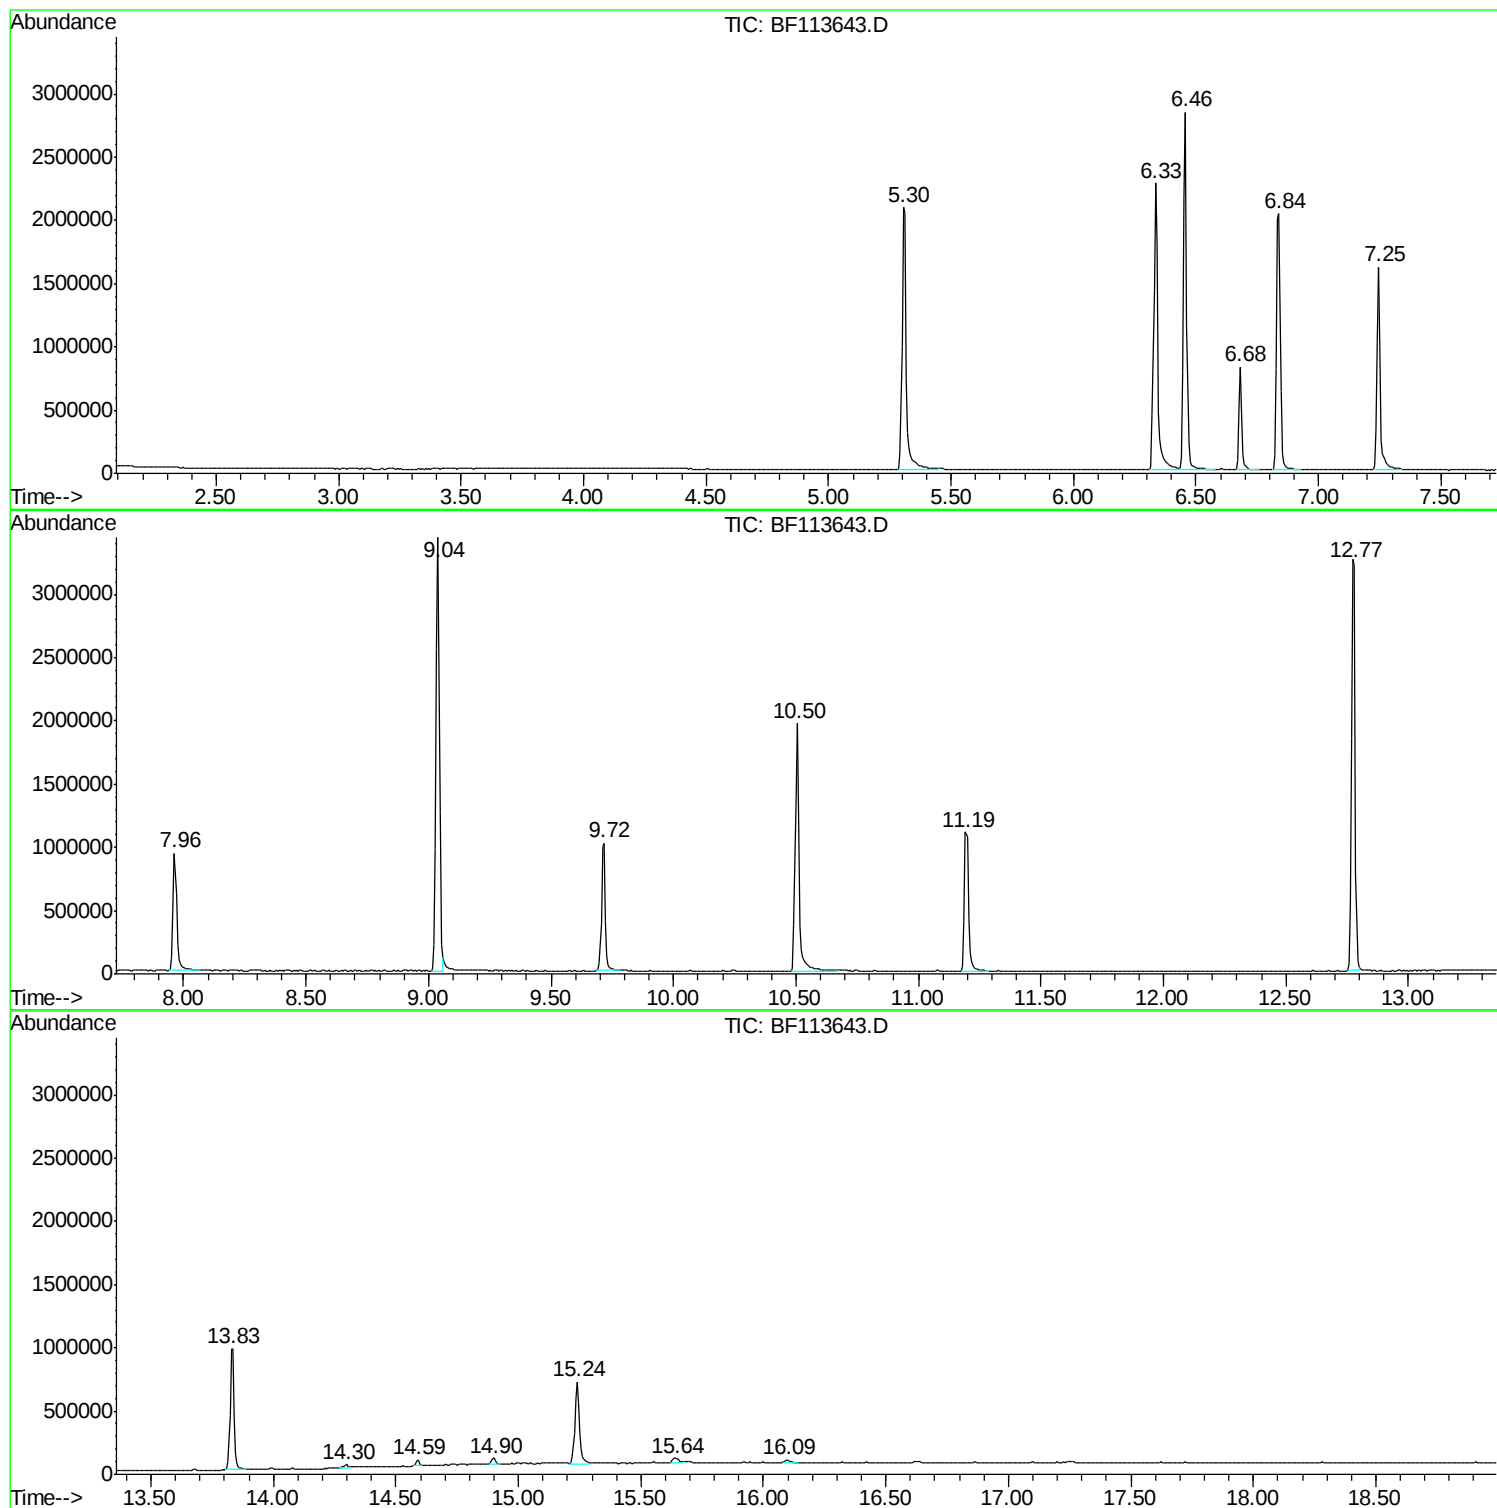

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040819\
Data File : BF113643.D
Acq On : 8 Apr 2019 16:52
Operator : JU/SJ
Sample : PB118680BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118680BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	73.19 ng	2605830	1,4-Dichlorobenzene-d4	6.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		Xenon	132	Xe	007440-63-3	9

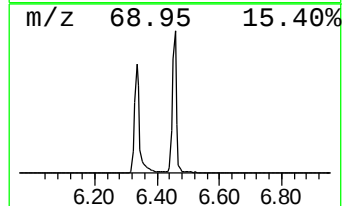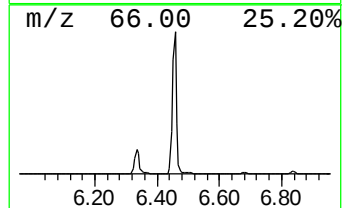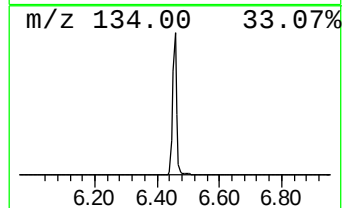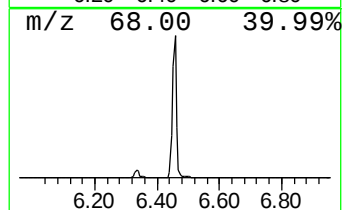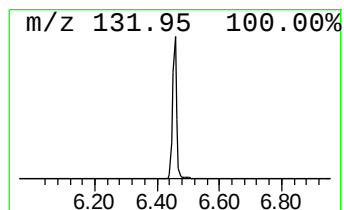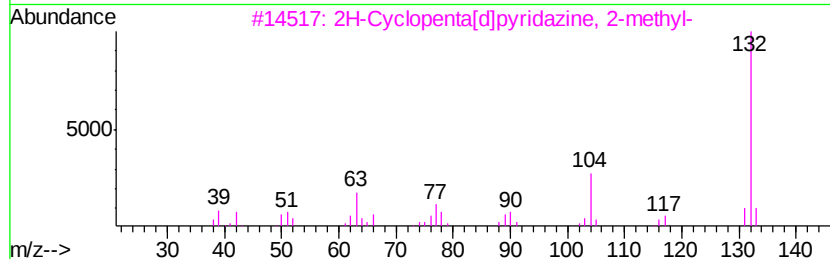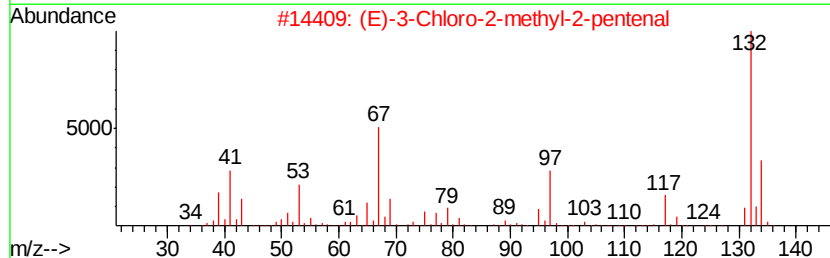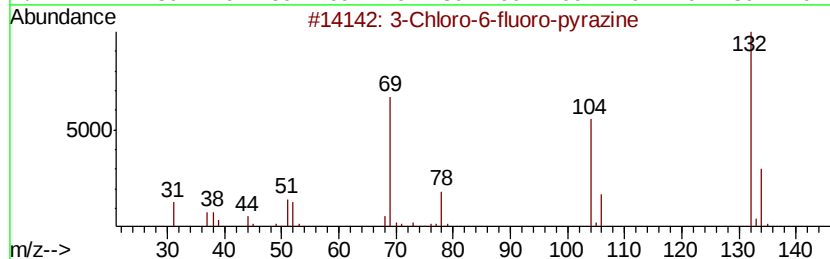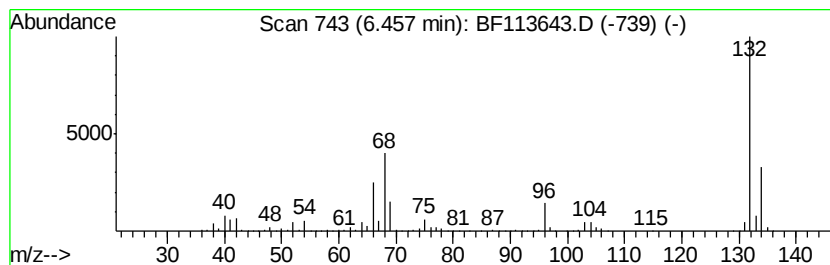

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040819\
Data File : BF113643.D
Acq On : 8 Apr 2019 16:52
Operator : JU/SJ
Sample : PB118680BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118680BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.46	6.46	73.2	ng	2605830	1	6.68	712065	20.0