


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040819\
 Data File : BF113640.D
 Acq On : 8 Apr 2019 15:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

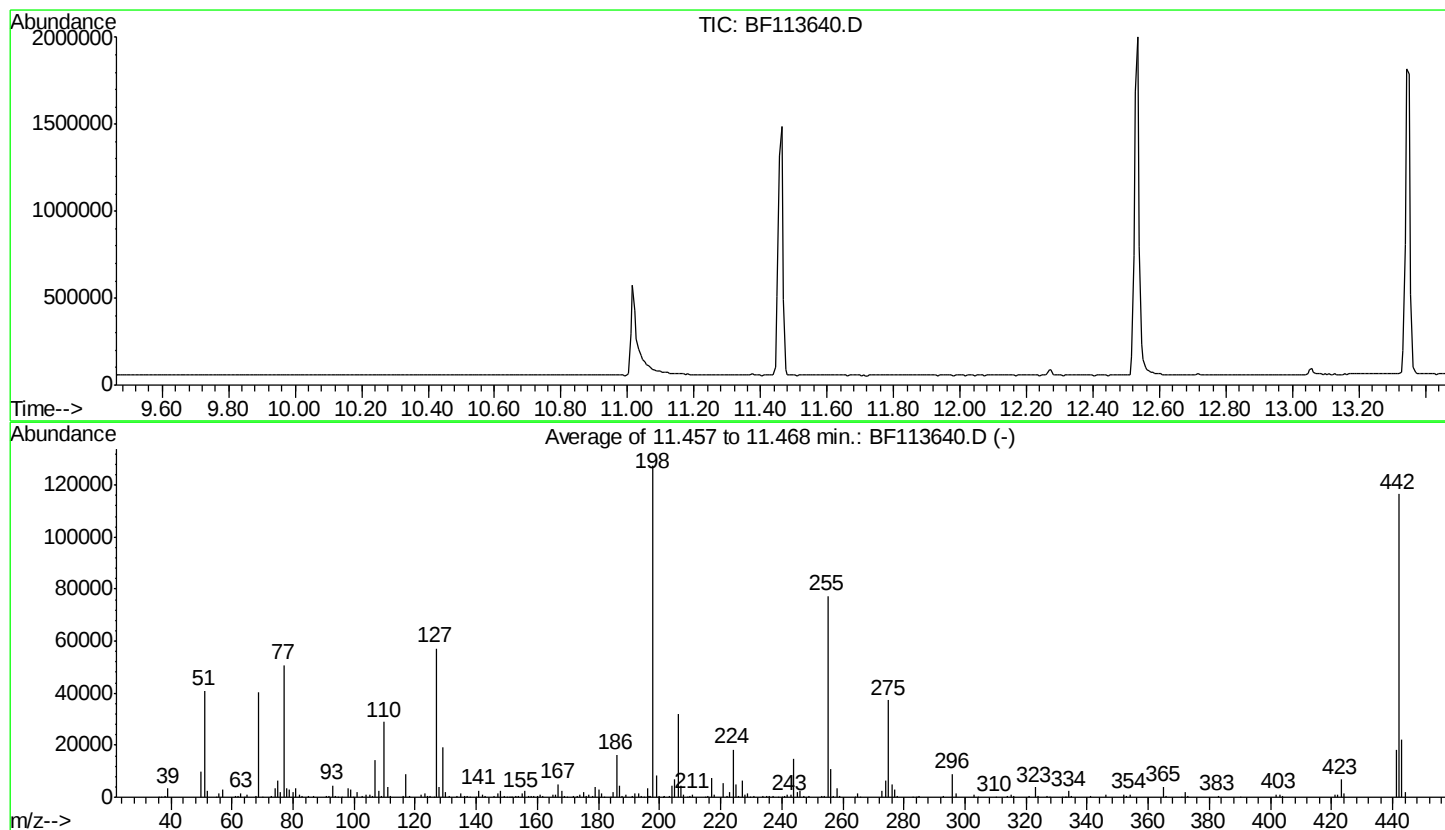

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	41083	PASS
68	69	0.00	2	1.4	569	PASS
69	198	0.00	100	31.6	40332	PASS
70	69	0.00	2	0.3	109	PASS
127	198	10	80	44.8	57114	PASS
197	198	0.00	2	0.4	489	PASS
198	198	100	100	100.0	127458	PASS
199	198	5	9	6.6	8432	PASS
275	198	10	60	29.2	37280	PASS
365	198	1	100	3.2	4024	PASS
441	198	0.01	100	14.4	18291	PASS
442	198	50	100	91.3	116384	PASS
443	442	15	24	18.9	22002	PASS