

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040820\
 Data File : BF119843.D
 Acq On : 9 Apr 2020 00:17
 Operator : MA/SJ
 Sample : PB128044BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128044BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	555	561	564	rBV	4910091	5079325	70.25%	11.834%
2	6.398	727	733	736	rBV	4359668	5097344	70.50%	11.876%
3	6.763	791	795	799	rBV	1040964	875034	12.10%	2.039%
4	6.922	817	822	825	rBV	4457197	4167232	57.64%	9.709%
5	7.328	885	891	894	rBV	3087906	3386176	46.83%	7.889%
6	8.045	1009	1013	1017	rBV	1056170	1136051	15.71%	2.647%
7	9.127	1191	1197	1201	rBV	5090030	6158937	85.18%	14.350%
8	9.804	1307	1312	1316	rBV	1368413	1316754	18.21%	3.068%
9	10.598	1440	1447	1450	rBV	4034080	4136996	57.22%	9.639%
10	11.292	1557	1565	1568	rBV	1729355	1483659	20.52%	3.457%
11	12.892	1831	1837	1840	rBV	6898261	7230184	100.00%	16.846%
12	13.933	2010	2014	2017	rBV	1761814	1484629	20.53%	3.459%
13	15.368	2253	2258	2262	rBV	1159764	1368186	18.92%	3.188%


Sum of corrected areas: 42920507

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040820\
Data File : BF119843.D
Acq On : 9 Apr 2020 00:17
Operator : MA/SJ
Sample : PB128044BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128044BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

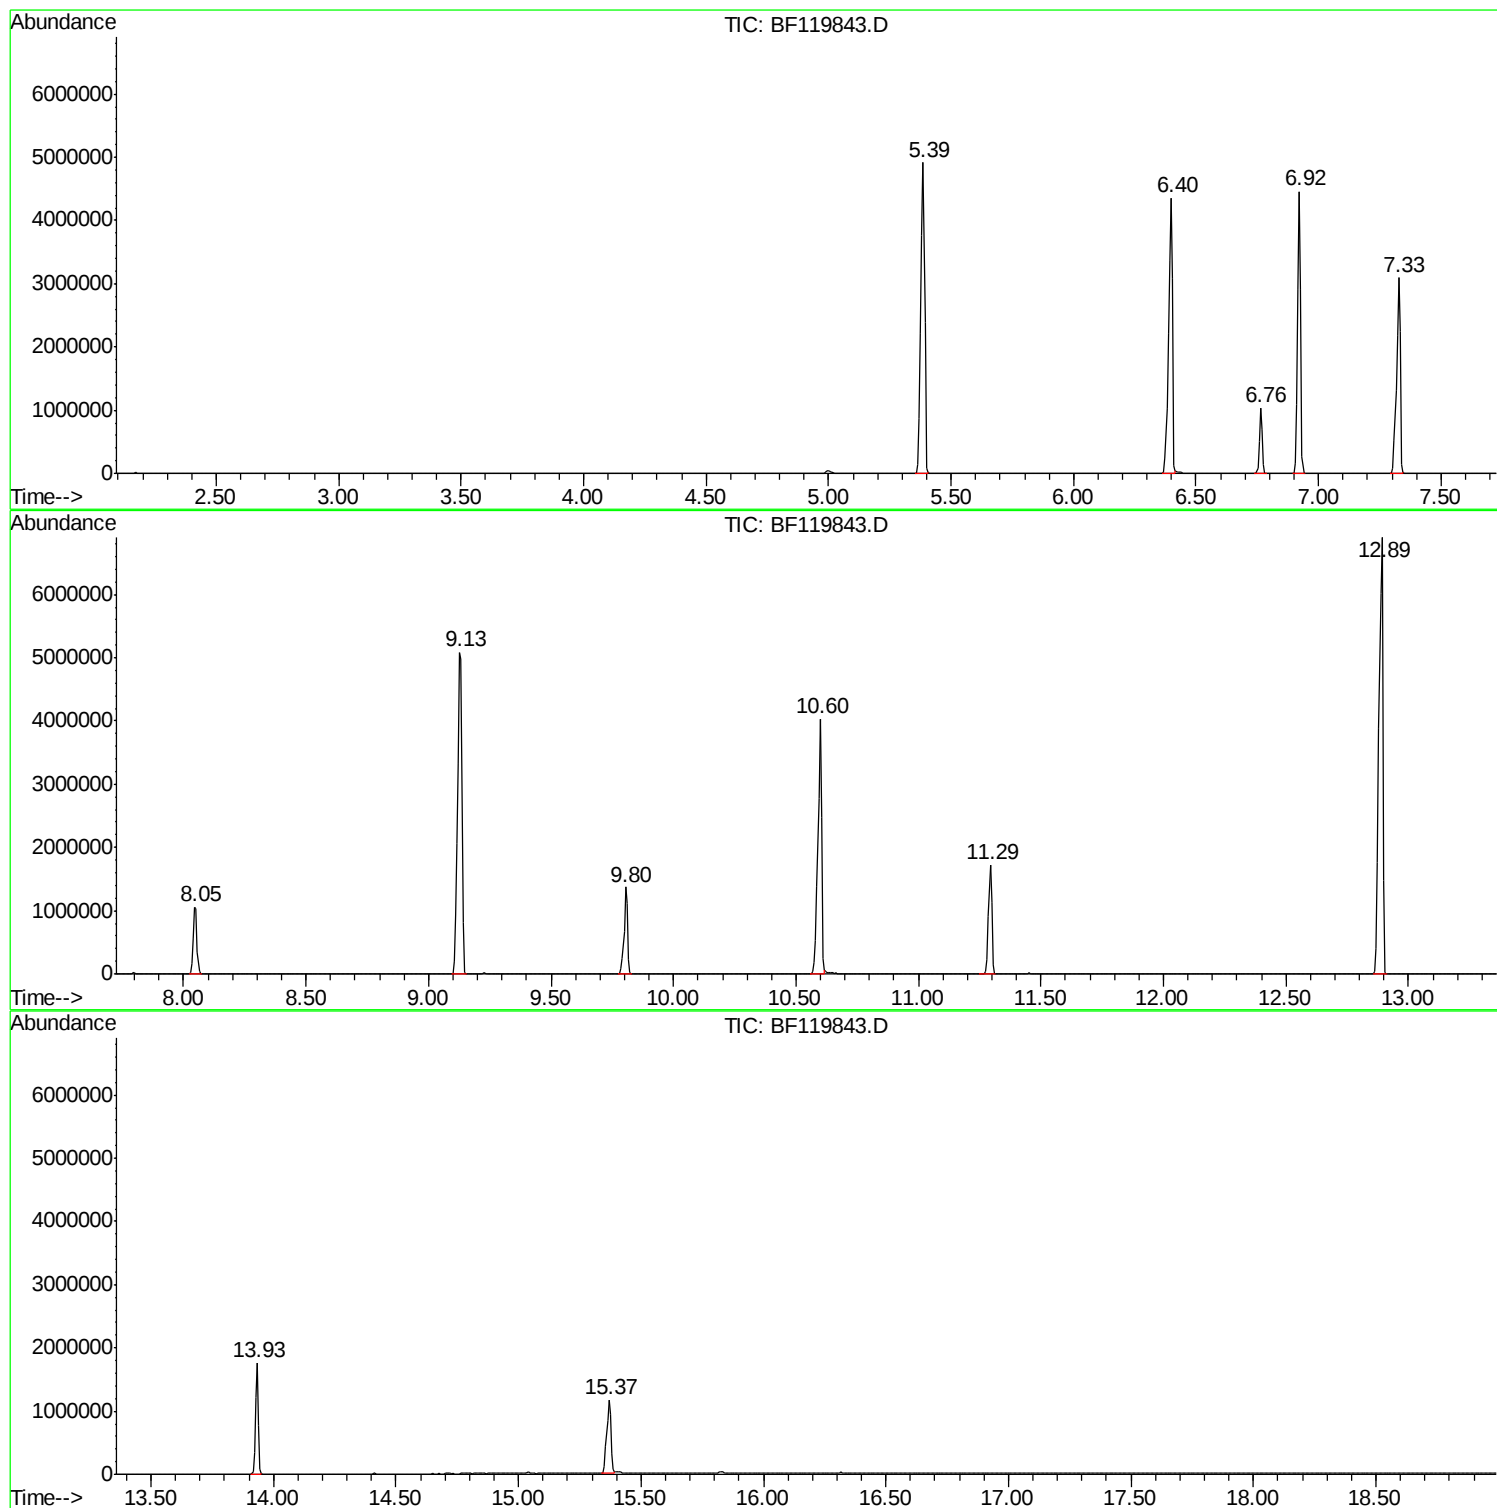

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040820\
Data_File : BF119843.D
Acq_On : 9-Apr-2020 00:177
Operator : MA/SJJ
Sample : PB128044BLL
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB128044BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
