


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040820\
 Data File : BF119831.D
 Acq On : 8 Apr 2020 18:20
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 09 01:21:19 2020

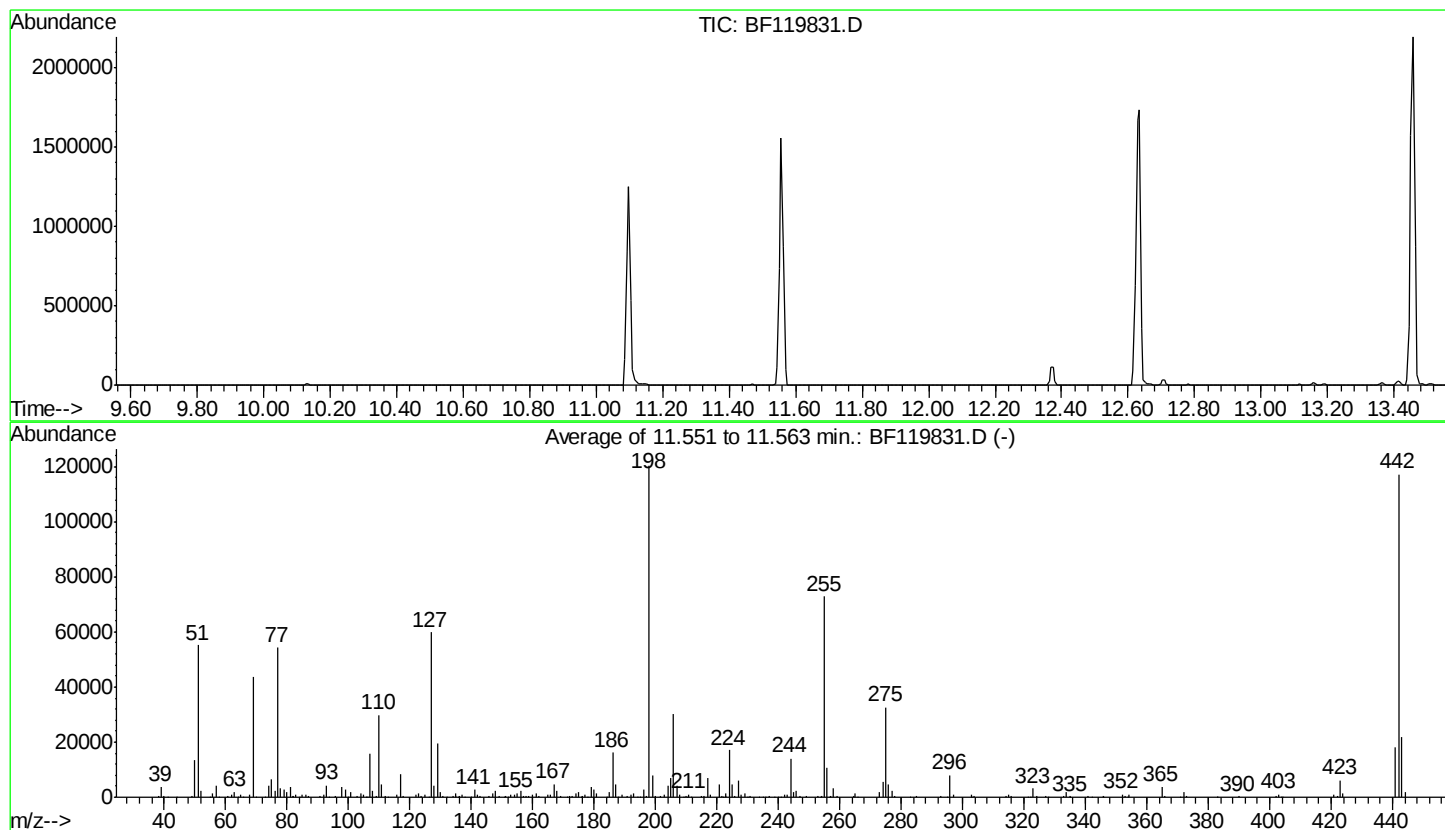

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	55266	PASS
68	69	0.00	2	1.8	807	PASS
69	198	0.00	100	36.3	43680	PASS
70	69	0.00	2	0.4	158	PASS
127	198	10	80	49.8	59869	PASS
197	198	0.00	2	0.5	548	PASS
198	198	100	100	100.0	120336	PASS
199	198	5	9	6.4	7727	PASS
275	198	10	60	27.0	32546	PASS
365	198	1	100	3.3	3920	PASS
441	198	0.01	100	15.2	18341	PASS
442	198	50	100	97.5	117274	PASS
443	442	15	24	18.8	22054	PASS