


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040820\
 Data File : BF119869.D
 Acq On : 9 Apr 2020 15:09
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 09 01:21:19 2020

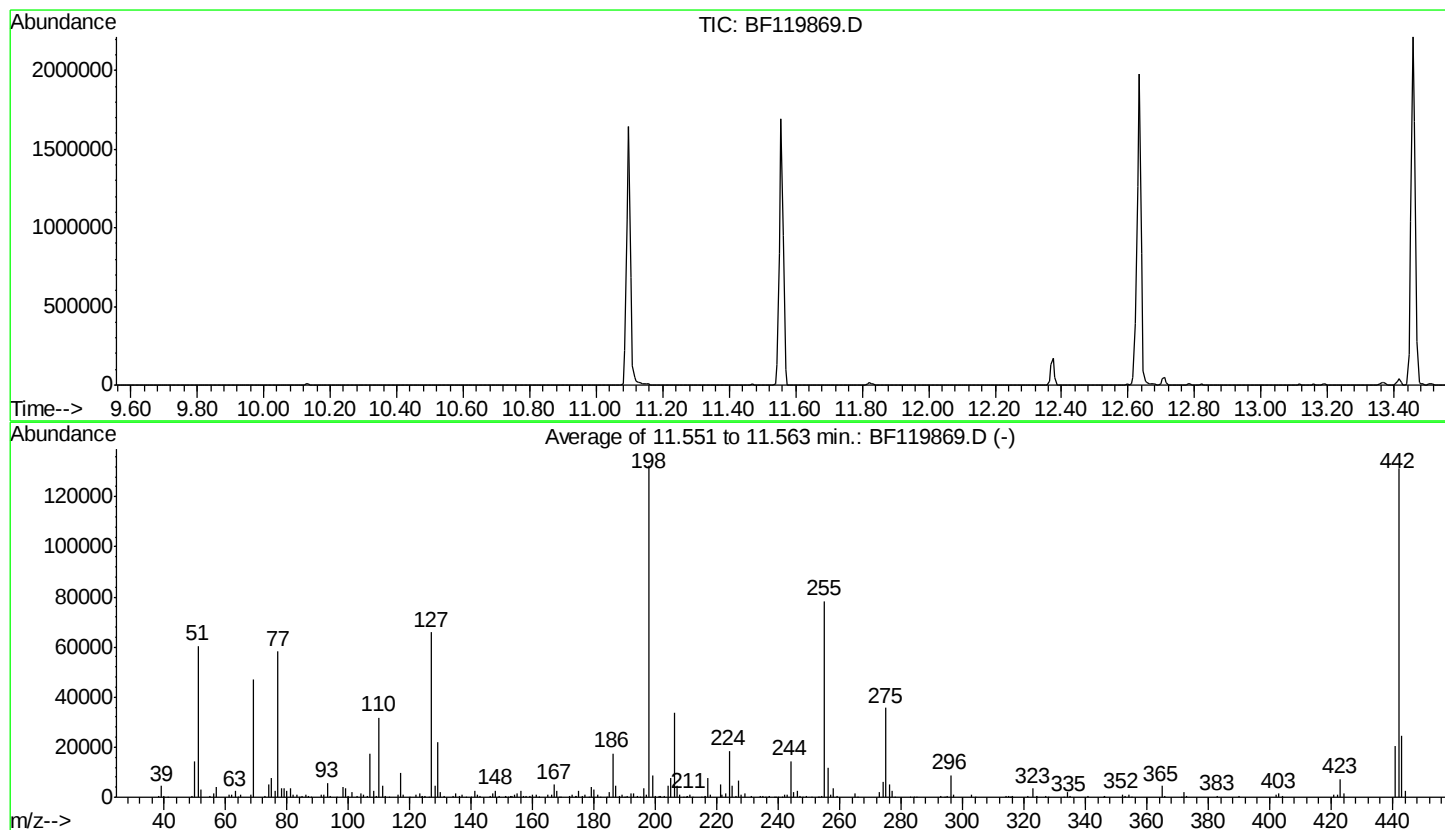

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	60578	PASS
68	69	0.00	2	1.8	830	PASS
69	198	0.00	100	35.6	47117	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	65928	PASS
197	198	0.00	2	0.7	948	PASS
198	198	100	100	100.0	132432	PASS
199	198	5	9	6.7	8875	PASS
275	198	10	60	26.9	35594	PASS
365	198	1	100	3.5	4579	PASS
441	198	0.01	100	15.5	20550	PASS
442	198	50	100	99.1	131304	PASS
443	442	15	24	18.6	24390	PASS