


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041019\
 Data File : BF113695.D
 Acq On : 10 Apr 2019 13:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

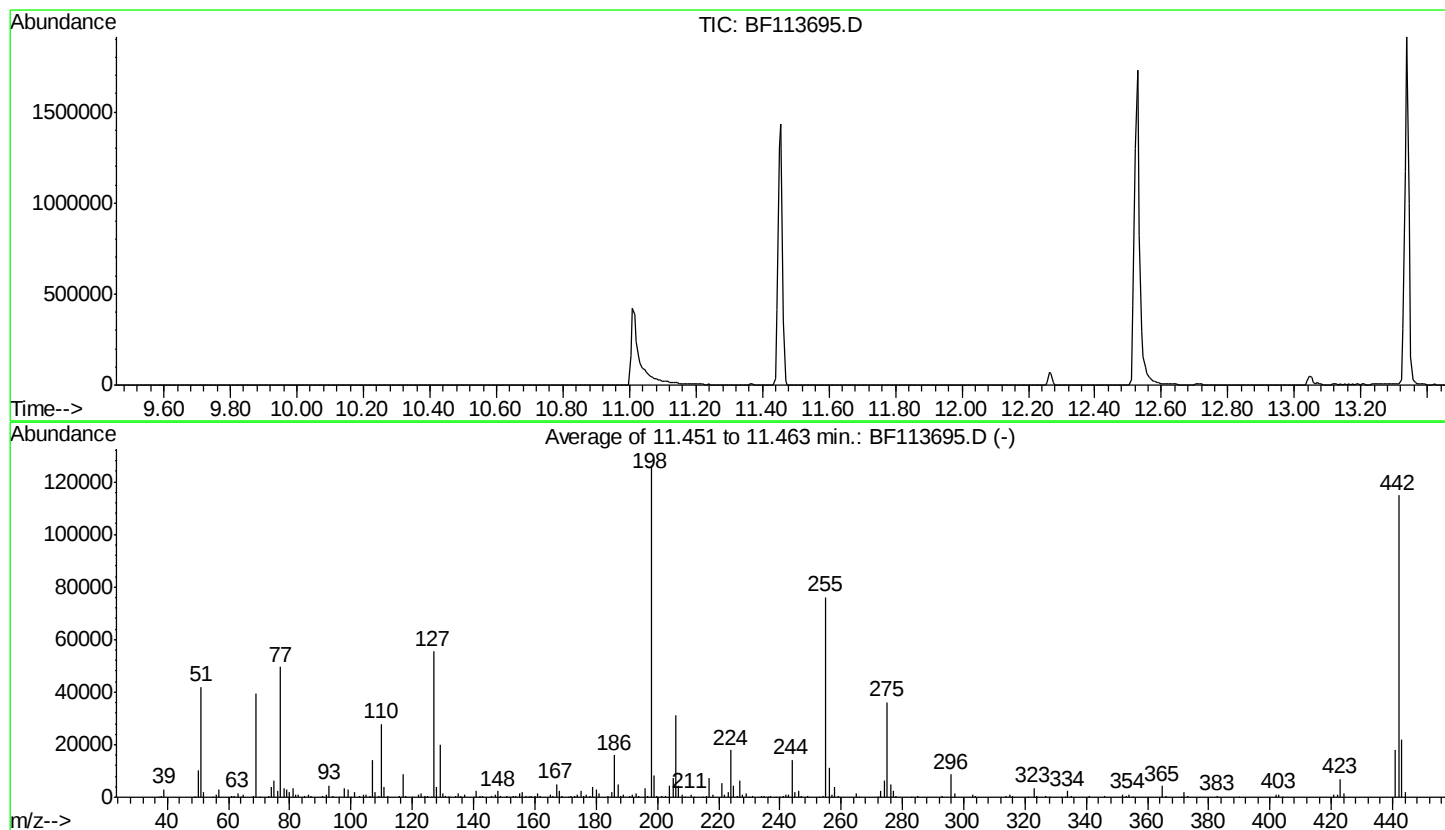

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	42117	PASS
68	69	0.00	2	1.3	527	PASS
69	198	0.00	100	31.5	39681	PASS
70	69	0.00	2	0.3	124	PASS
127	198	10	80	44.0	55496	PASS
197	198	0.00	2	0.6	731	PASS
198	198	100	100	100.0	126170	PASS
199	198	5	9	6.5	8234	PASS
275	198	10	60	28.6	36105	PASS
365	198	1	100	3.4	4313	PASS
441	198	0.01	100	14.5	18244	PASS
442	198	50	100	90.9	114714	PASS
443	442	15	24	19.2	22009	PASS