
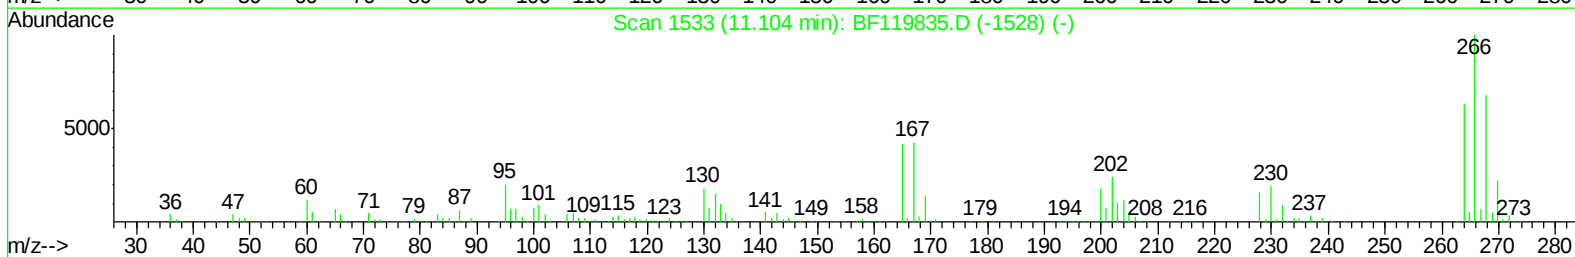
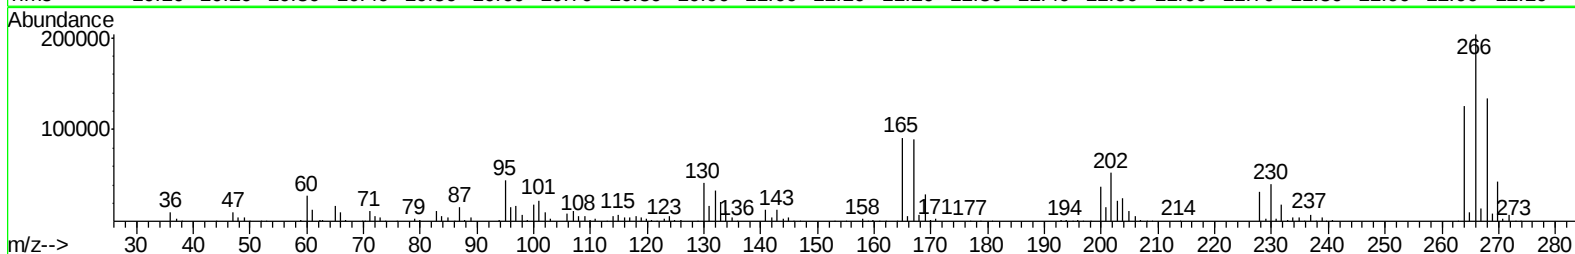


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF041020\
Data File : BF119889.D
Acq On : 10 Apr 2020 11:55
Operator : MA/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 01:12:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 10 13:48:19 2020
Response via : Initial Calibration

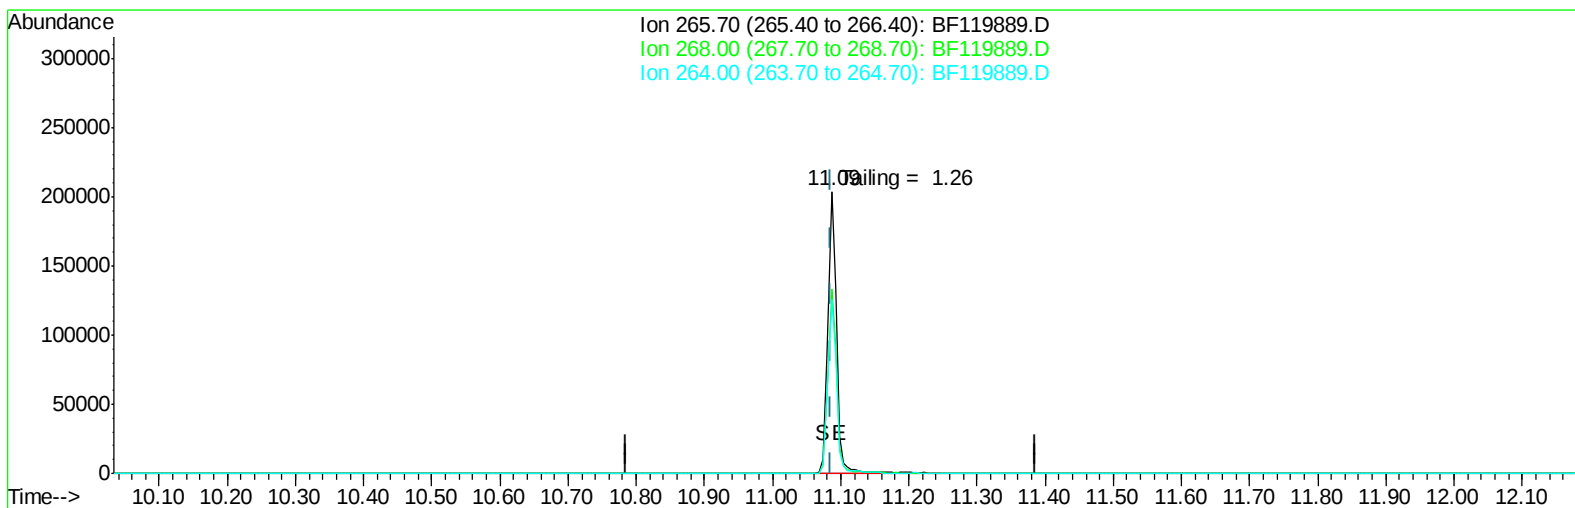

TIC: BF119889.D

(70) Pentachlorophenol (C)




11.086min (+0.000) 56007.18ng

response 171425

Ion	Exp%	Act%
265.70	100	100
268.00	67.80	65.58
264.00	63.30	61.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF041020\
 Data File : BF119889.D
 Acq On : 10 Apr 2020 11:55
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 01:12:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 10 13:48:19 2020
 Response via : Initial Calibration

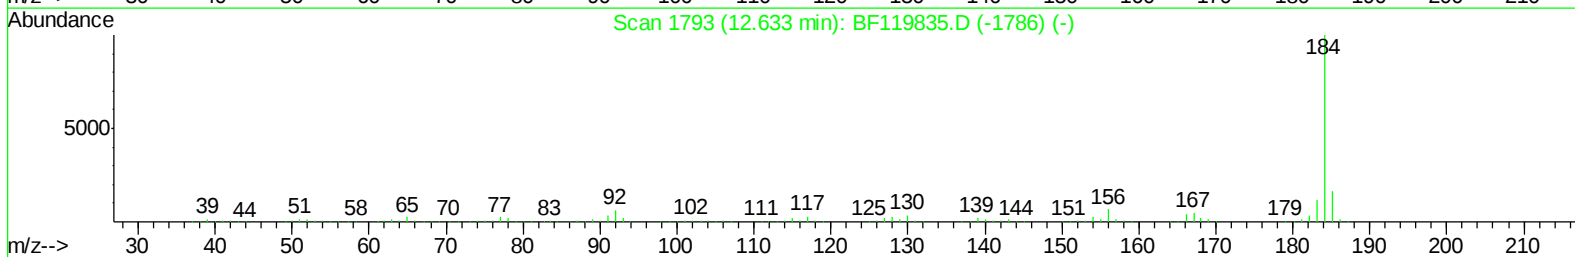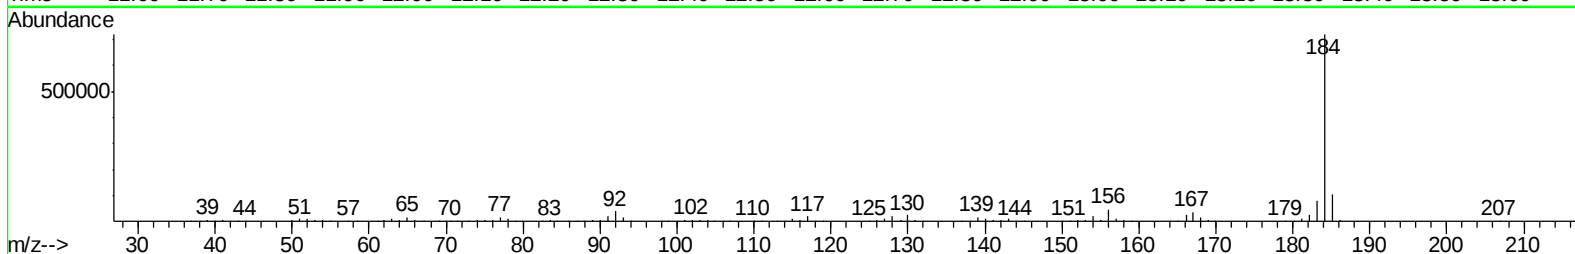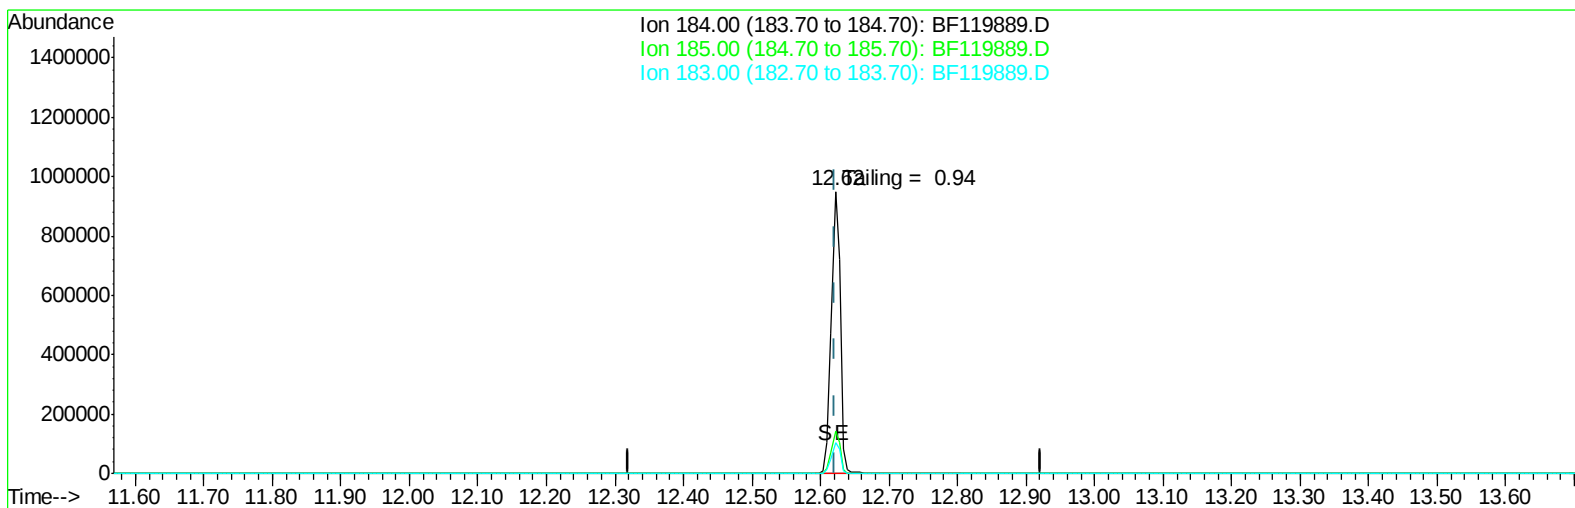

TIC: BF119889.D

(77) Benzidine

12.622min (+0.000) 0.00ng

response 837786

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	15.07
183.00	11.40	11.14
0.00	0.00	0.00