

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041020\
 Data File : BF119898.D
 Acq On : 10 Apr 2020 16:51
 Operator : MA/SJ
 Sample : L2201-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CG-SUB

Quant Time: Apr 11 01:51:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 10 13:48:19 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	151201	20.00	ng	0.00
21) Naphthalene-d8	8.03	136	578930	20.00	ng	0.00
39) Acenaphthene-d10	9.79	164	309719	20.00	ng	0.00
64) Phenanthrene-d10	11.28	188	605809	20.00	ng	0.00
76) Chrysene-d12	13.92	240	476415	20.00	ng	0.00
87) Perylene-d12	15.35	264	401581	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	1034433	118.23	ng	0.00
7) Phenol-d6	6.39	99	1332738	118.22	ng	0.00
23) Nitrobenzene-d5	7.32	82	793047	70.87	ng	0.00
42) 2,4,6-Tribromophenol	10.59	330	409561	108.01	ng	0.00
45) 2-Fluorobiphenyl	9.12	172	1516574	69.52	ng	0.00
79) Terphenyl-d14	12.87	244	1668783	58.94	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.51	163	282657	11.799	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041020\
Data File : BF119898.D
Acq On : 10 Apr 2020 16:51
Operator : MA/SJ
Sample : L2201-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CG-SUB

Quant Time: Apr 11 01:51:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 10 13:48:19 2020
Response via : Initial Calibration

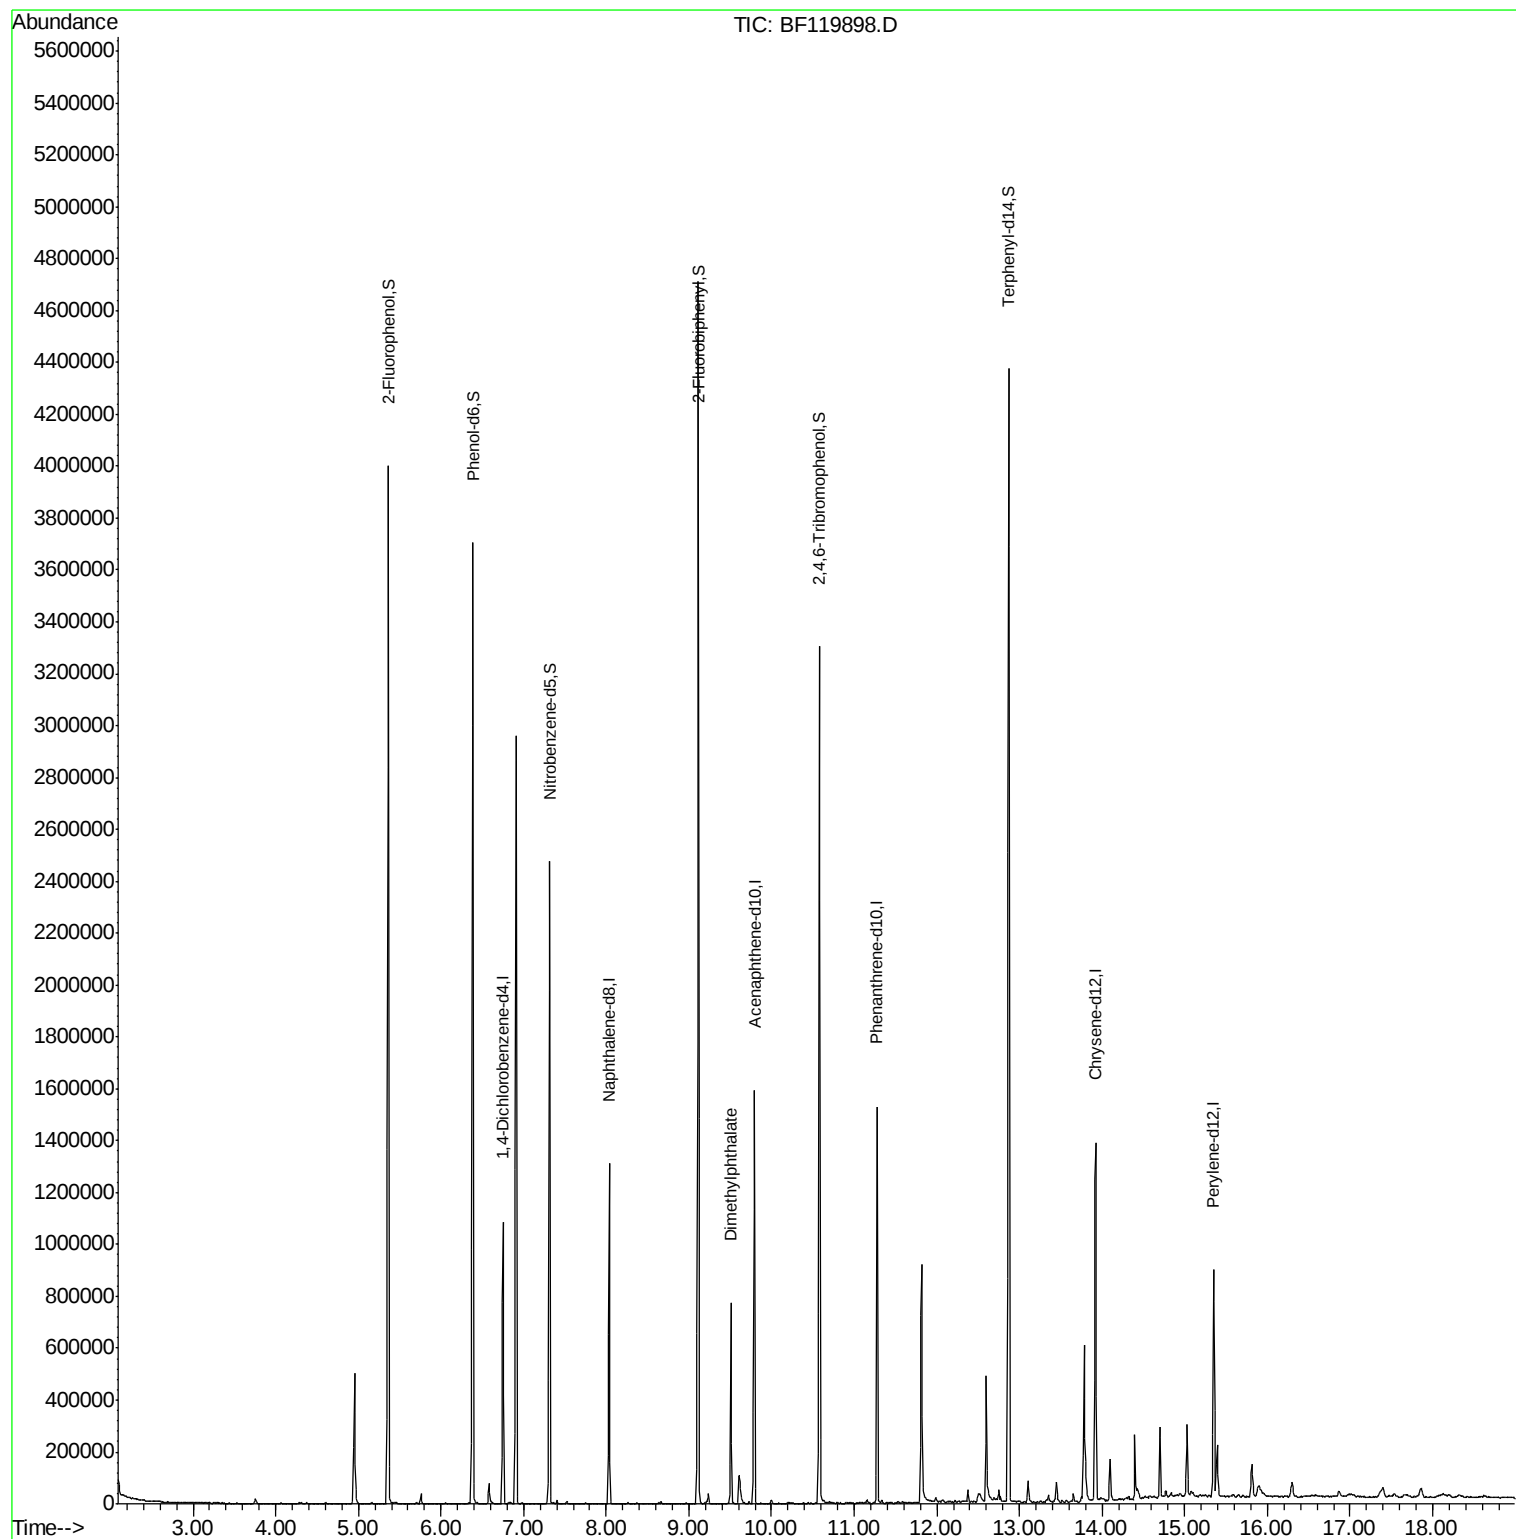




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 793
Delta R.T. 0.00 min
Lab File: BF119898.D
Acq: 10 Apr 2020 16:51

Instrument :
BNA_F
ClientSampleId :
CG-SUB

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.2	124.8	187.2
115	59.1	46.5	69.7

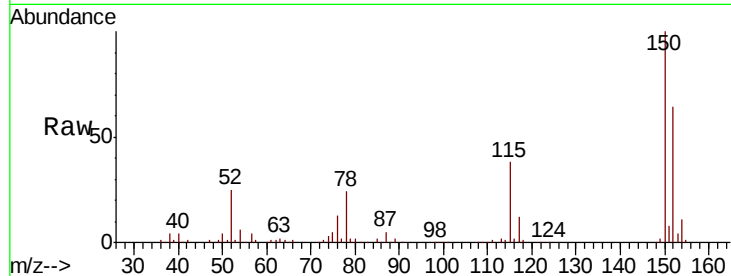


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

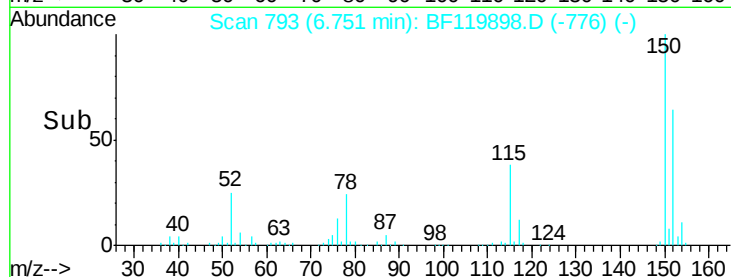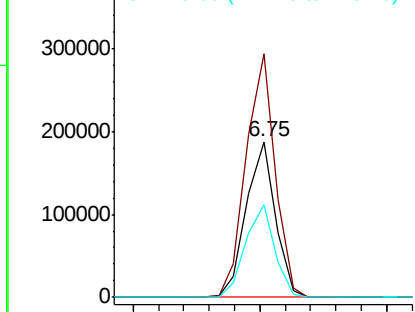



#5

2-Fluorophenol
Concen: 118.233 ng
RT: 5.36 min Scan# 557
Delta R.T. 0.01 min
Lab File: BF119898.D
Acq: 10 Apr 2020 16:51

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.8	55.5	83.3
63	35.9	29.1	43.7

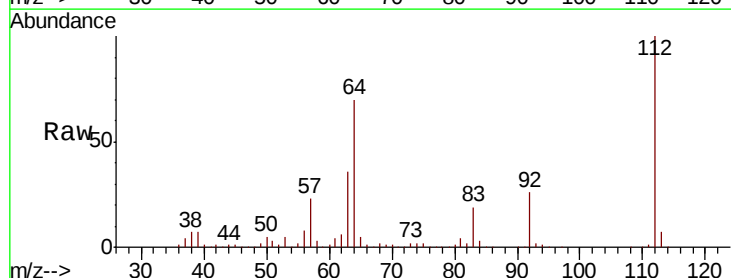

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

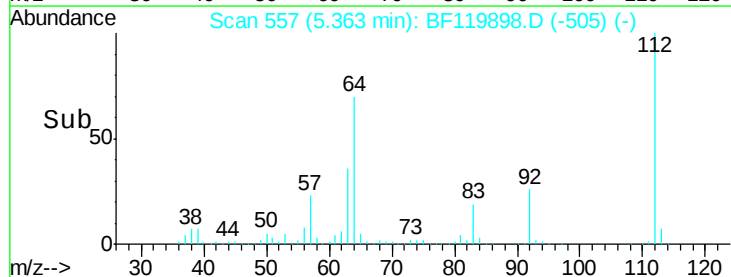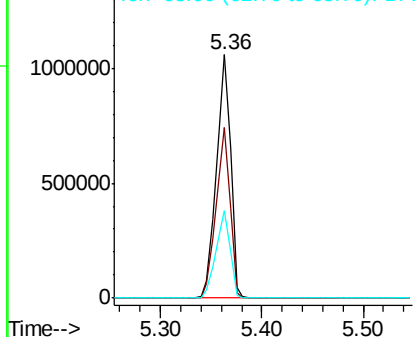



#7

Phenol-d6

Concen: 118.217 ng

RT: 6.39 min Scan# 731

Delta R.T. -0.01 min

Lab File: BF119898.D

Acq: 10 Apr 2020 16:51

Instrument :

BNA_F

ClientSampleId :

CG-SUB




Tot Ion: 99 Resp: 1332738

Ion Ratio Lower Upper

99 100

42 19.9 16.9 25.3

71 33.0 26.3 39.5

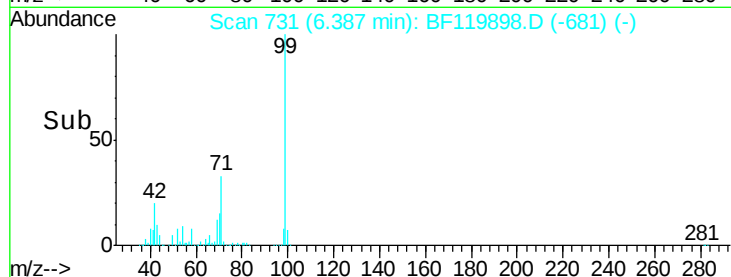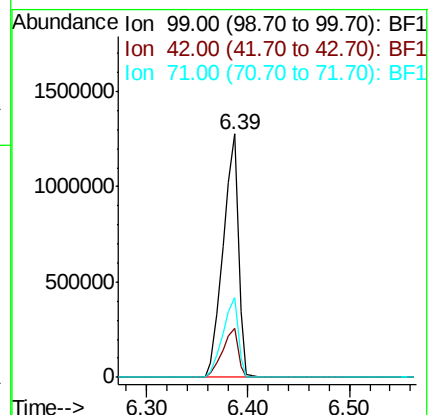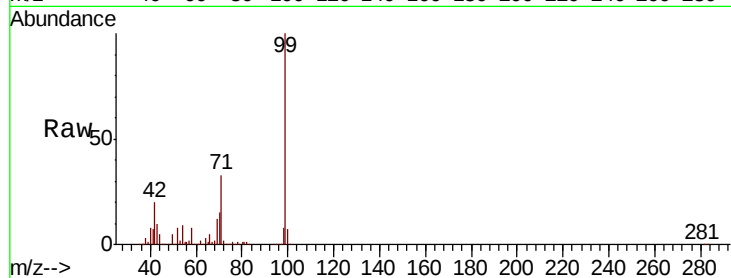

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.03 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF119898.D

Acq: 10 Apr 2020 16:51

Tgt Ion: 136 Resp: 578930




Ion Ratio Lower Upper

136 100

137 11.0 8.7 13.1

54 10.6 8.5 12.7

68 5.4 3.9 5.9

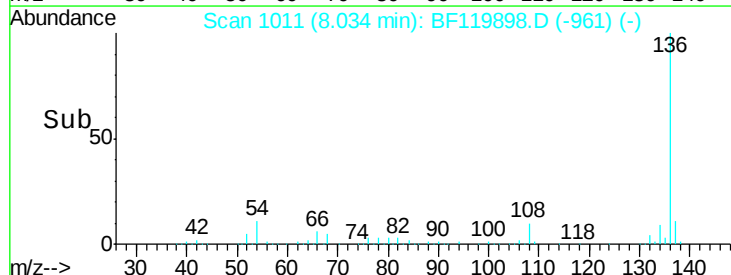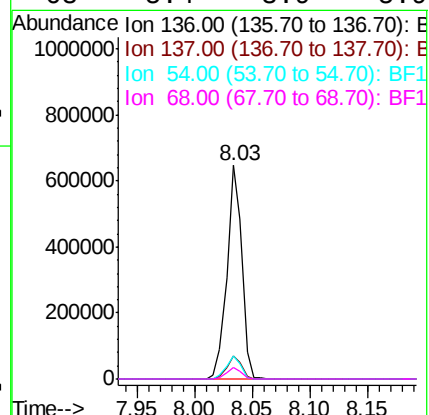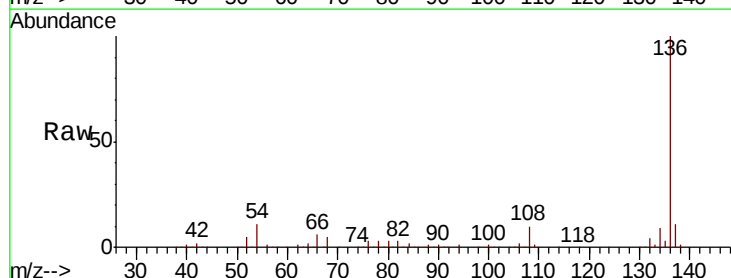






#23
Nitrobenzene-d5
Concen: 70.867 ng
RT: 7.32 min Scan# 889
Delta R.T. -0.01 min
Lab File: BF119898.D
Acq: 10 Apr 2020 16:51

Instrument :
BNA_F
ClientSampleId :
CG-SUB

Tot Ion: 82 Resp: 793047
Ion Ratio Lower Upper
82 100
128 46.5 36.2 54.4
54 61.8 50.4 75.6

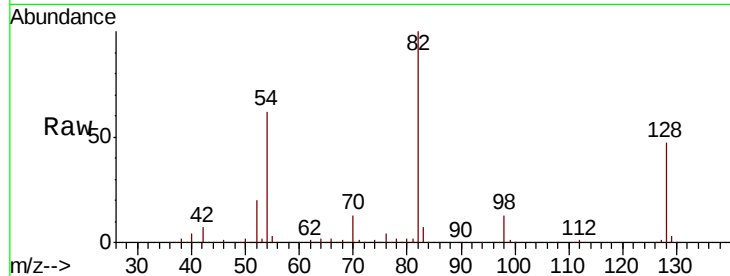


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

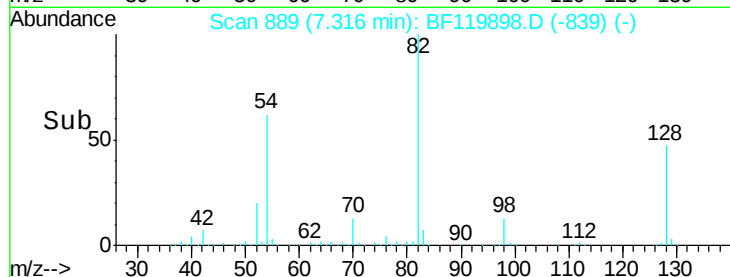
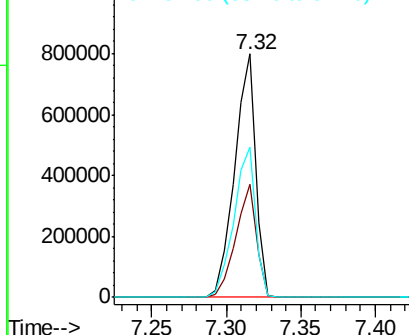



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.79 min Scan# 1310
Delta R.T. -0.01 min
Lab File: BF119898.D
Acq: 10 Apr 2020 16:51

Tgt Ion:164 Resp: 309719
Ion Ratio Lower Upper
164 100
162 102.0 81.9 122.9
160 45.6 36.6 54.8

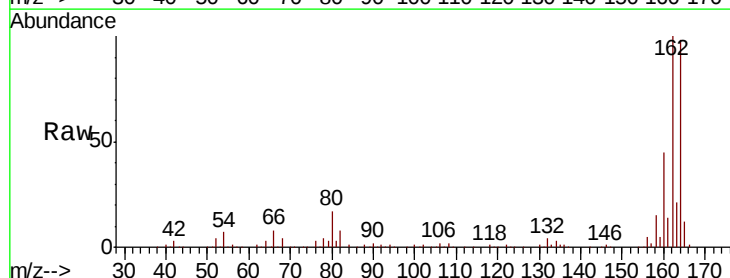

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1



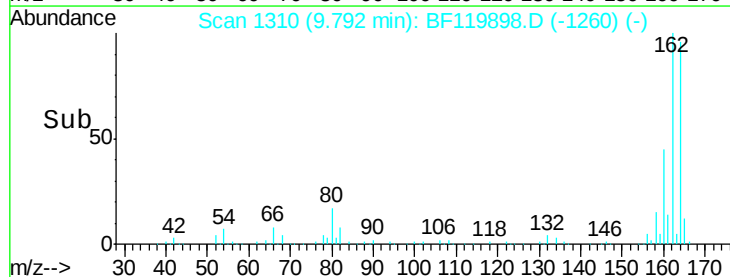
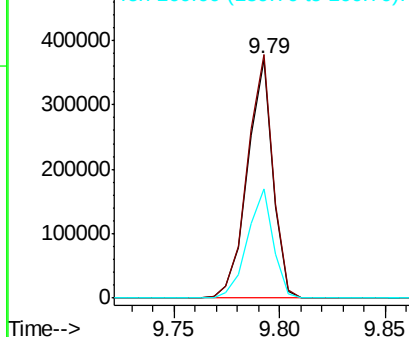


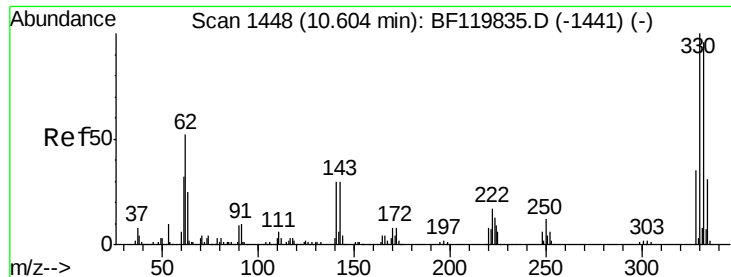

#42
 2,4,6-Tribromophenol
 Concen: 108.006 ng
 RT: 10.59 min Scan# 1445
 Delta R.T. 0.00 min
 Lab File: BF119898.D
 Acq: 10 Apr 2020 16:51




Instrument :
 BNA_F
 ClientSampleId :
 CG-SUB


Tot Ion:330 Resp: 409561
 Ion Ratio Lower Upper
 330 100
 332 96.9 76.8 115.2
 141 31.6 25.1 37.7

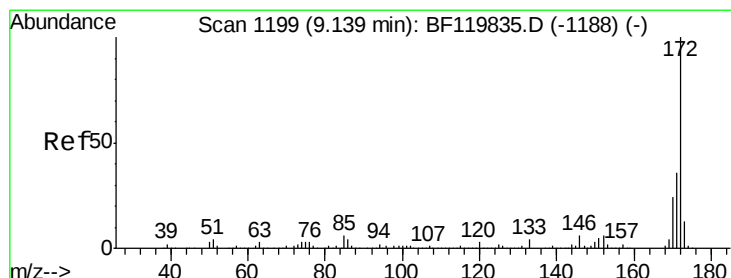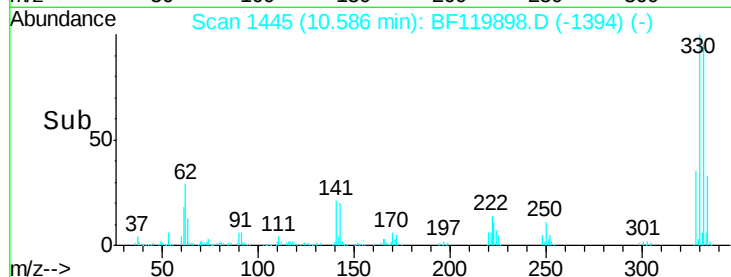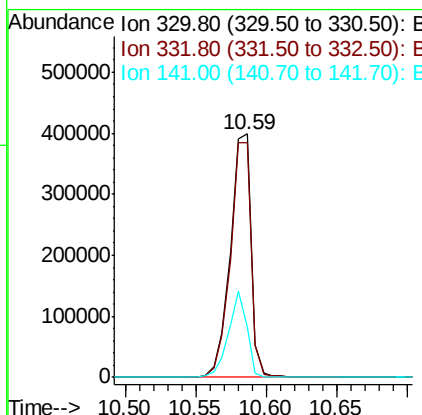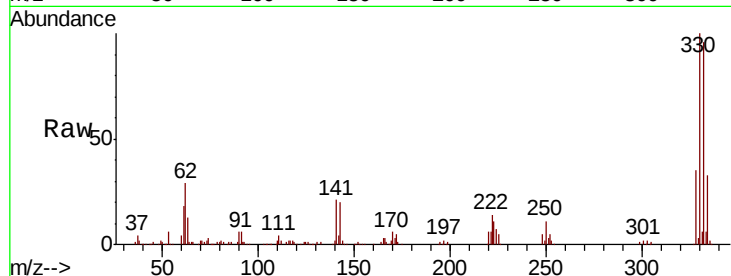

#45
 2-Fluorobiphenyl
 Concen: 69.521 ng
 RT: 9.12 min Scan# 1195
 Delta R.T. -0.01 min
 Lab File: BF119898.D
 Acq: 10 Apr 2020 16:51

Tgt Ion:172 Resp: 1516574
 Ion Ratio Lower Upper
 172 100
 171 36.5 28.9 43.3
 170 24.2 19.4 29.2

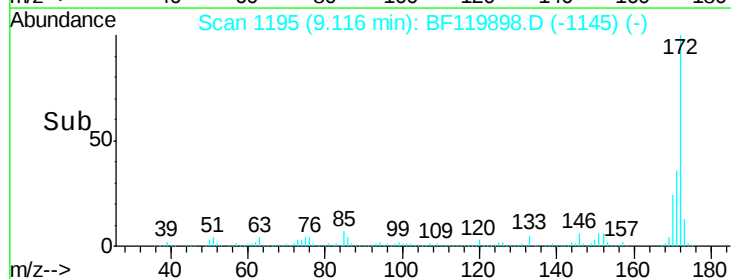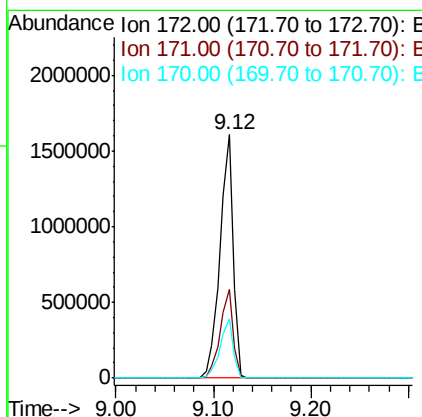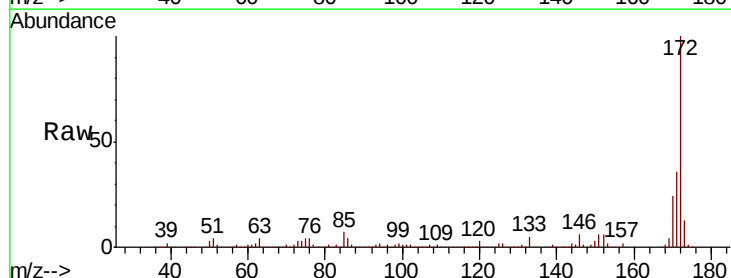

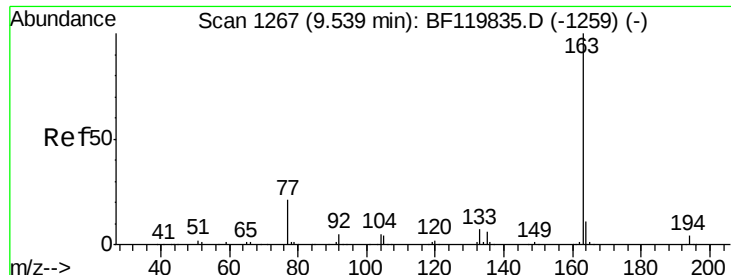

#50

Dimethylphthalate

Concen: 11.799 ng

RT: 9.51 min Scan# 1262

Delta R.T. -0.02 min

Lab File: BF119898.D

Acq: 10 Apr 2020 16:51

Instrument :

BNA_F

ClientSampleId :

CG-SUB


Tot Ion:163 Resp: 282657

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.4




164 10.3 8.4 12.6

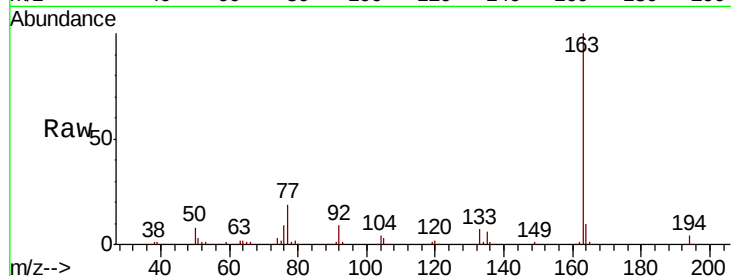

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

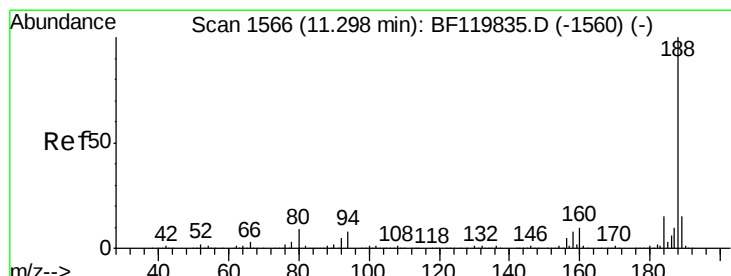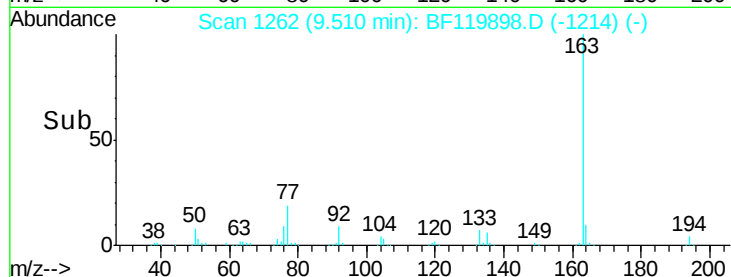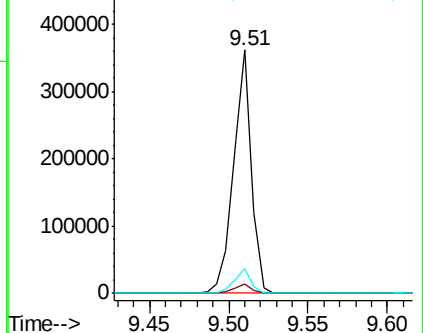

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.28 min Scan# 1563

Delta R.T. 0.00 min

Lab File: BF119898.D

Acq: 10 Apr 2020 16:51


Tgt Ion:188 Resp: 605809

Ion Ratio Lower Upper

188 100

94 7.6 6.7 10.1



80 8.2 7.4 11.2

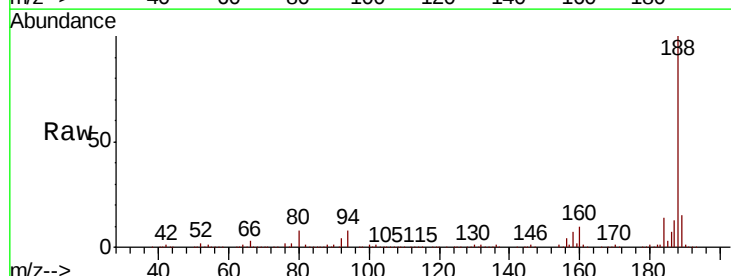


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

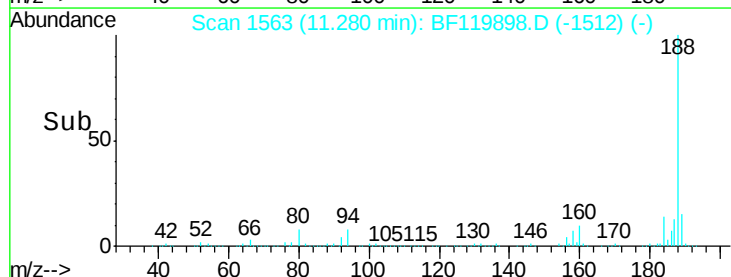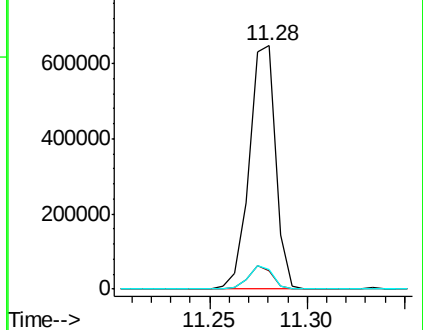

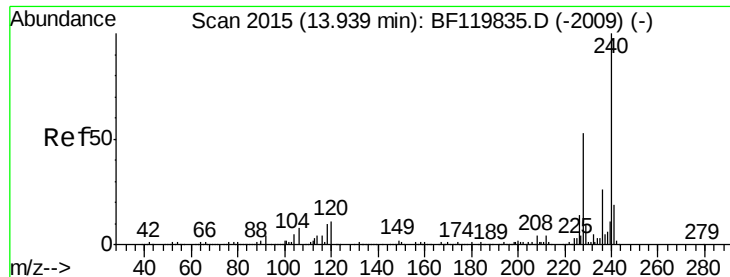

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.92 min Scan# 2012

Delta R.T. -0.01 min

Lab File: BF119898.D

Acq: 10 Apr 2020 16:51

Instrument :

BNA_F

ClientSampleId :

CG-SUB


Tot Ion:240 Resp: 476415

Ion Ratio Lower Upper

240 100

120 9.8 9.0 13.6




236 25.6 20.7 31.1

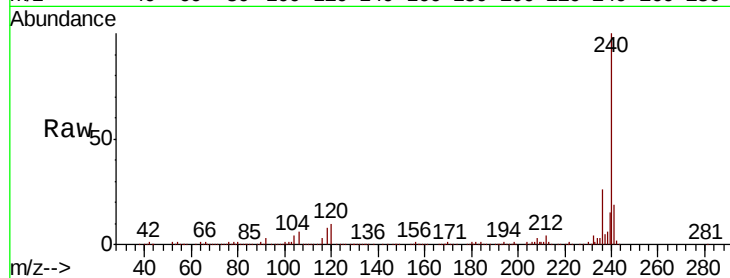

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

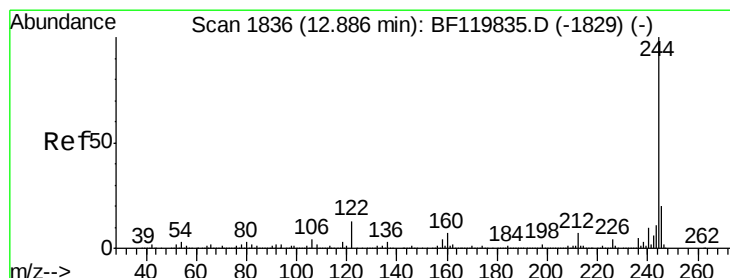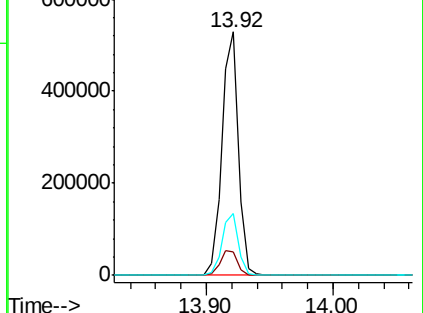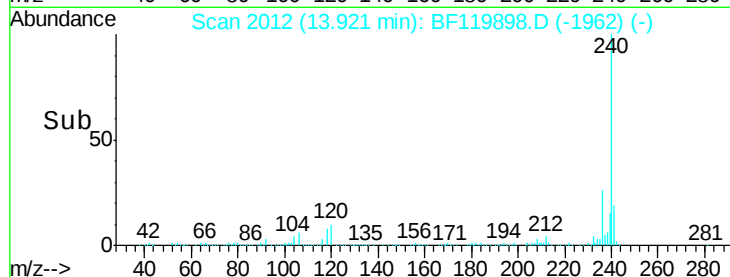

#79

Terphenyl-d14

Concen: 58.940 ng

RT: 12.87 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BF119898.D

Acq: 10 Apr 2020 16:51


Tgt Ion:244 Resp: 1668783

Ion Ratio Lower Upper

244 100

212 6.6 5.4 8.0



122 12.1 10.3 15.5

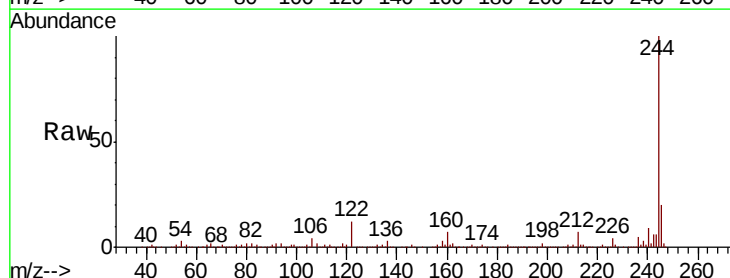


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

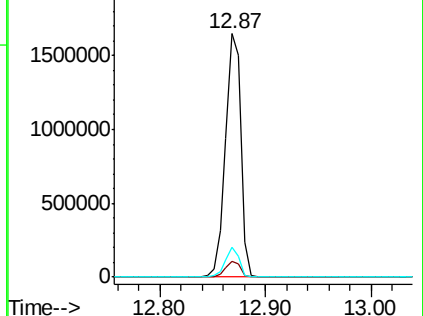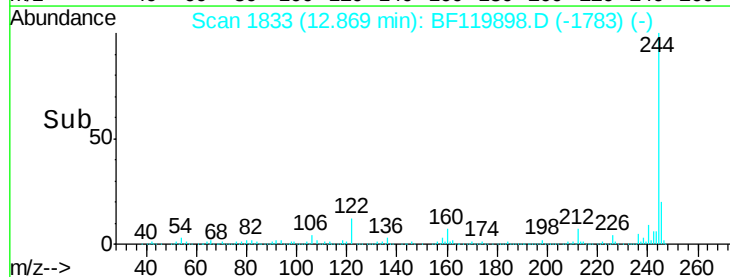


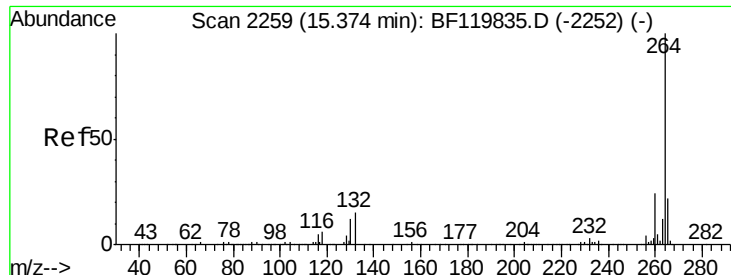

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.35 min Scan# 2255
Delta R.T. -0.01 min
Lab File: BF119898.D
Acq: 10 Apr 2020 16:51

Instrument :
BNA_F
ClientSampleId :
CG-SUB

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.3	28.9
265	21.6	17.6	26.4

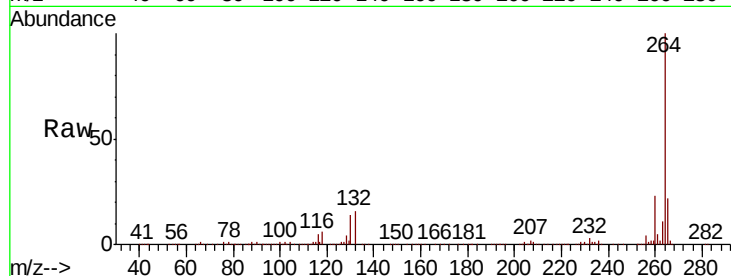

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

