


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041020\
 Data File : BF119889.D
 Acq On : 10 Apr 2020 11:55
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 10 13:48:19 2020

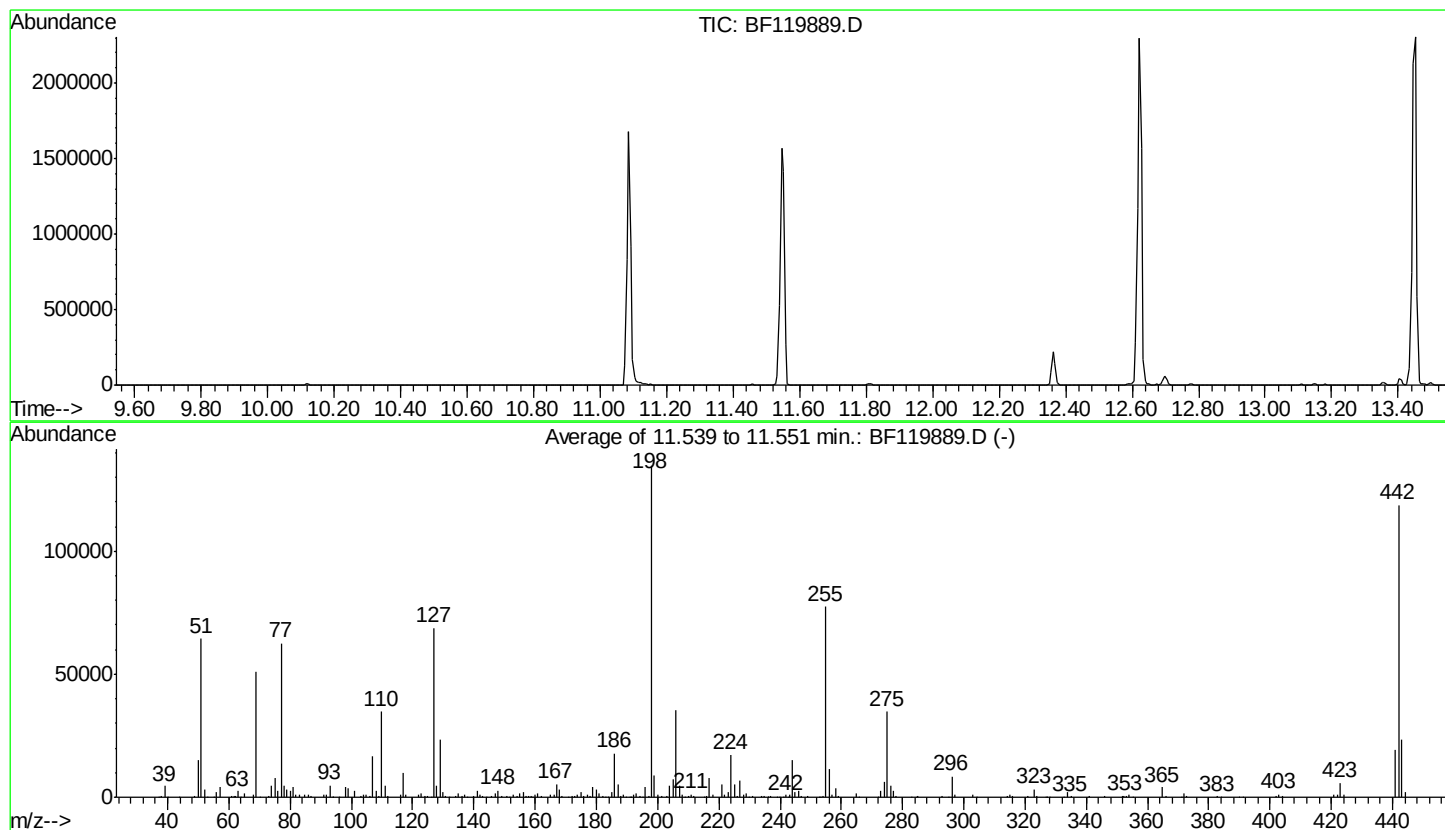

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	64357	PASS
68	69	0.00	2	1.6	831	PASS
69	198	0.00	100	37.8	50890	PASS
70	69	0.00	2	0.3	128	PASS
127	198	10	80	51.0	68685	PASS
197	198	0.00	2	0.3	349	PASS
198	198	100	100	100.0	134720	PASS
199	198	5	9	6.6	8831	PASS
275	198	10	60	25.8	34704	PASS
365	198	1	100	3.1	4136	PASS
441	198	0.01	100	14.4	19334	PASS
442	198	50	100	88.2	118802	PASS
443	442	15	24	19.8	23563	PASS