
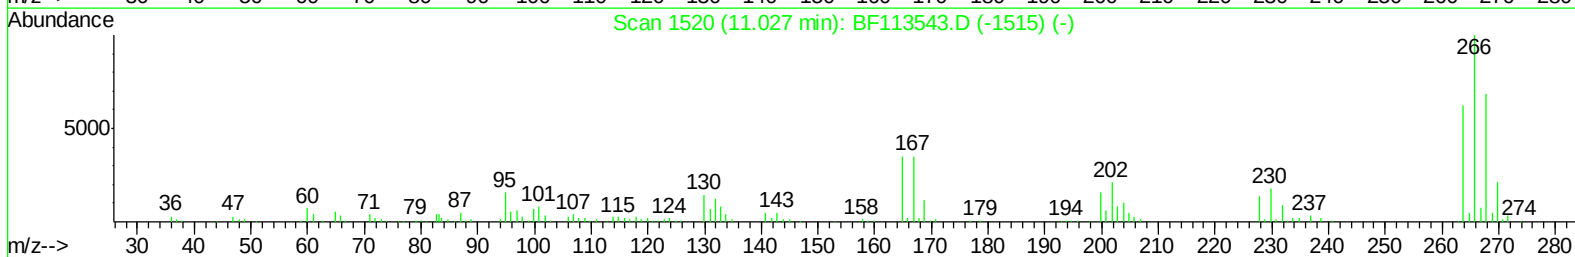
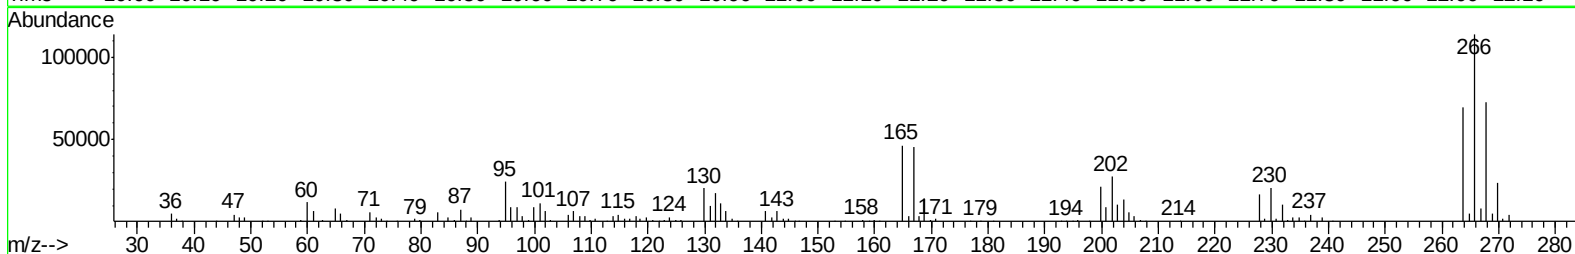


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041119\
Data File : BF113714.D
Acq On : 11 Apr 2019 11:27
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 06:52:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

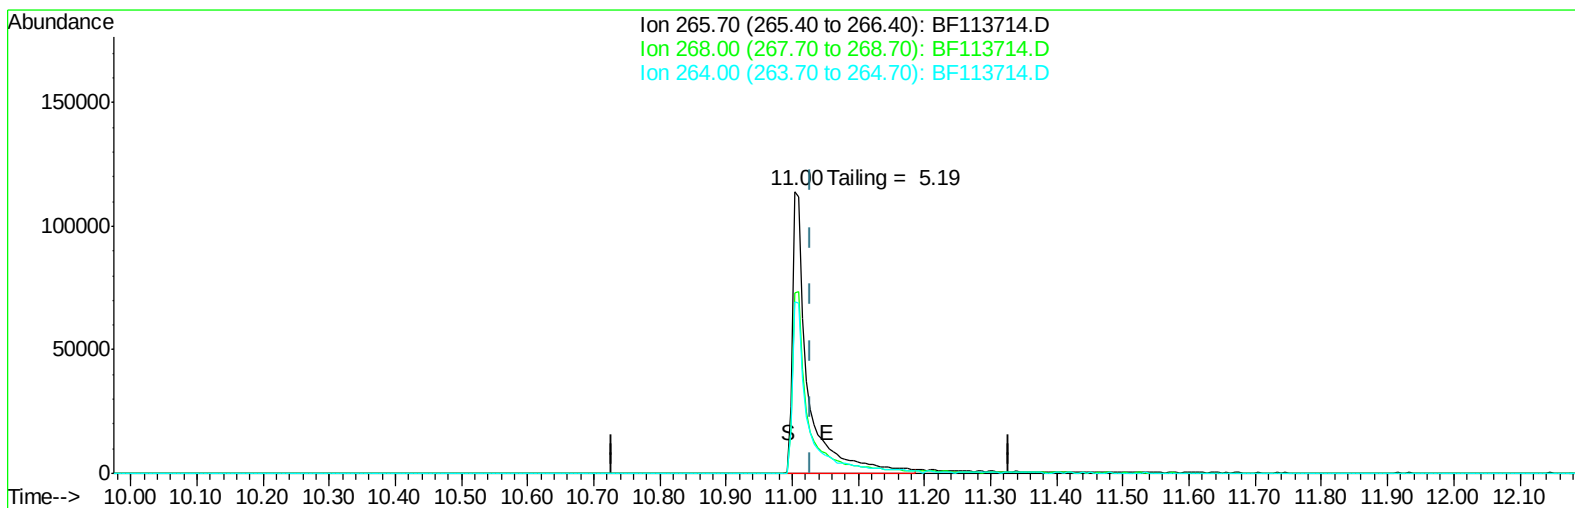

TIC: BF113714.D

(70) Pentachlorophenol (C)




11.004min (-0.024) 50290.74ng

response 188811

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	64.09
264.00	61.50	61.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041119\
 Data File : BF113714.D
 Acq On : 11 Apr 2019 11:27
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 06:52:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration

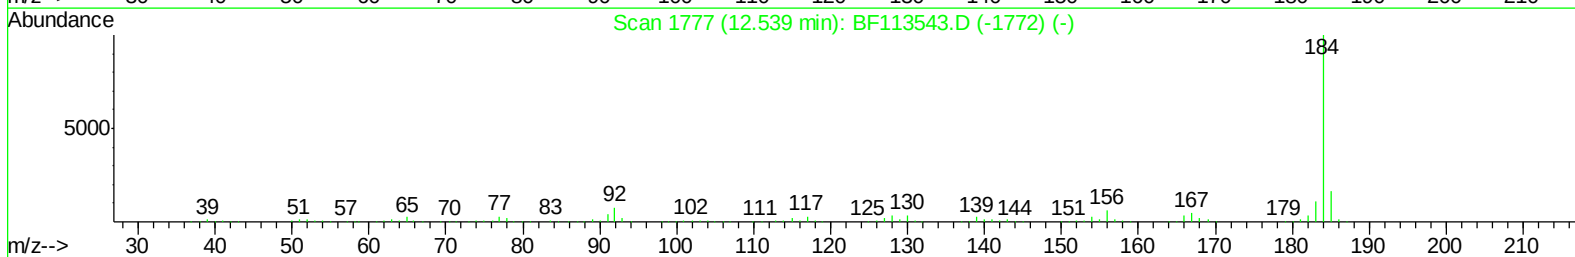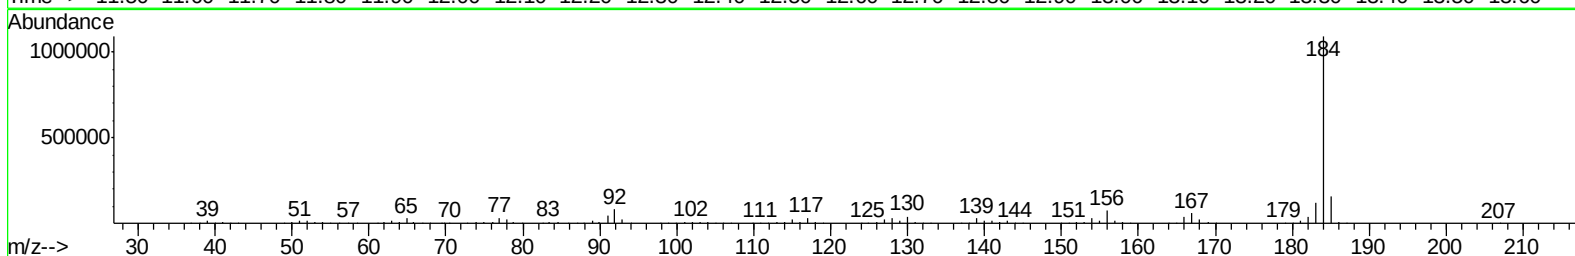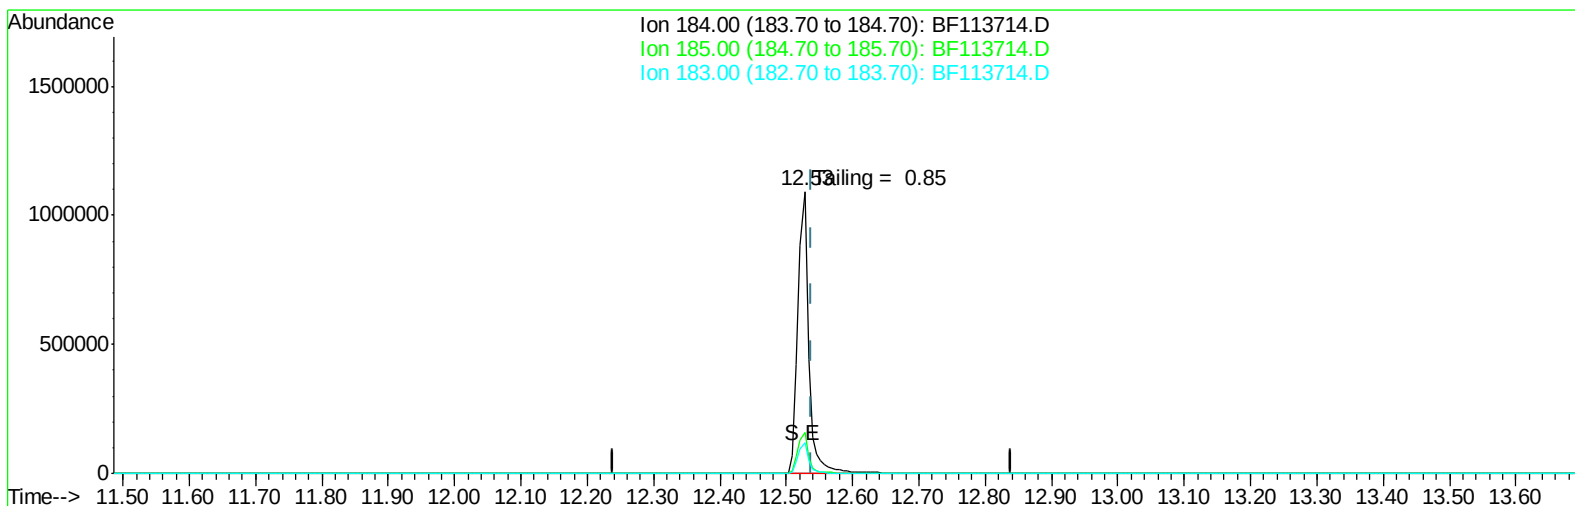

TIC: BF113714.D

(77) Benzidine

12.527min (-0.012) 142306.23ng

response 1185387

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.51
183.00	11.20	10.88
0.00	0.00	0.00