

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041119\
 Data File : BF113723.D
 Acq On : 11 Apr 2019 16:35
 Operator : JU/SJ
 Sample : K2342-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-11-S

Quant Time: Apr 12 01:54:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.67	152	120525	20.00	ng	-0.01
21) Naphthalene-d8	7.96	136	449251	20.00	ng	-0.01
39) Acenaphthene-d10	9.70	164	216972	20.00	ng	-0.02
64) Phenanthrene-d10	11.19	188	445453	20.00	ng	-0.02
76) Chrysene-d12	13.82	240	348837	20.00	ng	-0.02
87) Perylene-d12	15.23	264	330802	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	814831	115.29	ng	0.00
7) Phenol-d6	6.33	99	957264	109.89	ng	-0.01
23) Nitrobenzene-d5	7.24	82	731919	95.43	ng	-0.02
42) 2,4,6-Tribromophenol	10.50	330	369897	141.92	ng	-0.02
45) 2-Fluorobiphenyl	9.03	172	1373618	101.92	ng	-0.02
79) Terphenyl-d14	12.77	244	1532723	89.46	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041119\
Data File : BF113723.D
Acq On : 11 Apr 2019 16:35
Operator : JU/SJ
Sample : K2342-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-11-S

Quant Time: Apr 12 01:54:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

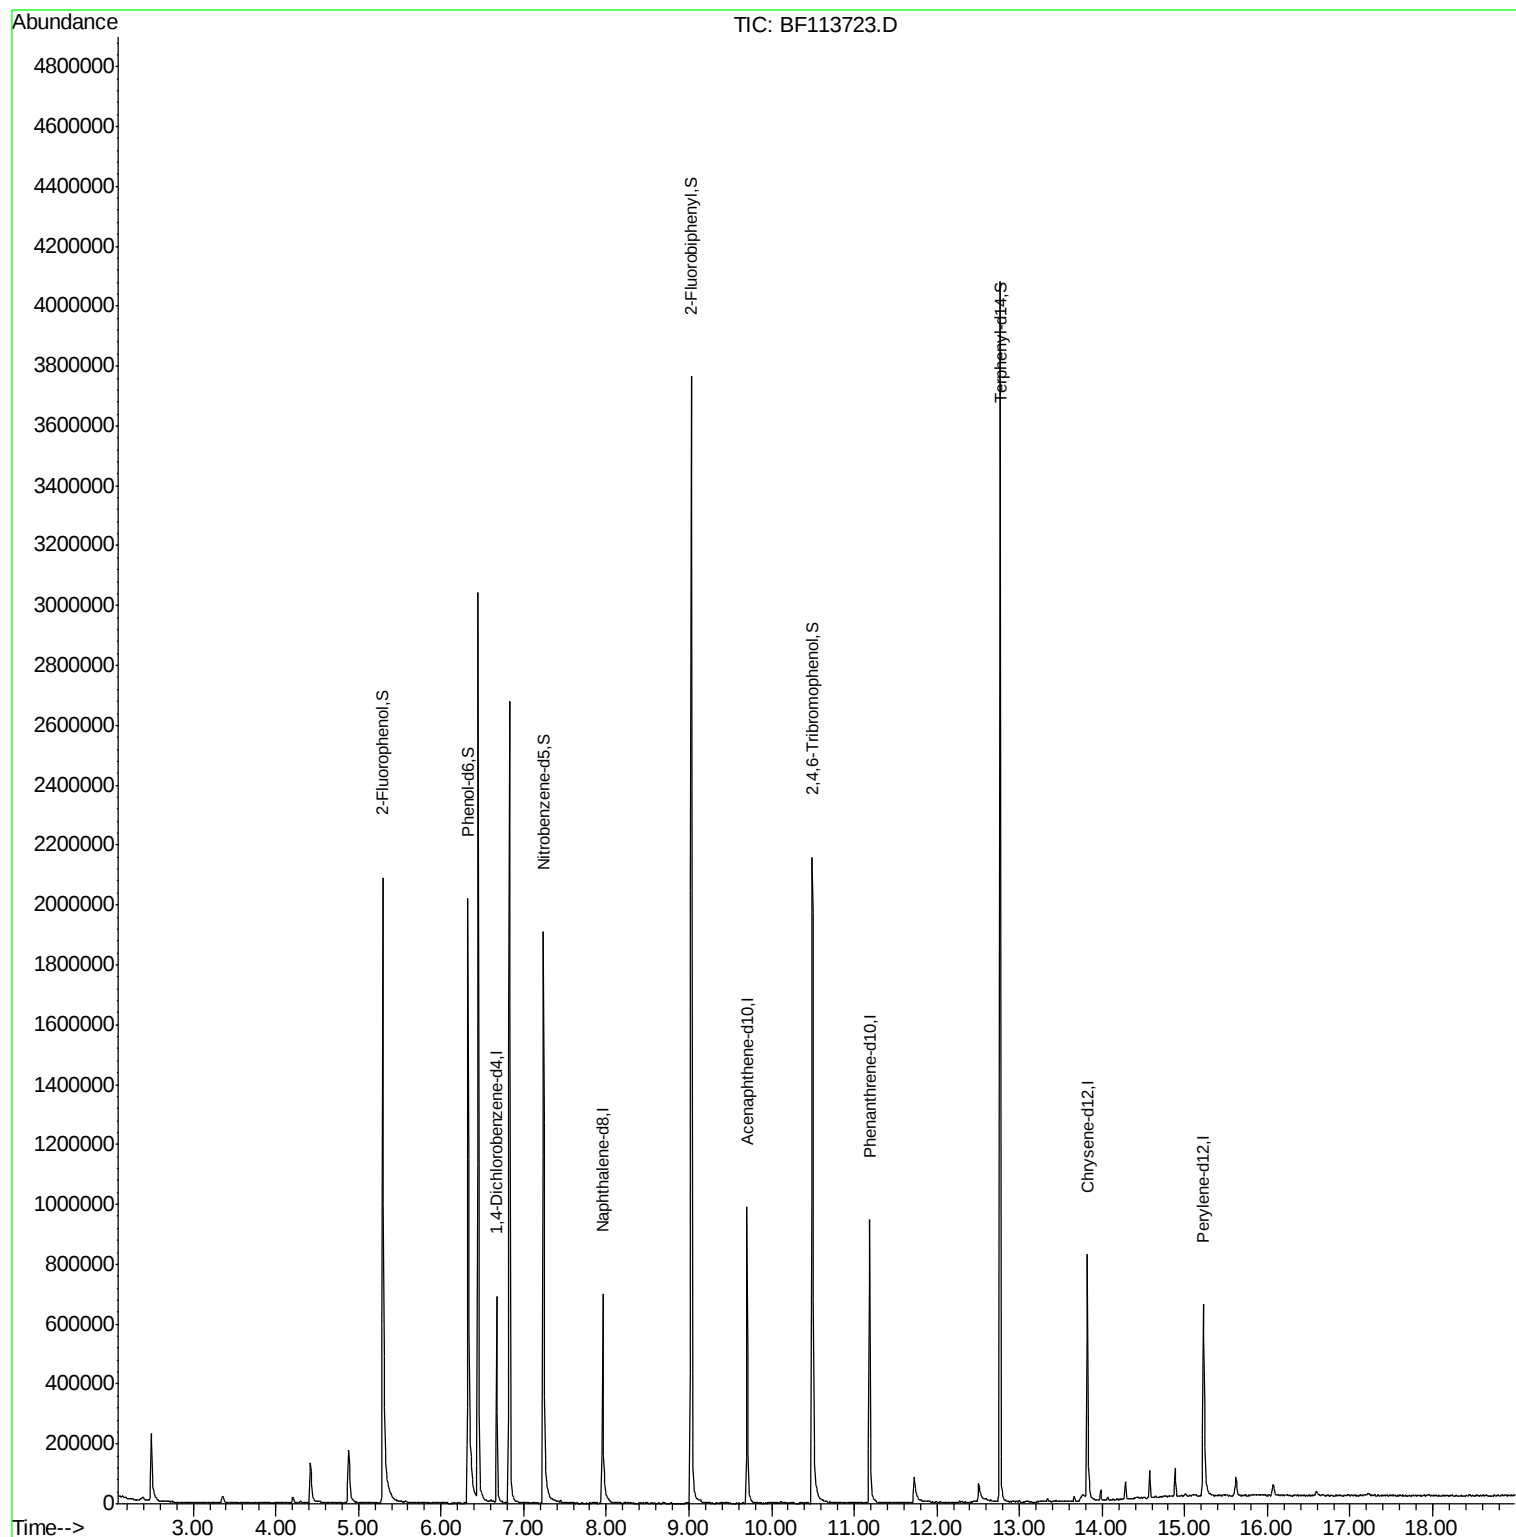




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.67 min Scan# 780
Delta R.T. -0.01 min
Lab File: BF113723.D
Acq: 11 Apr 2019 16:35

Instrument :
BNA_F
ClientSampleId :
TP-11-S

Tot Ion:152 Resp: 120525
Ion Ratio Lower Upper
152 100
150 156.0 124.7 187.1
115 56.1 46.0 69.0

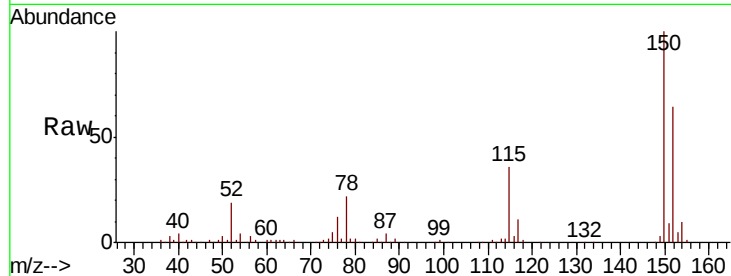


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

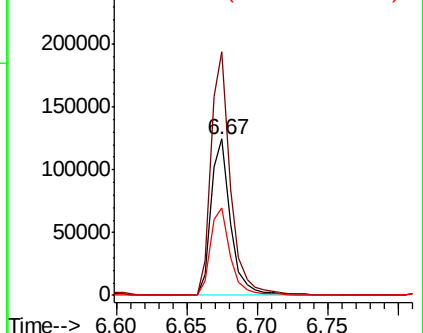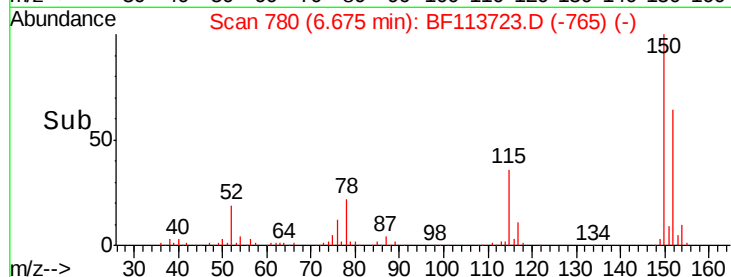



#5


2-Fluorophenol
Concen: 115.285 ng
RT: 5.30 min Scan# 546
Delta R.T. 0.00 min
Lab File: BF113723.D
Acq: 11 Apr 2019 16:35

Tgt Ion:112 Resp: 814831
Ion Ratio Lower Upper
112 100
64 57.5 49.2 73.8
63 28.9 24.9 37.3

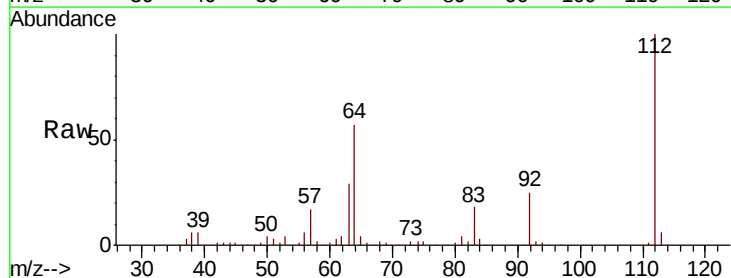

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

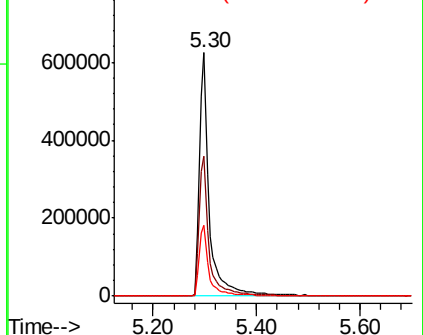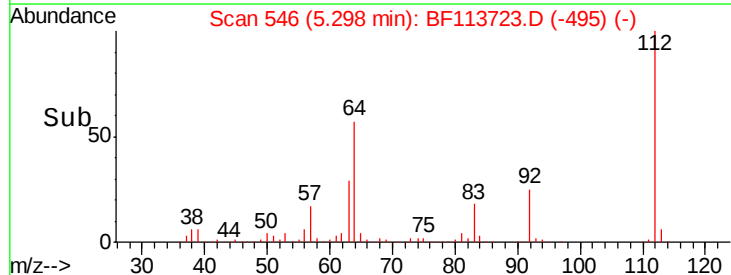

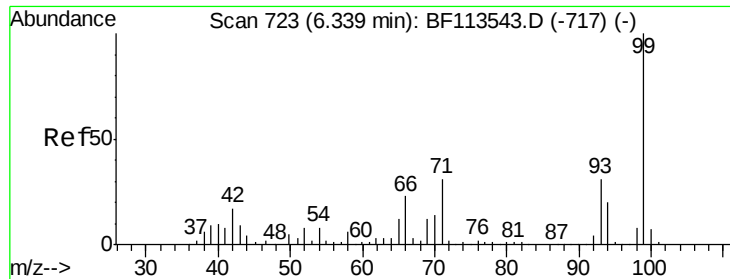

#7

Phenol-d6

Concen: 109.888 ng

RT: 6.33 min Scan# 721

Delta R.T. -0.01 min

Lab File: BF113723.D

Acq: 11 Apr 2019 16:35

Instrument :

BNA_F

ClientSampled :

TP-11-S


Tot Ion: 99 Resp: 957264

Ion Ratio Lower Upper

99 100

42 18.0 14.8 22.2




71 31.1 24.9 37.3

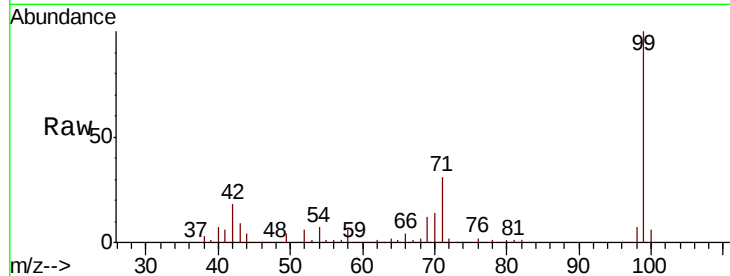

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

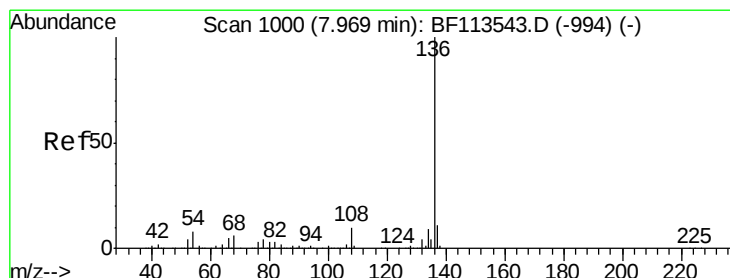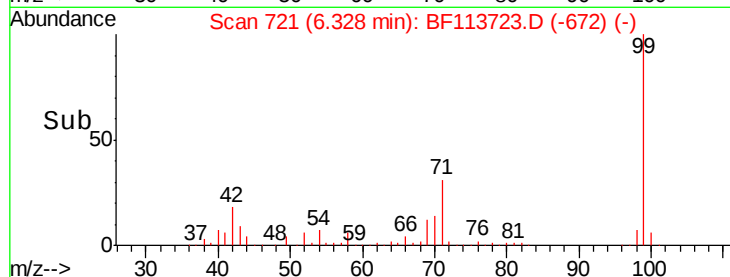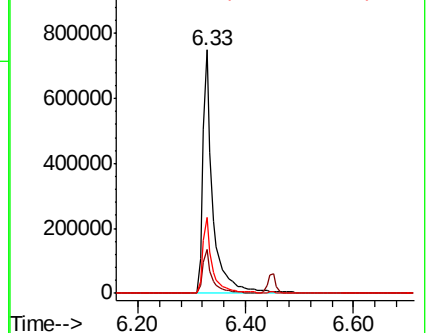

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 998

Delta R.T. -0.01 min

Lab File: BF113723.D

Acq: 11 Apr 2019 16:35

Tgt Ion: 136 Resp: 449251


Ion Ratio Lower Upper

136 100

137 10.6 8.9 13.3

54 7.3 7.0 10.6

68 5.5 4.8 7.2


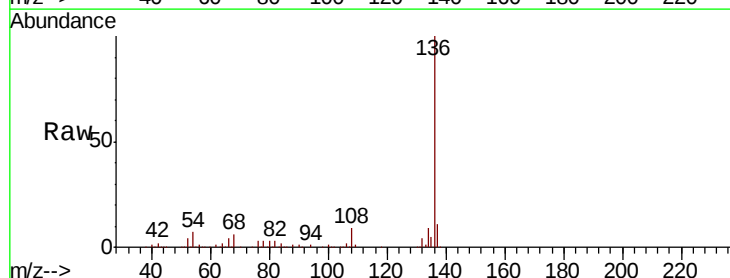


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



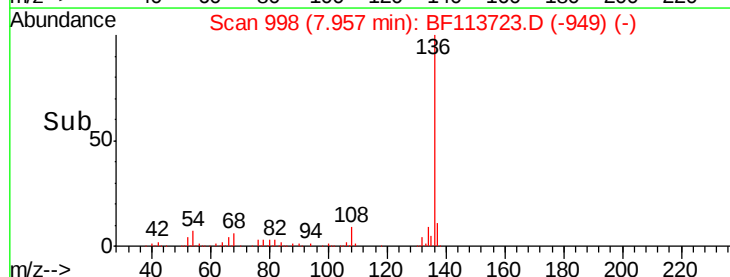
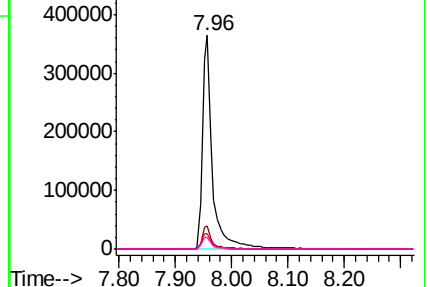




#23
Nitrobenzene-d5
Concen: 95.431 ng
RT: 7.24 min Scan# 876
Delta R.T. -0.02 min
Lab File: BF113723.D
Acq: 11 Apr 2019 16:35




Instrument :
BNA_F
ClientSampleId :
TP-11-S


Tot Ion: 82 Resp: 731919
Ion Ratio Lower Upper
82 100
128 46.5 36.5 54.7
54 52.7 42.2 63.2

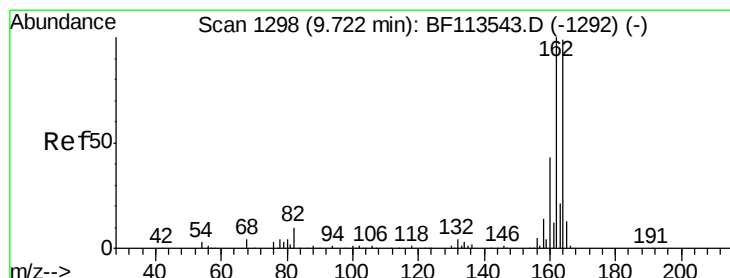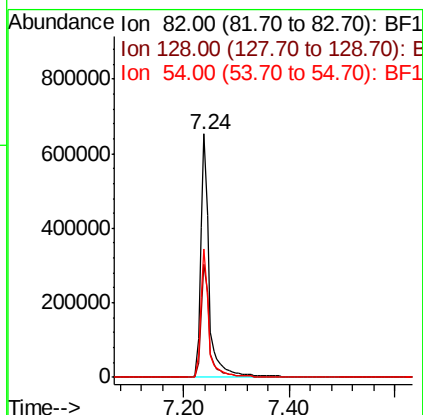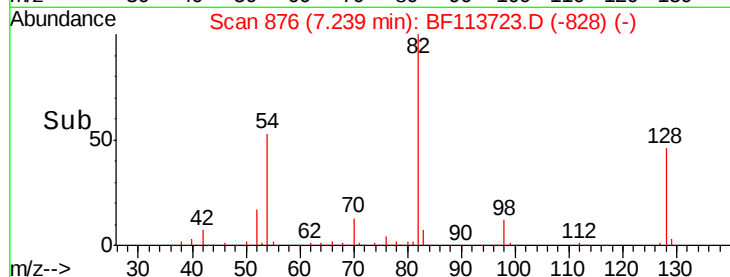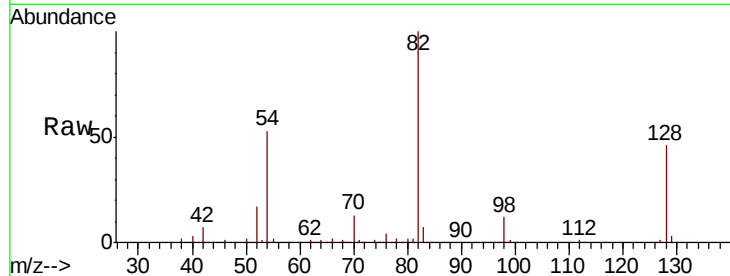

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.70 min Scan# 1295
Delta R.T. -0.02 min
Lab File: BF113723.D
Acq: 11 Apr 2019 16:35

Tgt Ion:164 Resp: 216972
Ion Ratio Lower Upper
164 100
162 100.2 81.8 122.6
160 45.2 36.4 54.6

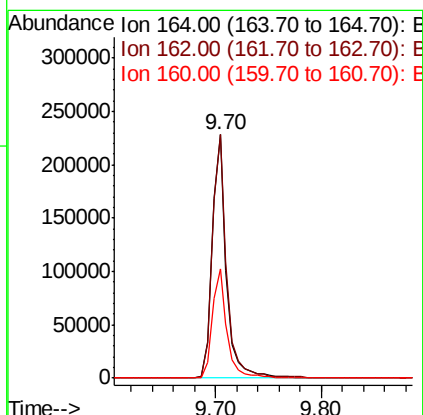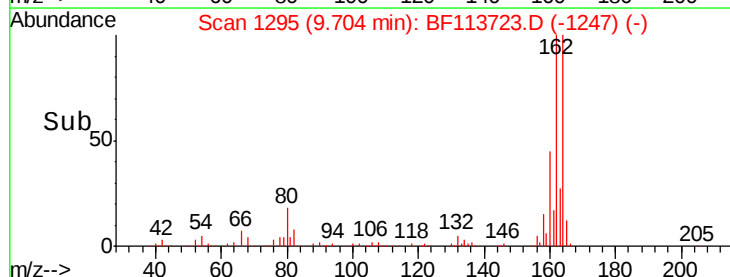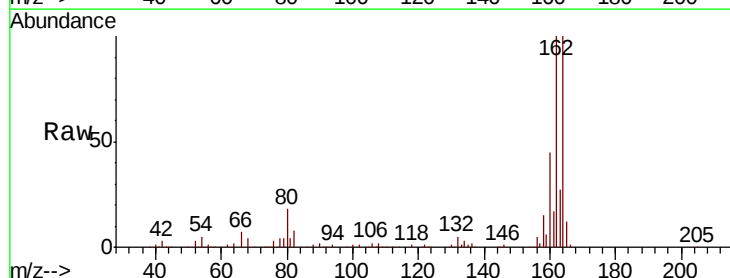


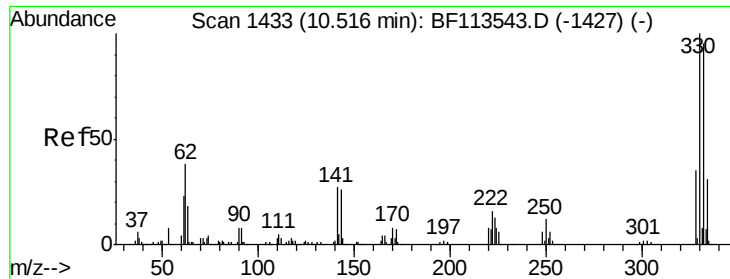

#42
 2,4,6-Tribromophenol
 Concen: 141.921 ng
 RT: 10.50 min Scan# 1430
 Delta R.T. -0.02 min
 Lab File: BF113723.D
 Acq: 11 Apr 2019 16:35

Instrument :
 BNA_F
 ClientSampleId :
 TP-11-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	77.8	116.6
141	28.0	22.7	34.1



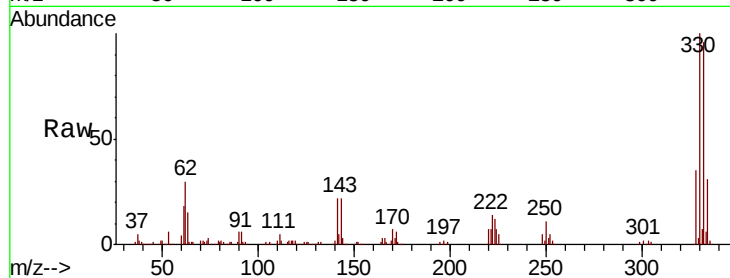


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

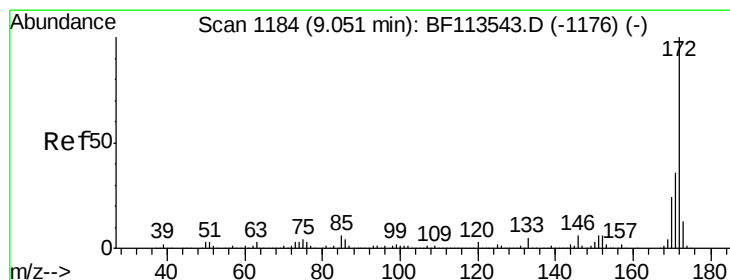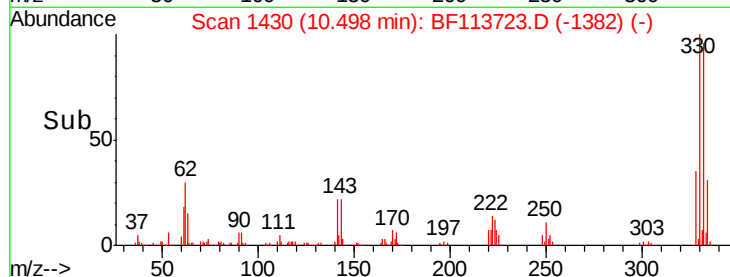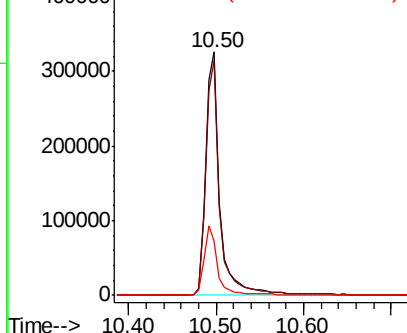

#45
 2-Fluorobiphenyl
 Concen: 101.920 ng
 RT: 9.03 min Scan# 1180
 Delta R.T. -0.02 min
 Lab File: BF113723.D
 Acq: 11 Apr 2019 16:35

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	29.0	43.6
170	24.5	19.5	29.3


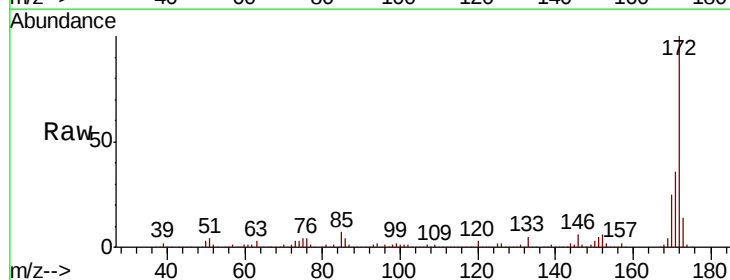



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



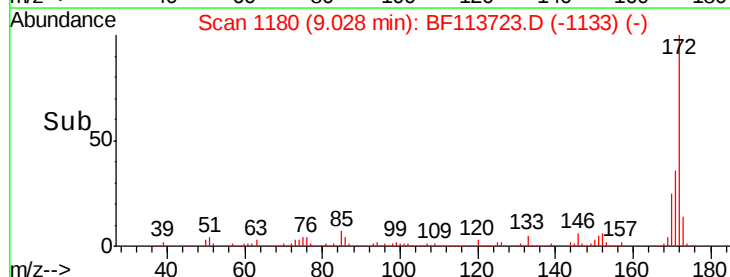
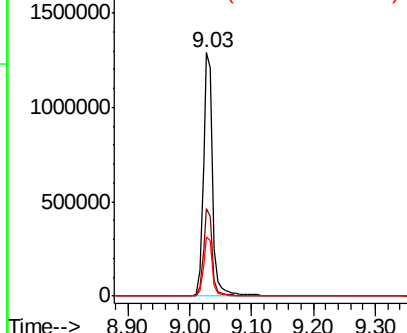


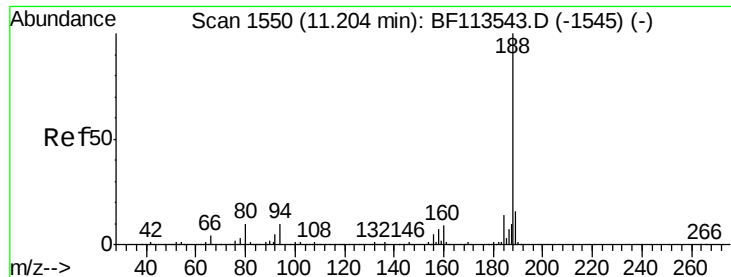

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.19 min Scan# 1547
Delta R.T. -0.02 min
Lab File: BF113723.D
Acq: 11 Apr 2019 16:35




Instrument :
BNA_F
ClientSampleId :
TP-11-S


Tot Ion:188 Resp: 445453
Ion Ratio Lower Upper
188 100
94 8.6 7.0 10.6
80 8.8 7.7 11.5

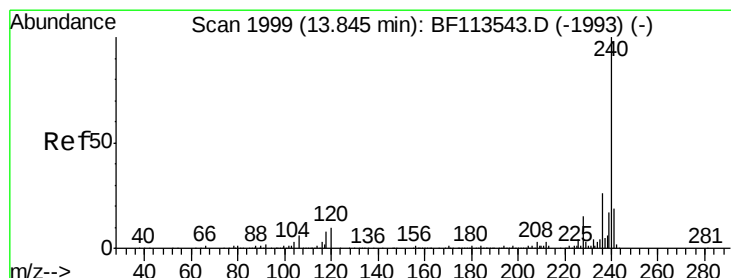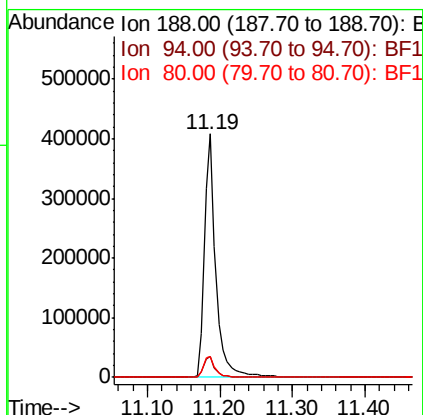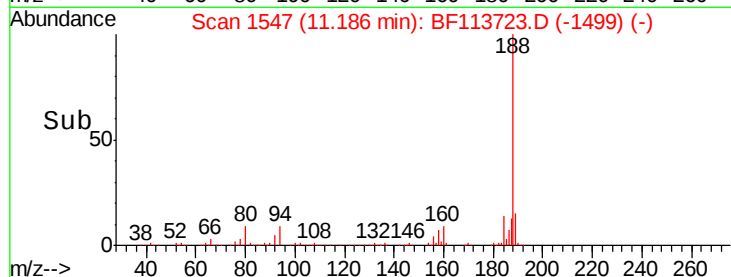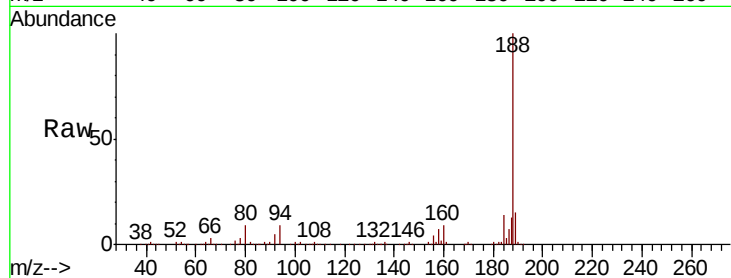

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.82 min Scan# 1995
Delta R.T. -0.02 min
Lab File: BF113723.D
Acq: 11 Apr 2019 16:35

Tgt Ion:240 Resp: 348837
Ion Ratio Lower Upper
240 100
120 10.1 8.8 13.2
236 25.8 20.9 31.3


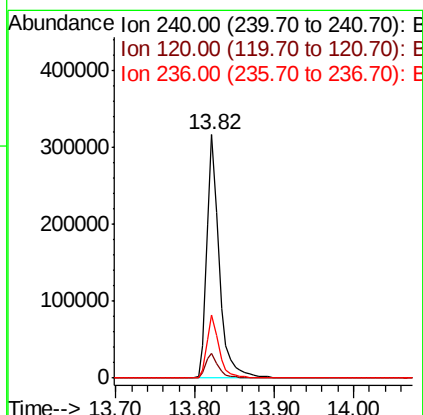
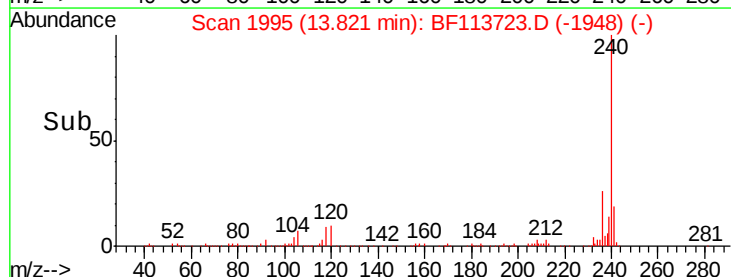
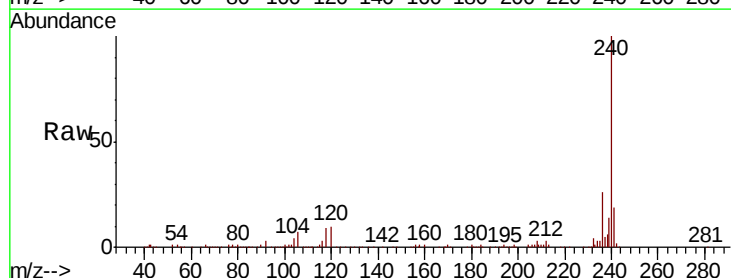


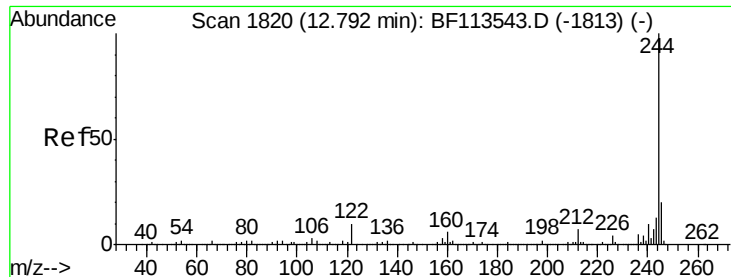

#79
 Terphenyl-d14
 Concen: 89.459 ng
 RT: 12.77 min Scan# 1816
 Delta R.T. -0.02 min
 Lab File: BF113723.D
 Acq: 11 Apr 2019 16:35

Instrument :
 BNA_F
 ClientSampleId :
 TP-11-S

Tot Ion:244 Resp: 1532723
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.5 8.3
 122 10.7 8.6 13.0

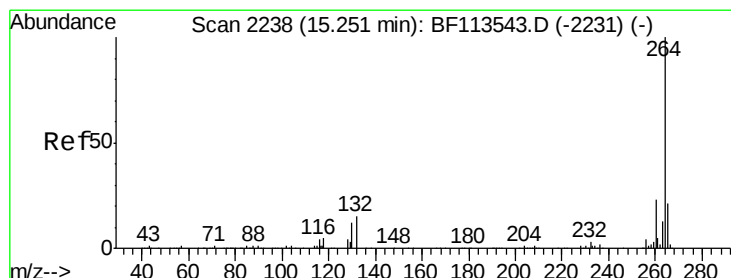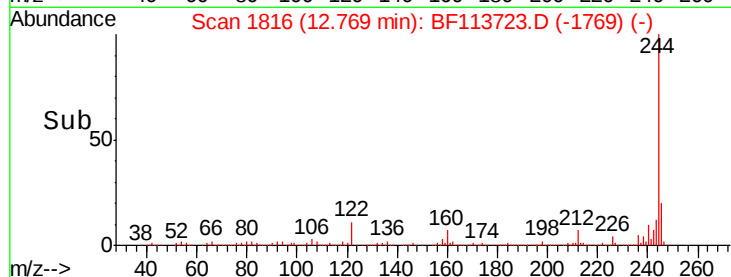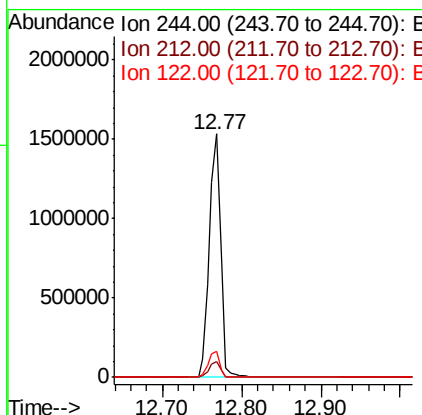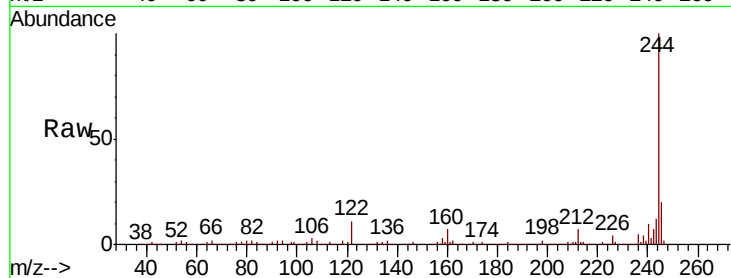

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.23 min Scan# 2234
 Delta R.T. -0.02 min
 Lab File: BF113723.D
 Acq: 11 Apr 2019 16:35

Tgt Ion:264 Resp: 330802
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.1 28.7
 265 21.3 17.1 25.7

