

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041219\
 Data File : BF113741.D
 Acq On : 12 Apr 2019 16:31
 Operator : JU/SJ
 Sample : K2355-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 12 23:00:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.67	152	105346	20.00	ng	-0.01
21) Naphthalene-d8	7.96	136	405646	20.00	ng	-0.01
39) Acenaphthene-d10	9.70	164	195967	20.00	ng	-0.02
64) Phenanthrene-d10	11.19	188	398584	20.00	ng	-0.02
76) Chrysene-d12	13.82	240	300652	20.00	ng	-0.02
87) Perylene-d12	15.23	264	319782	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	656942	106.34	ng	0.00
7) Phenol-d6	6.33	99	742464	97.51	ng	-0.01
23) Nitrobenzene-d5	7.24	82	584361	84.38	ng	-0.02
42) 2,4,6-Tribromophenol	10.50	330	302548	128.52	ng	-0.02
45) 2-Fluorobiphenyl	9.03	172	1090062	89.55	ng	-0.02
79) Terphenyl-d14	12.77	244	1217179	82.43	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.24	70	74087	15.779	ng	# 77
25) Isophorone	7.24	82	584358	43.803	ng	# 64
50) Dimethylphthalate	9.70	163	44130	3.055	ng	# 1
51) 2,6-Dinitrotoluene	9.70	165	24572	7.717	ng	# 25
57) 2,4-Dinitrotoluene	9.70	165	24572	6.381	ng	# 22
67) 4-Bromophenyl-phenylether	10.50	248	16832	3.765	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041219\
Data File : BF113741.D
Acq On : 12 Apr 2019 16:31
Operator : JU/SJ
Sample : K2355-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 12 23:00:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

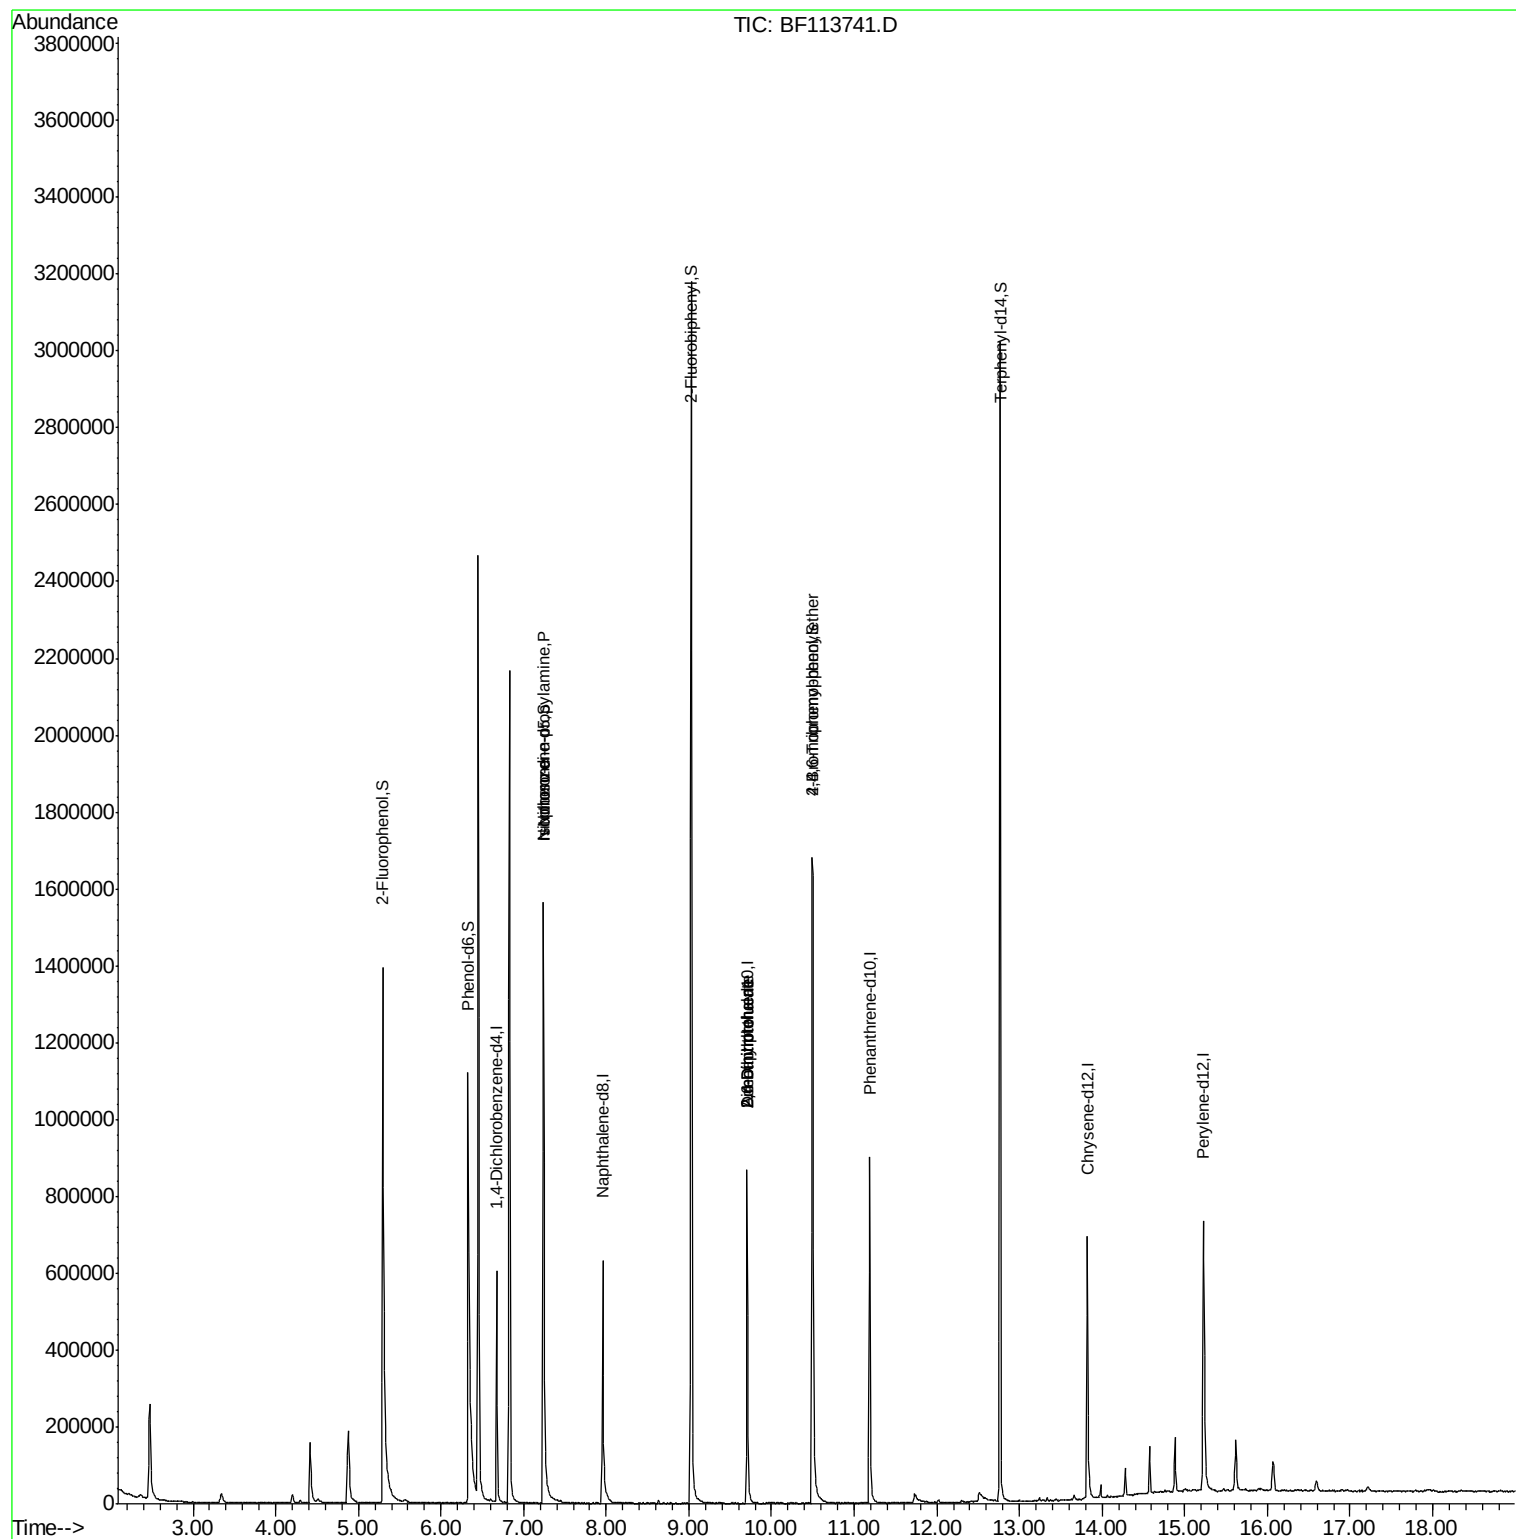




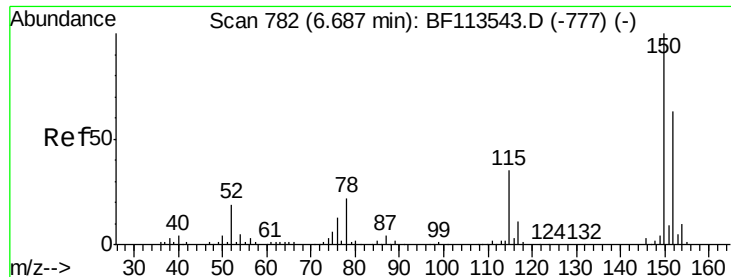


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.67 min Scan# 780
Delta R.T. -0.01 min
Lab File: BF113741.D
Acq: 12 Apr 2019 16:31

Instrument :
BNA_F
ClientSampleId :




Tot Ion:152 Resp: 105346
Ion Ratio Lower Upper
152 100
150 156.2 124.7 187.1
115 53.5 46.0 69.0

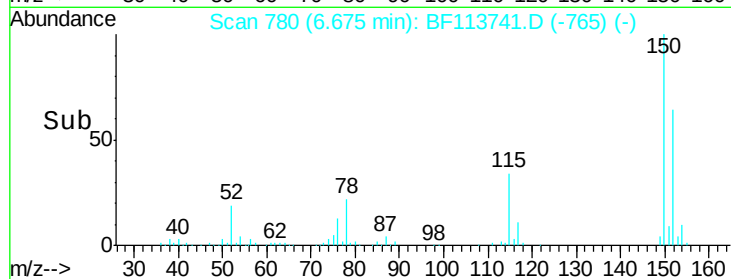
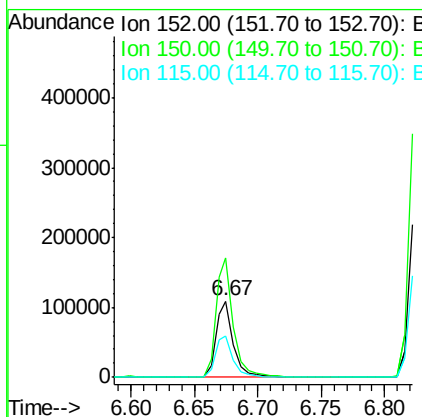
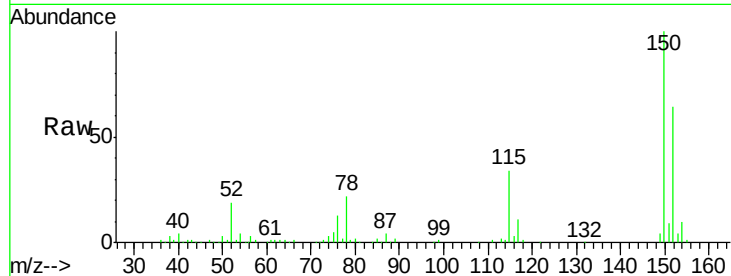


#5

2-Fluorophenol
Concen: 106.339 ng
RT: 5.30 min Scan# 546
Delta R.T. 0.00 min
Lab File: BF113741.D
Acq: 12 Apr 2019 16:31

Tgt Ion:112 Resp: 656942
Ion Ratio Lower Upper
112 100
64 56.5 49.2 73.8
63 28.6 24.9 37.3

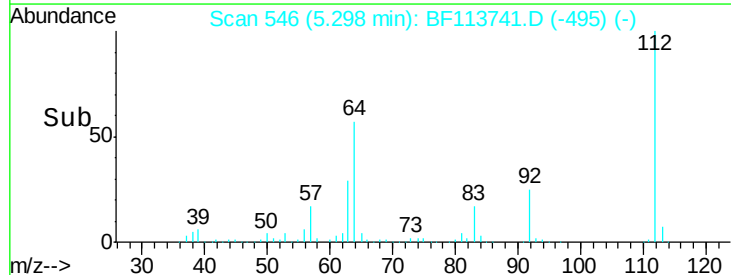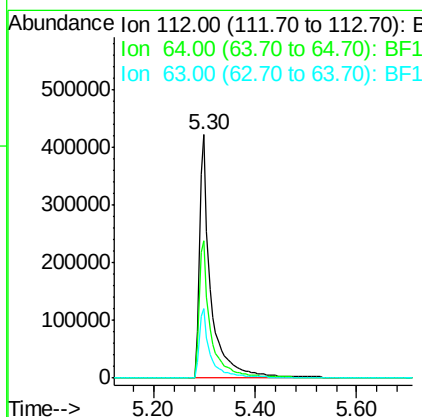

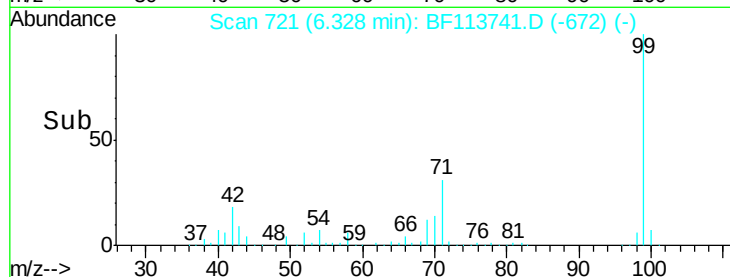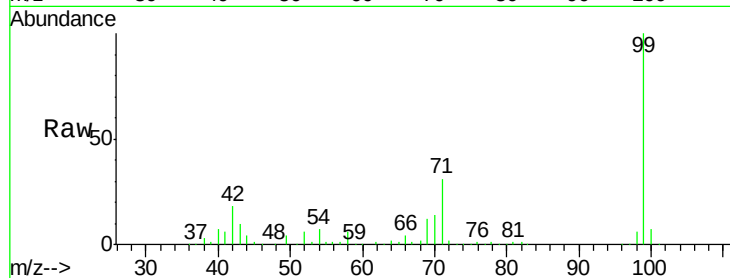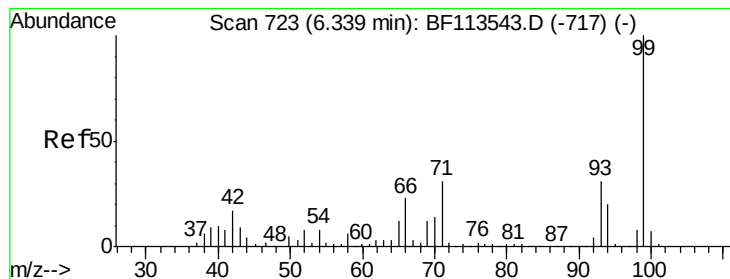

#7

Phenol-d6

Concen: 97.510 ng

RT: 6.33 min Scan# 721

Delta R.T. -0.01 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31

Instrument :

BNA_F

ClientSampled :





Tot Ion: 99 Resp: 742464

Ion Ratio Lower Upper

99 100

42 18.3 14.8 22.2

71 30.9 24.9 37.3

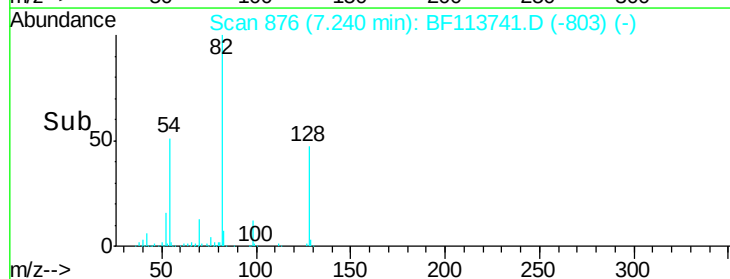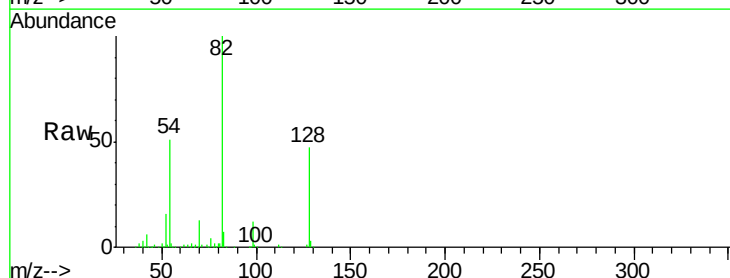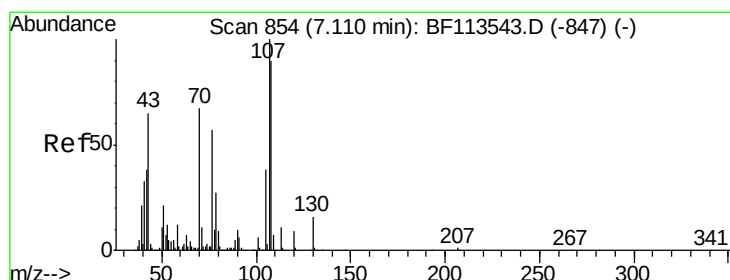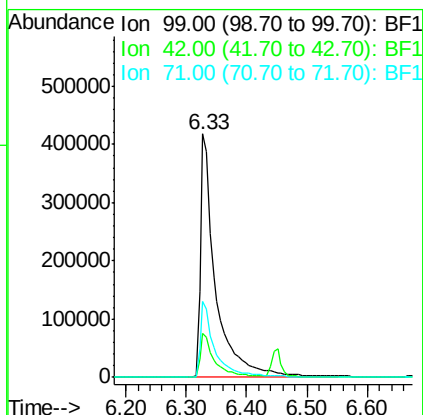

#19

n-Nitroso-di-n-propylamine

Concen: 15.779 ng

RT: 7.24 min Scan# 876

Delta R.T. 0.13 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31

Tgt Ion: 70 Resp: 74087


Ion Ratio Lower Upper


70 100

42 49.3 48.4 72.6

101 0.0 7.8 11.8#

130 2.8 18.2 27.4#

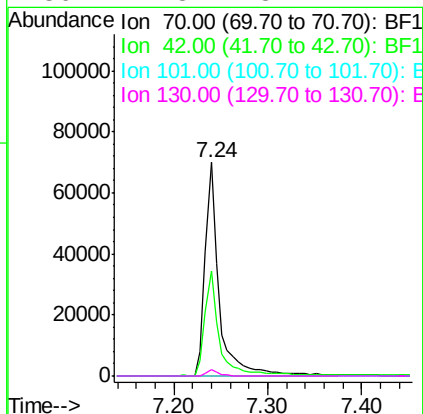


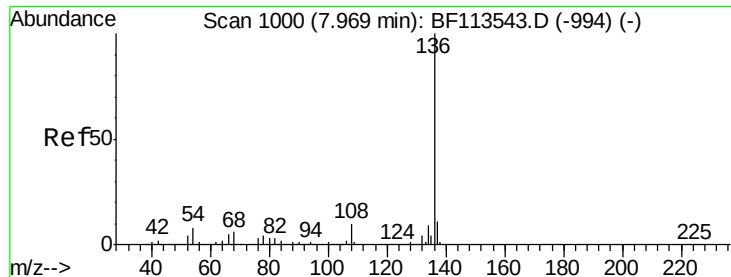




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.96 min Scan# 998
Delta R.T. -0.01 min
Lab File: BF113741.D
Acq: 12 Apr 2019 16:31

Instrument :
BNA_F
ClientSampled :

Tot Ion:136	Resp:	405646
Ion Ratio	Lower	Upper
136	100	
137	10.7	8.9 13.3
54	7.4	7.0 10.6
68	5.8	4.8 7.2

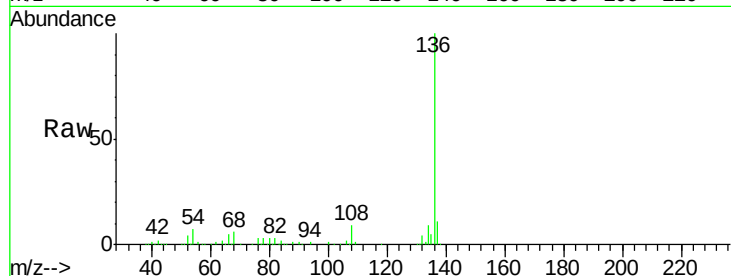


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

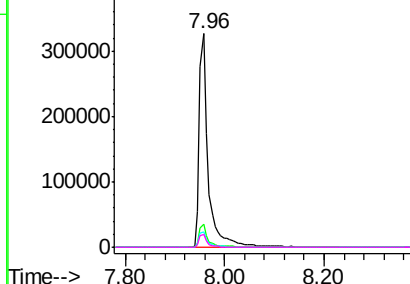
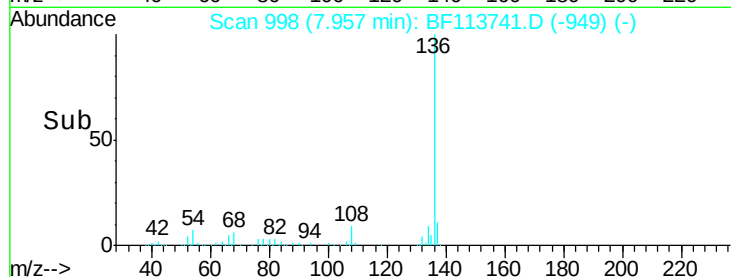



#23
Nitrobenzene-d5
Concen: 84.382 ng
RT: 7.24 min Scan# 876
Delta R.T. -0.02 min
Lab File: BF113741.D
Acq: 12 Apr 2019 16:31

Tgt Ion: 82	Resp:	584361
Ion Ratio	Lower	Upper
82	100	
128	46.6	36.5 54.7
54	51.4	42.2 63.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

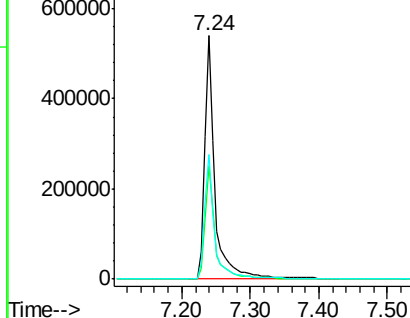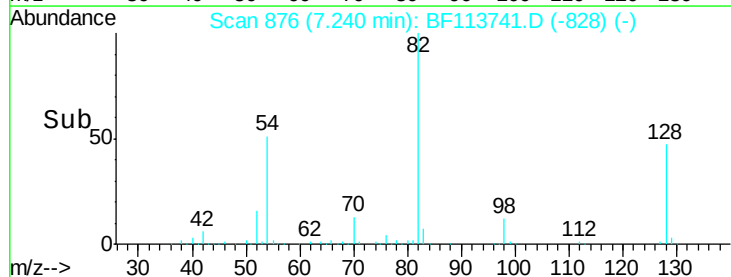

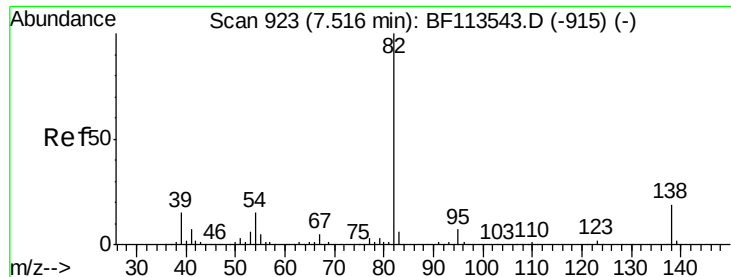

#25

Isophorone

Concen: 43.803 ng

RT: 7.24 min Scan# 876

Delta R.T. -0.28 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 584358

Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#




138 0.0 15.2 22.8#

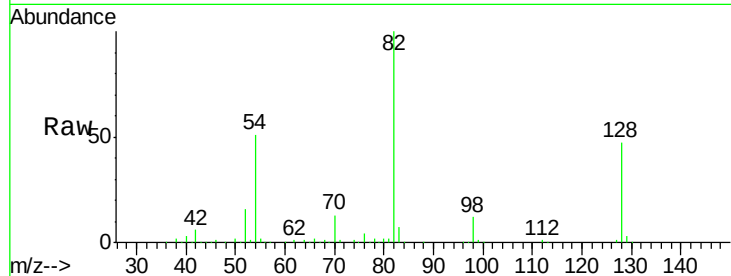

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

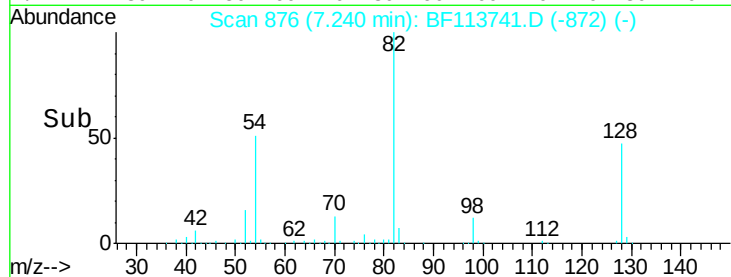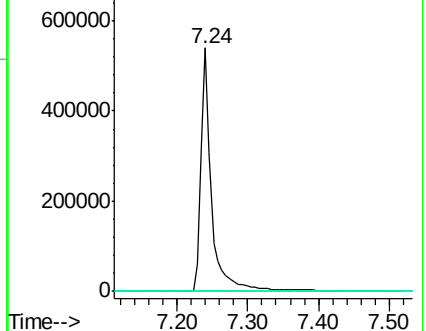

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.70 min Scan# 1295

Delta R.T. -0.02 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31


Tgt Ion:164 Resp: 195967

Ion Ratio Lower Upper

164 100

162 100.6 81.8 122.6



160 45.0 36.4 54.6

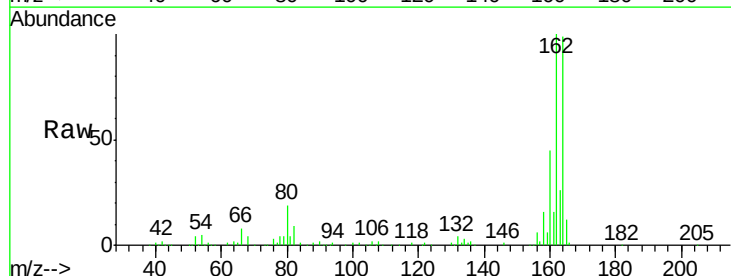


Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1



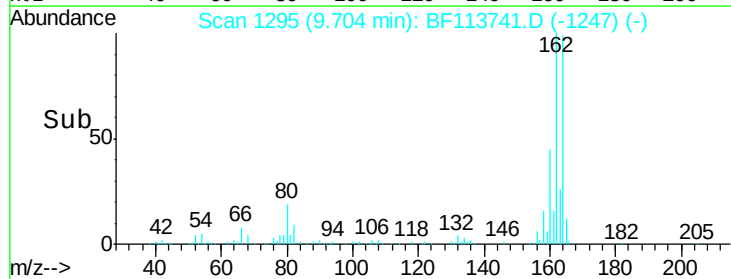
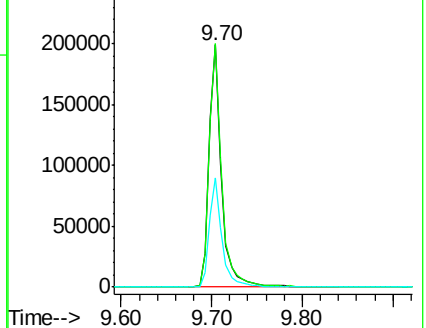


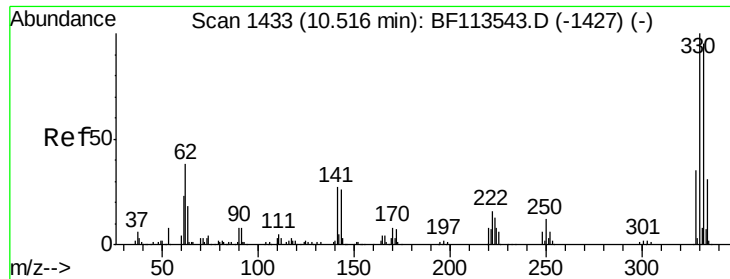

#42
 2,4,6-Tribromophenol
 Concen: 128.523 ng
 RT: 10.50 min Scan# 1430
 Delta R.T. -0.02 min
 Lab File: BF113741.D
 Acq: 12 Apr 2019 16:31




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	77.8	116.6
141	27.5	22.7	34.1

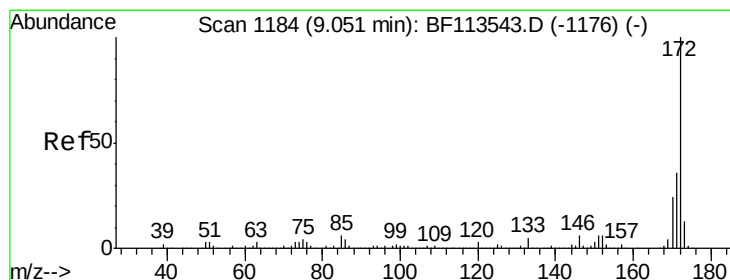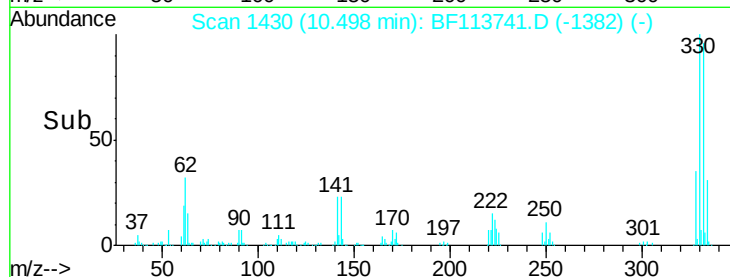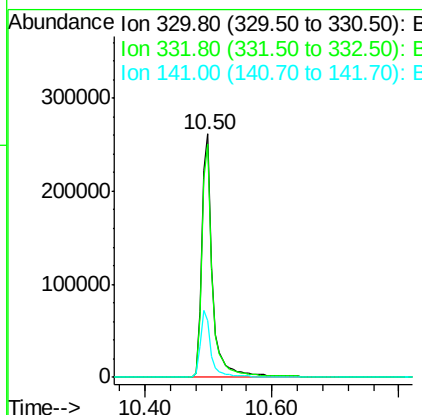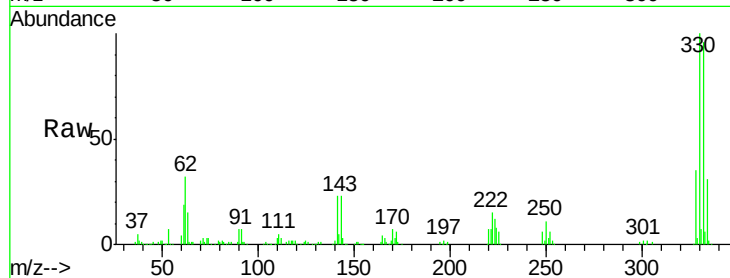

#45
 2-Fluorobiphenyl
 Concen: 89.550 ng
 RT: 9.03 min Scan# 1180
 Delta R.T. -0.02 min
 Lab File: BF113741.D
 Acq: 12 Apr 2019 16:31

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	29.0	43.6
170	24.2	19.5	29.3

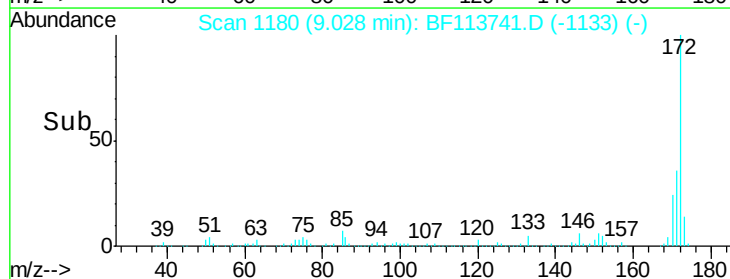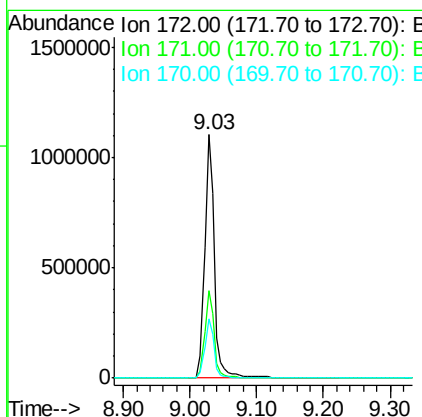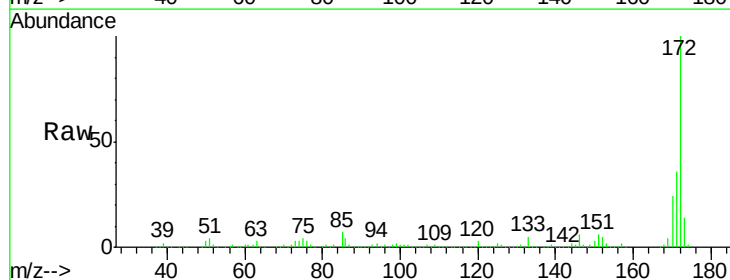

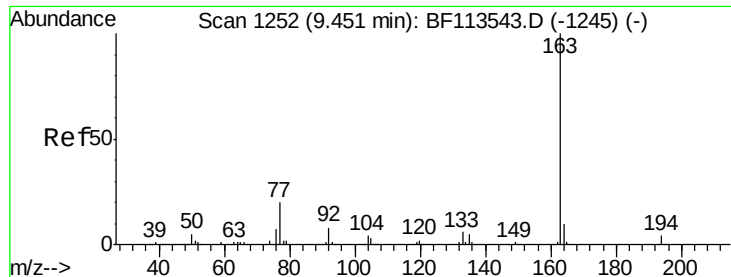

#50

Dimethylphthalate

Concen: 3.055 ng

RT: 9.70 min Scan# 1295

Delta R.T. 0.25 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31

Instrument :

BNA_F

ClientSampled :


Tot Ion:163 Resp: 44130

Ion Ratio Lower Upper




163 100

194 0.0 3.0 4.6#

164 384.1 8.1 12.1#

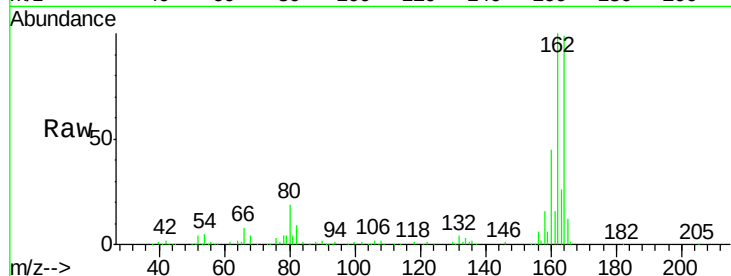

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

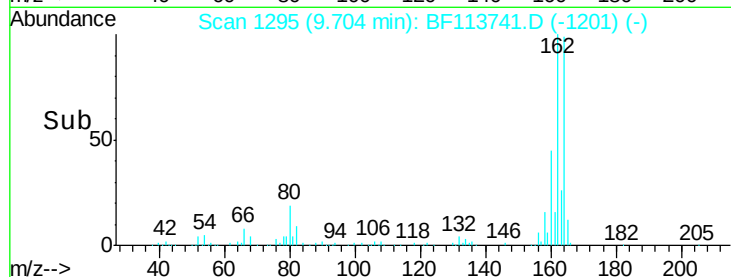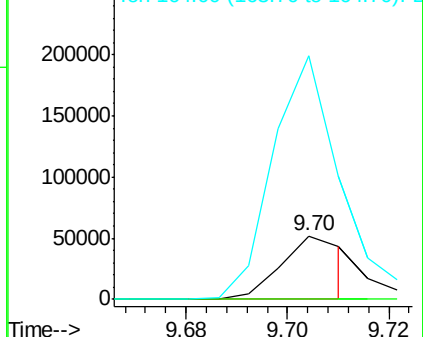

#51

2,6-Dinitrotoluene

Concen: 7.717 ng

RT: 9.70 min Scan# 1295

Delta R.T. 0.19 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31


Tgt Ion:165 Resp: 24572

Ion Ratio Lower Upper



165 100


63 0.0 43.4 65.0#

89 0.0 43.1 64.7#



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

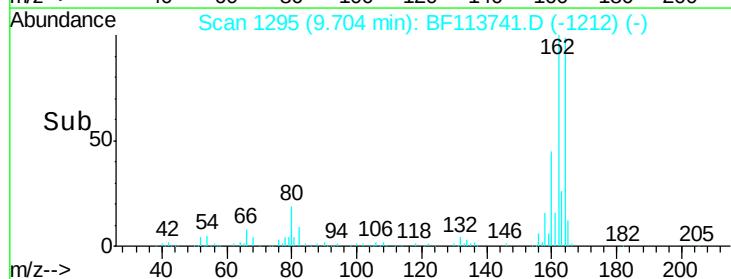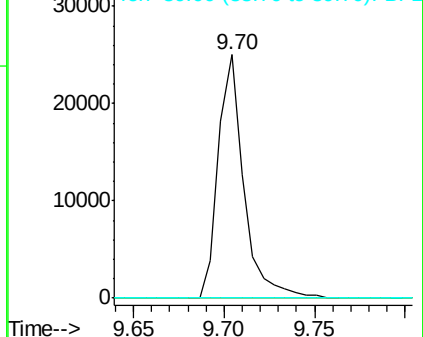

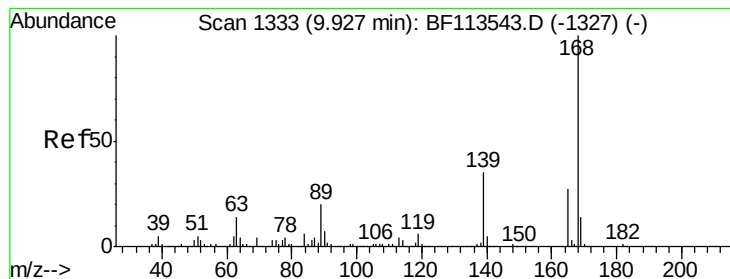

#57

2,4-Dinitrotoluene

Concen: 6.381 ng

RT: 9.70 min Scan# 1295

Delta R.T. -0.22 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31

Instrument :

BNA_F

ClientSampleId :

Tot Ion:165 Resp: 24572


Ion Ratio Lower Upper

165 100

63 0.0 37.5 56.3#

89 0.0 57.4 86.2#

182 1.2 2.0 3.0#



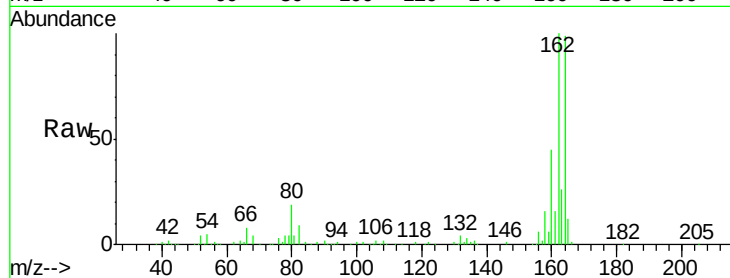


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

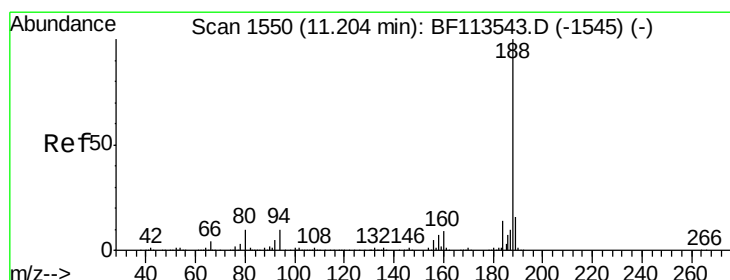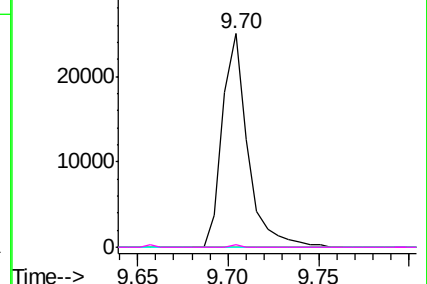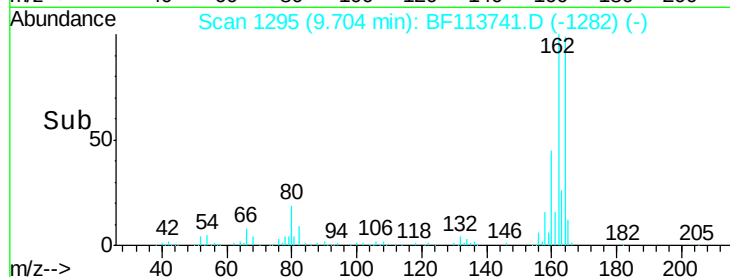

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.19 min Scan# 1547

Delta R.T. -0.02 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31


Tgt Ion:188 Resp: 398584

Ion Ratio Lower Upper

188 100

94 8.4 7.0 10.6



80 8.9 7.7 11.5

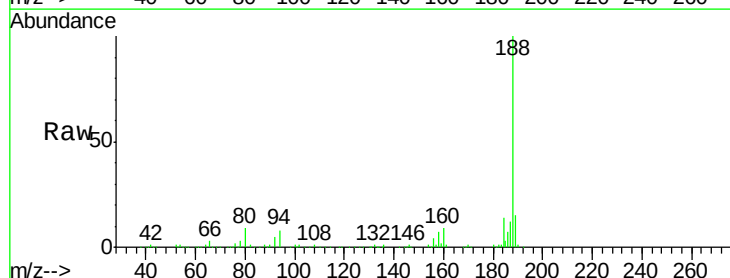


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

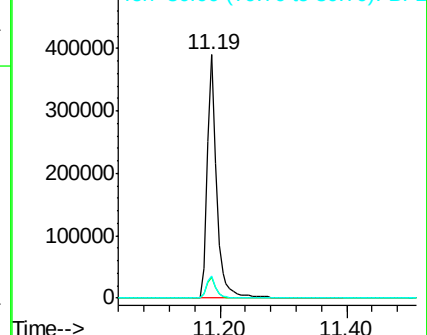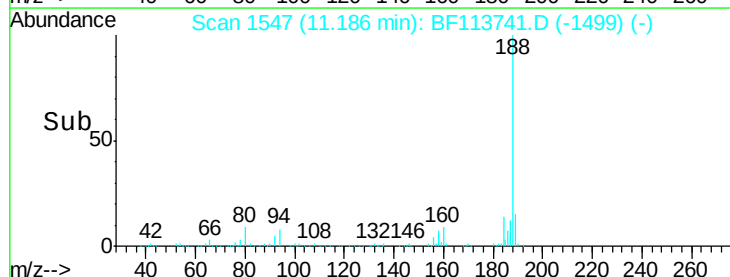


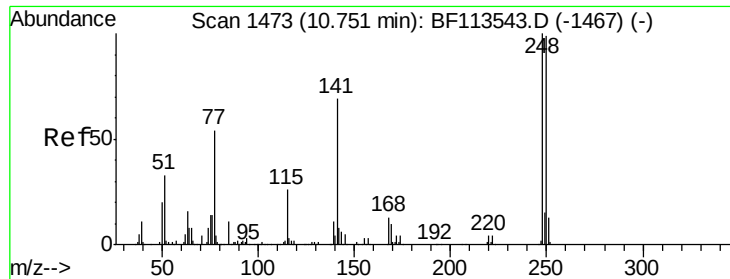




#67
4-Bromophenyl-phenylether
Concen: 3.765 ng
RT: 10.50 min Scan# 1430
Delta R.T. -0.25 min
Lab File: BF113741.D
Acq: 12 Apr 2019 16:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 16832
Ion Ratio Lower Upper
248 100
250 193.2 78.3 117.5#
141 406.7 56.2 84.4#

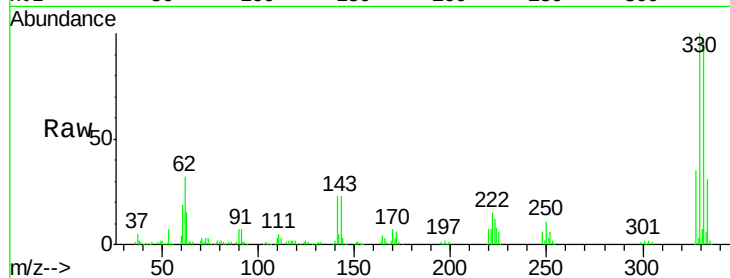


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

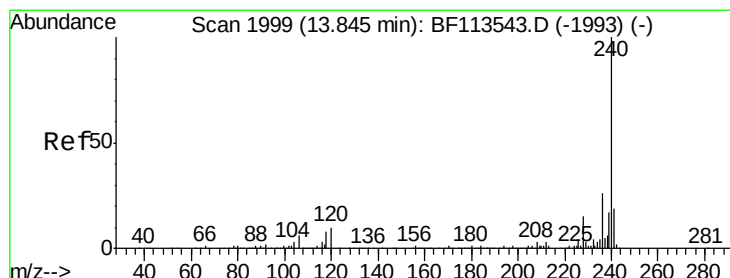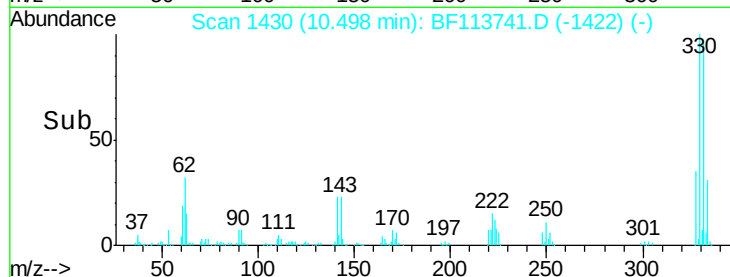
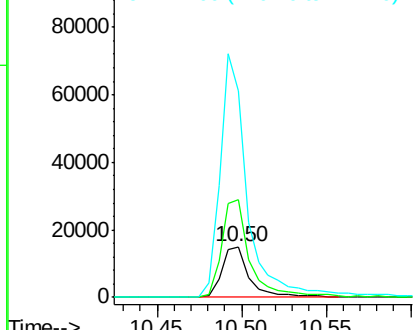



#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.82 min Scan# 1995
Delta R.T. -0.02 min
Lab File: BF113741.D
Acq: 12 Apr 2019 16:31

Tgt Ion:240 Resp: 300652
Ion Ratio Lower Upper
240 100
120 10.0 8.8 13.2
236 24.9 20.9 31.3

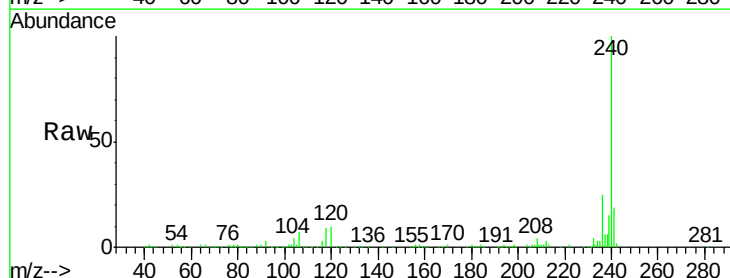

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

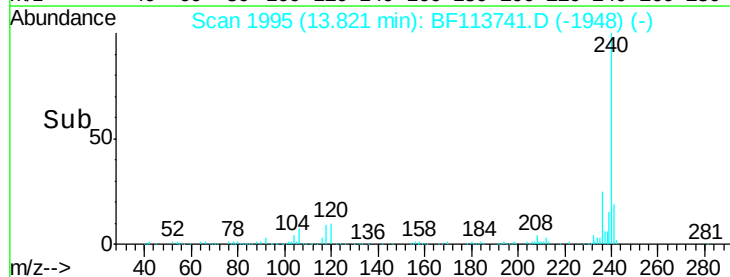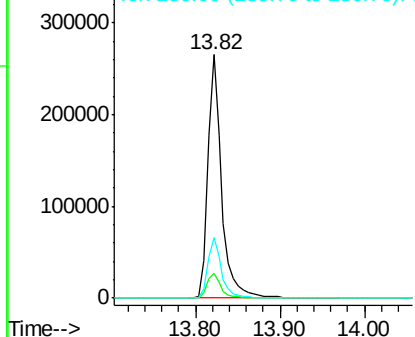

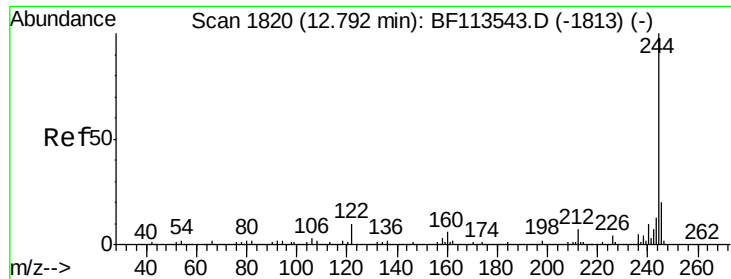

#79

Terphenyl-d14

Concen: 82.427 ng

RT: 12.77 min Scan# 1816

Delta R.T. -0.02 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 1217179

Ion Ratio Lower Upper

244 100

212 6.5 5.5 8.3




122 9.8 8.6 13.0



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

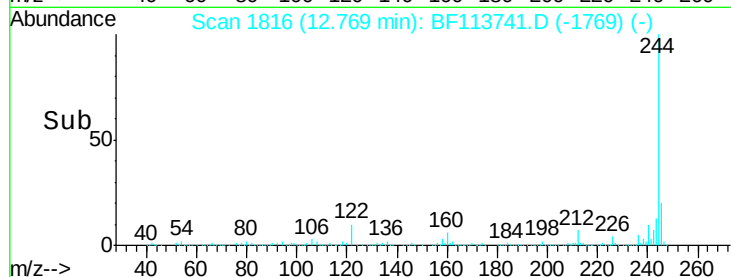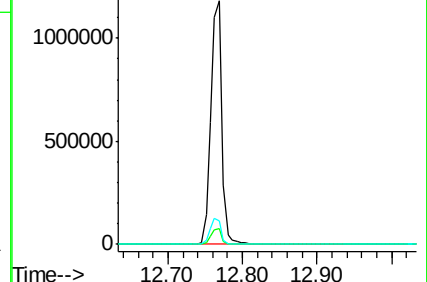

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.23 min Scan# 2234

Delta R.T. -0.02 min

Lab File: BF113741.D

Acq: 12 Apr 2019 16:31


Tgt Ion:264 Resp: 319782

Ion Ratio Lower Upper

264 100

260 22.9 19.1 28.7

265 20.6 17.1 25.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

