
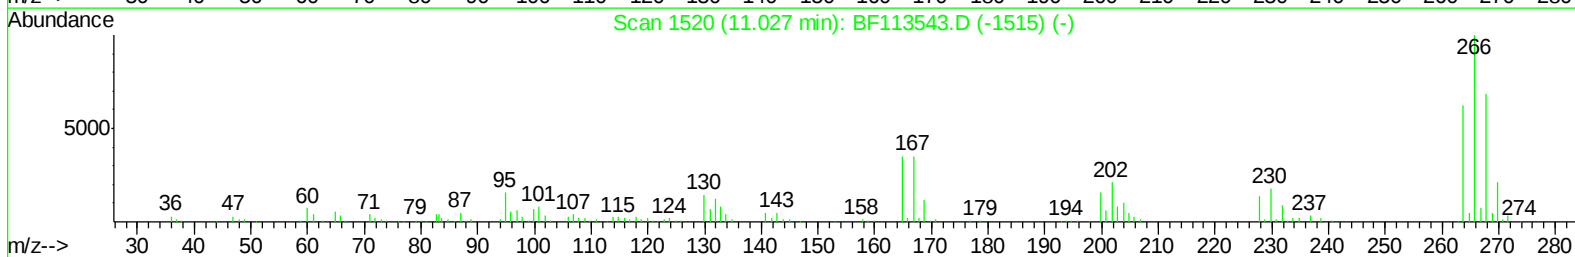
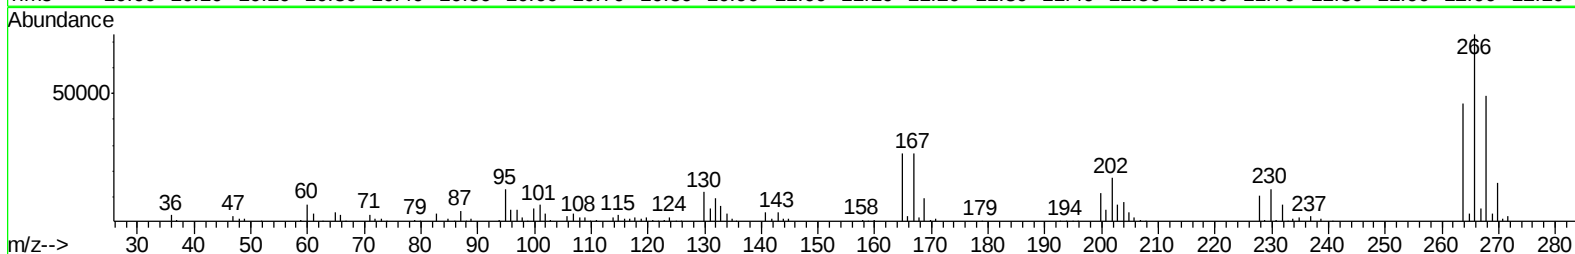


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041219\  
Data File : BF113736.D  
Acq On : 12 Apr 2019 13:47  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 05:35:03 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF040319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 04 04:05:31 2019  
Response via : Initial Calibration

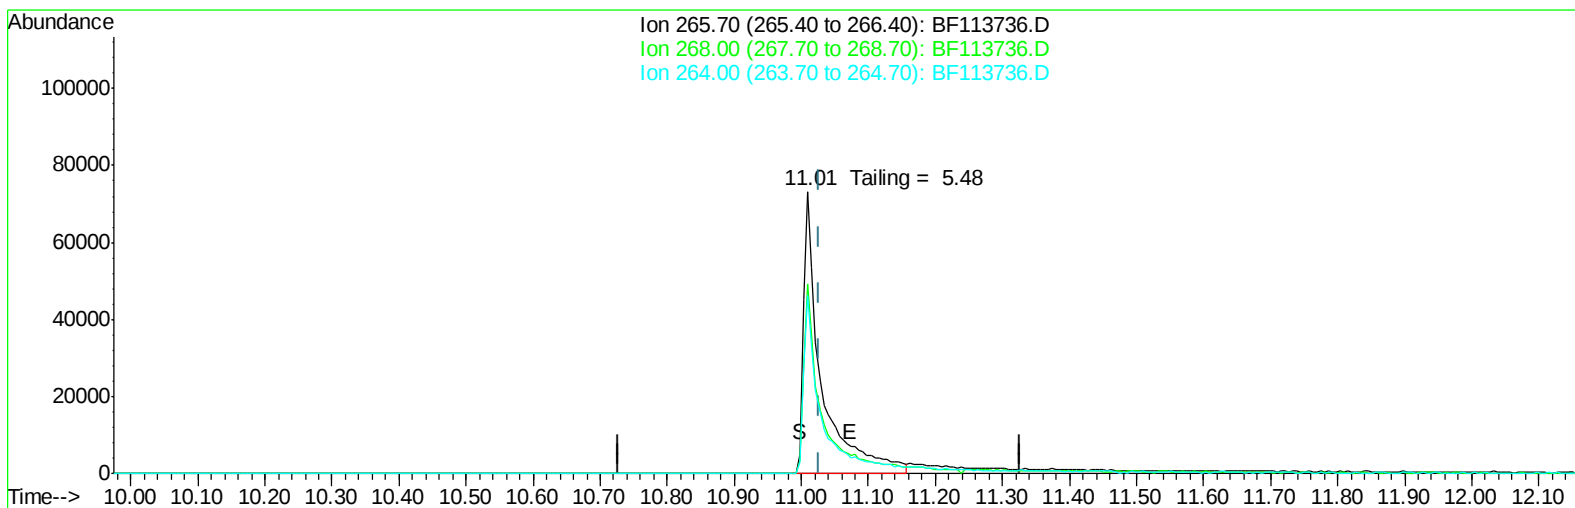

TIC: BF113736.D

(70) Pentachlorophenol (C)




11.010min (-0.018) 46787.84ng

response 135428

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 67.20 | 67.16 |
| 264.00 | 61.50 | 63.03 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF041219\  
Data File : BF113736.D  
Acq On : 12 Apr 2019 13:47  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 05:35:03 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF040319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 04 04:05:31 2019  
Response via : Initial Calibration

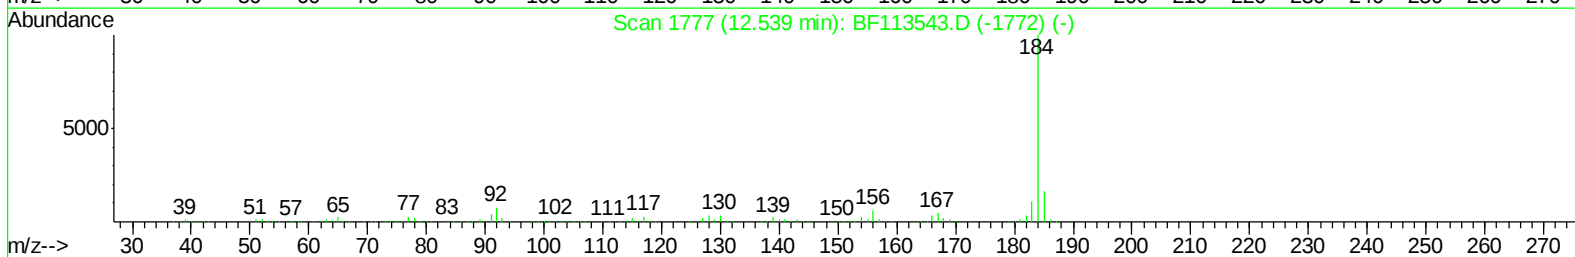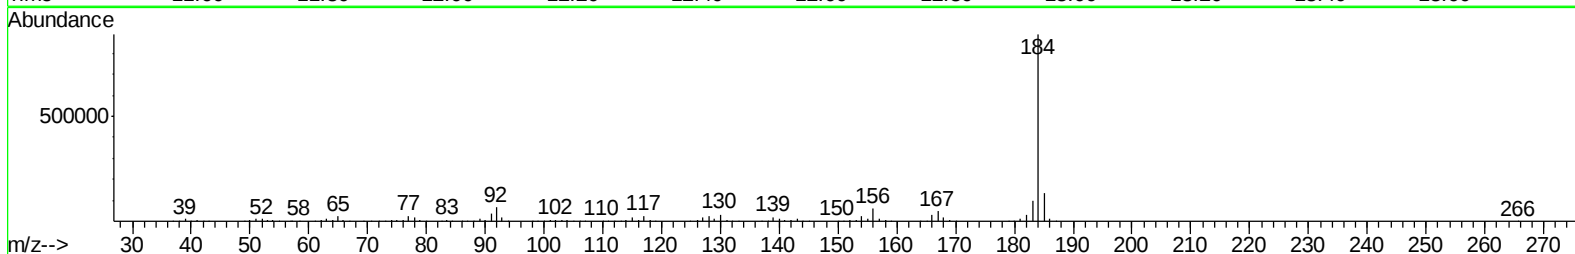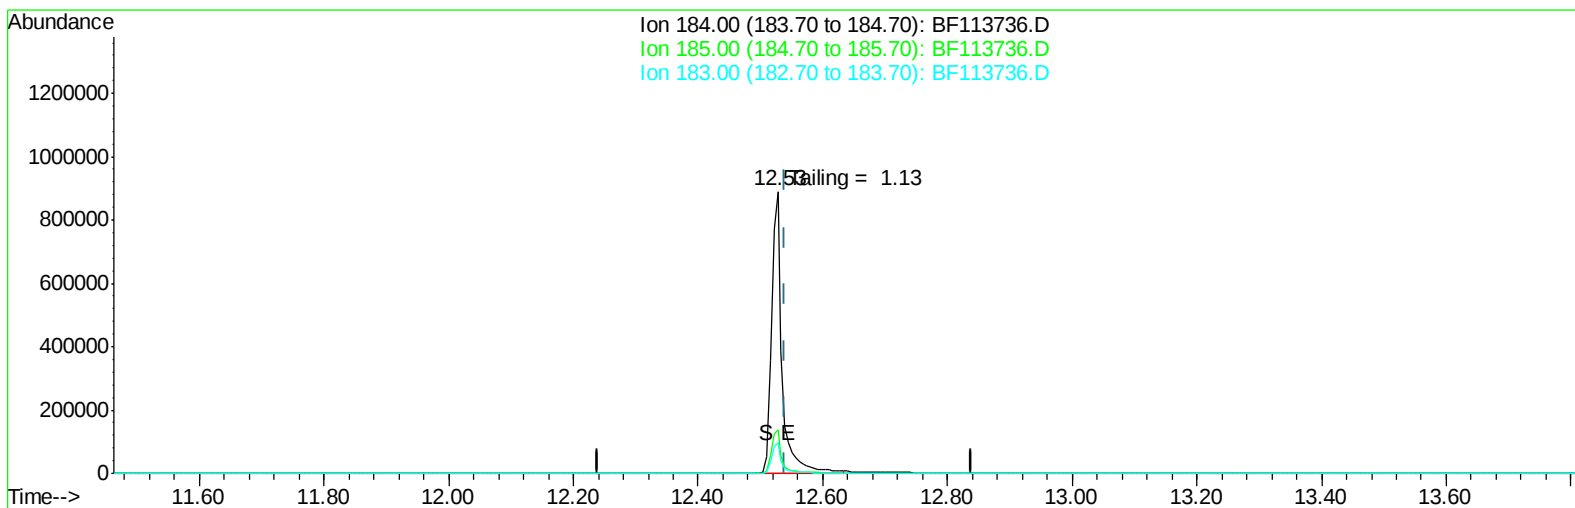

TIC: BF113736.D

(77) Benzidine

12.527min (-0.012) 0.00ng

response 1099904

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.30 | 15.36 |
| 183.00 | 11.20 | 10.78 |
| 0.00   | 0.00  | 0.00  |