
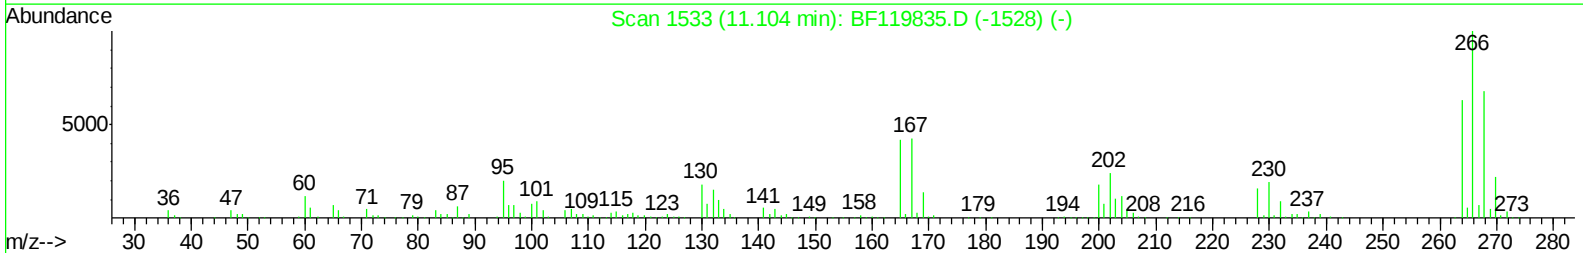
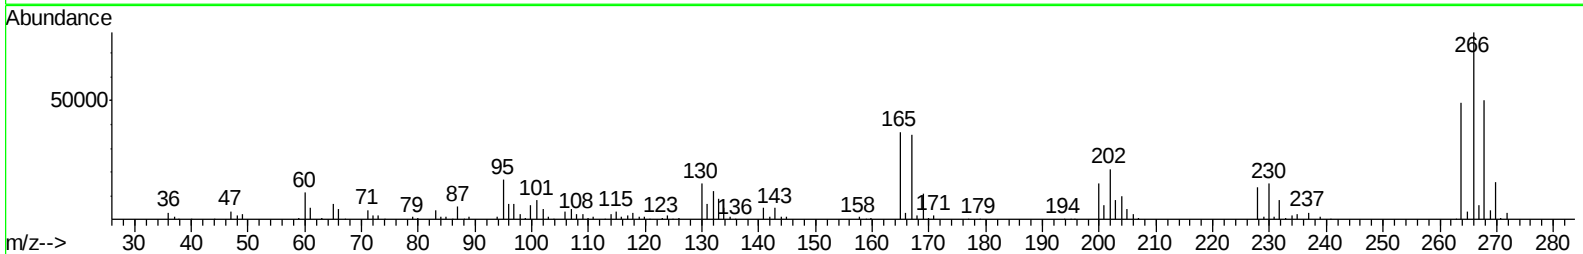


```
Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041320\  
Data File : BF119945.D  
Acq On    : 14 Apr 2020  11:45  
Operator  : MA/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```




Quant Time: Apr 15 05:47:15 2020
Quant Method : Z:\SV0ASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 12:44:44 2020
Response via : Initial Calibration

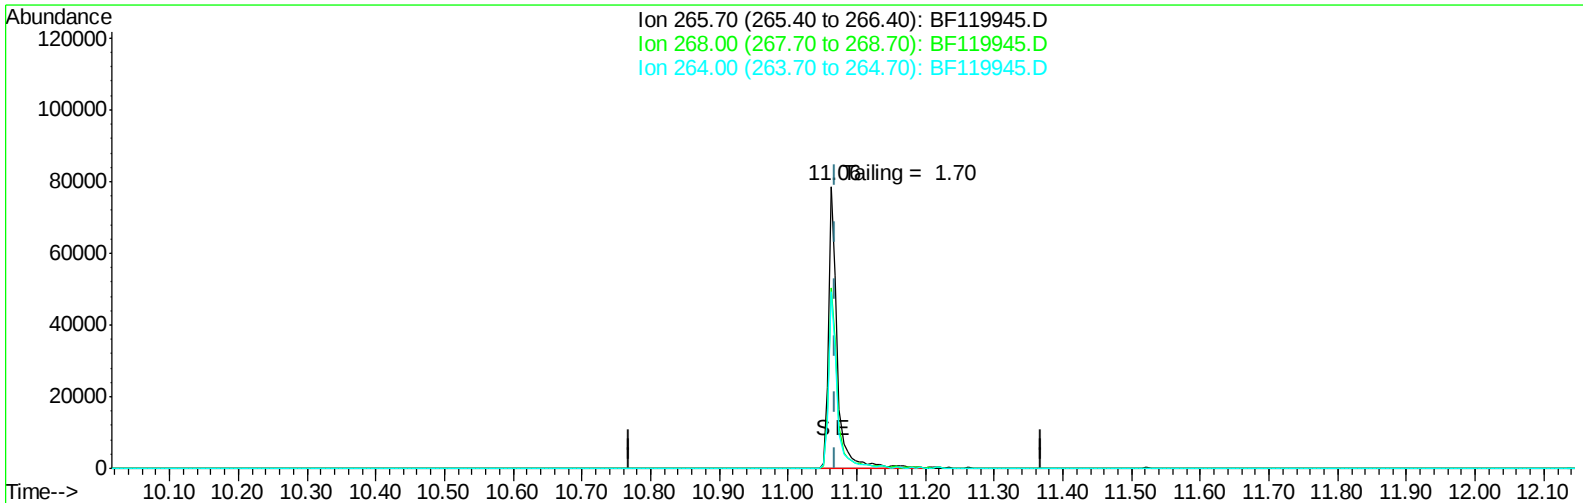

TIC: BF119945.D

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041320\
 Data File : BF119945.D
 Acq On : 14 Apr 2020 11:45
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 05:47:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 14 12:44:44 2020
 Response via : Initial Calibration

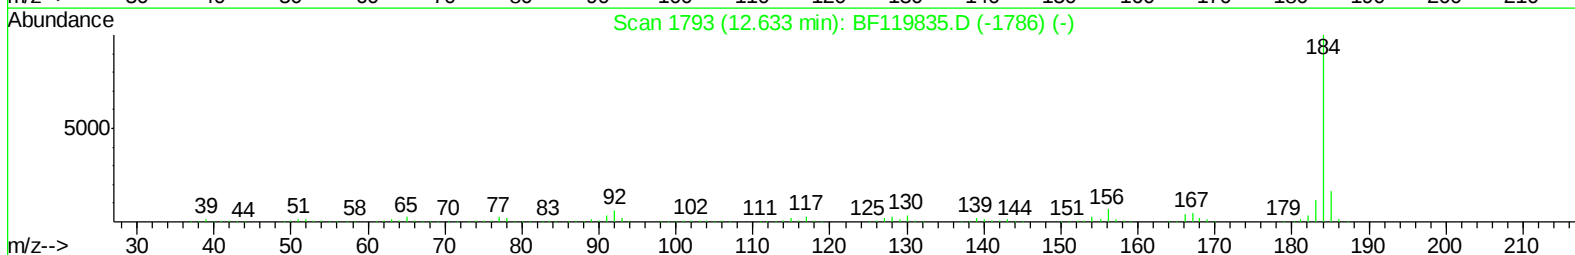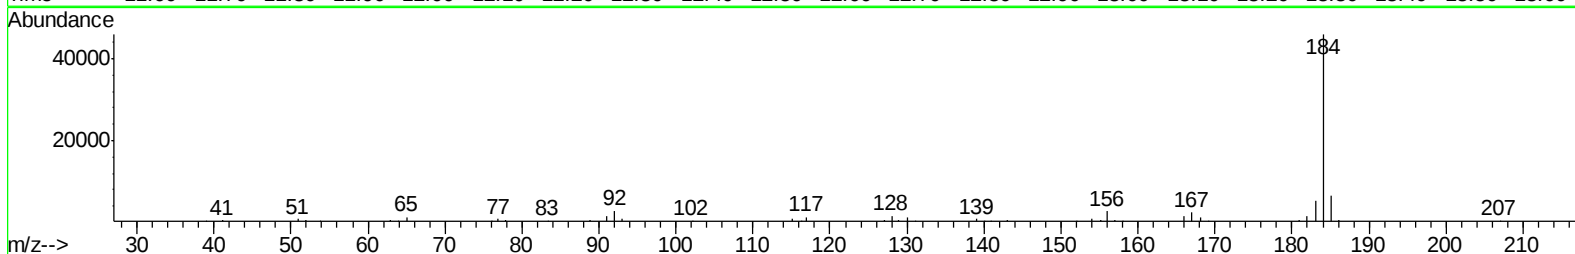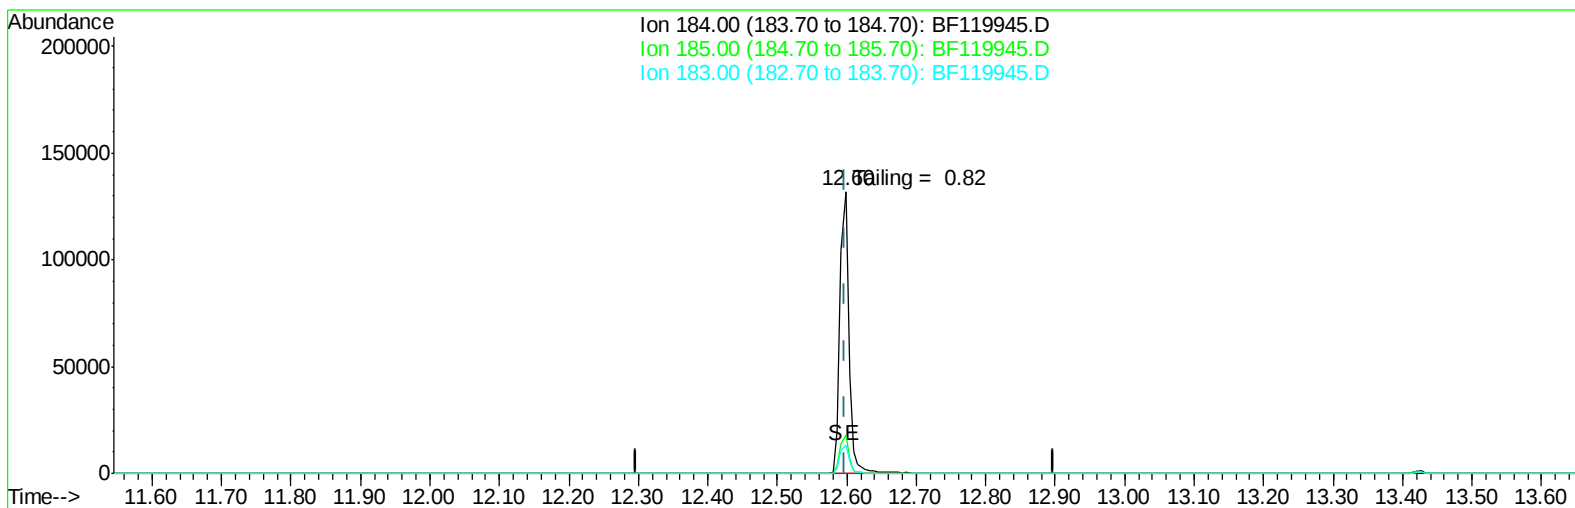

TIC: BF119945.D

(77) Benzidine

12.598min (+0.000) 0.00ng

response 114705

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	13.50
183.00	11.40	9.92
0.00	0.00	0.00