

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041320\
 Data File : BF119978.D
 Acq On : 15 Apr 2020 3:09
 Operator : MA/SJ
 Sample : L2215-29
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-2

Quant Time: Apr 15 04:53:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 14 12:44:44 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	240161	20.00	ng	0.00
21) Naphthalene-d8	8.02	136	939516	20.00	ng	0.00
39) Acenaphthene-d10	9.77	164	479489	20.00	ng	0.00
64) Phenanthrene-d10	11.26	188	876684	20.00	ng	0.00
76) Chrysene-d12	13.90	240	561724	20.00	ng	-0.01
87) Perylene-d12	15.32	264	451317	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	1196092	86.07	ng	0.00
7) Phenol-d6	6.37	99	1534262	85.68	ng	0.00
23) Nitrobenzene-d5	7.30	82	958364	52.77	ng	-0.01
42) 2,4,6-Tribromophenol	10.56	330	381964	65.06	ng	0.00
45) 2-Fluorobiphenyl	9.10	172	1804920	53.44	ng	0.00
79) Terphenyl-d14	12.85	244	1792319	53.69	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.49	163	297263	8.015	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041320\
Data File : BF119978.D
Acq On : 15 Apr 2020 3:09
Operator : MA/SJ
Sample : L2215-29
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Time: Apr 15 04:53:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 12:44:44 2020
Response via : Initial Calibration

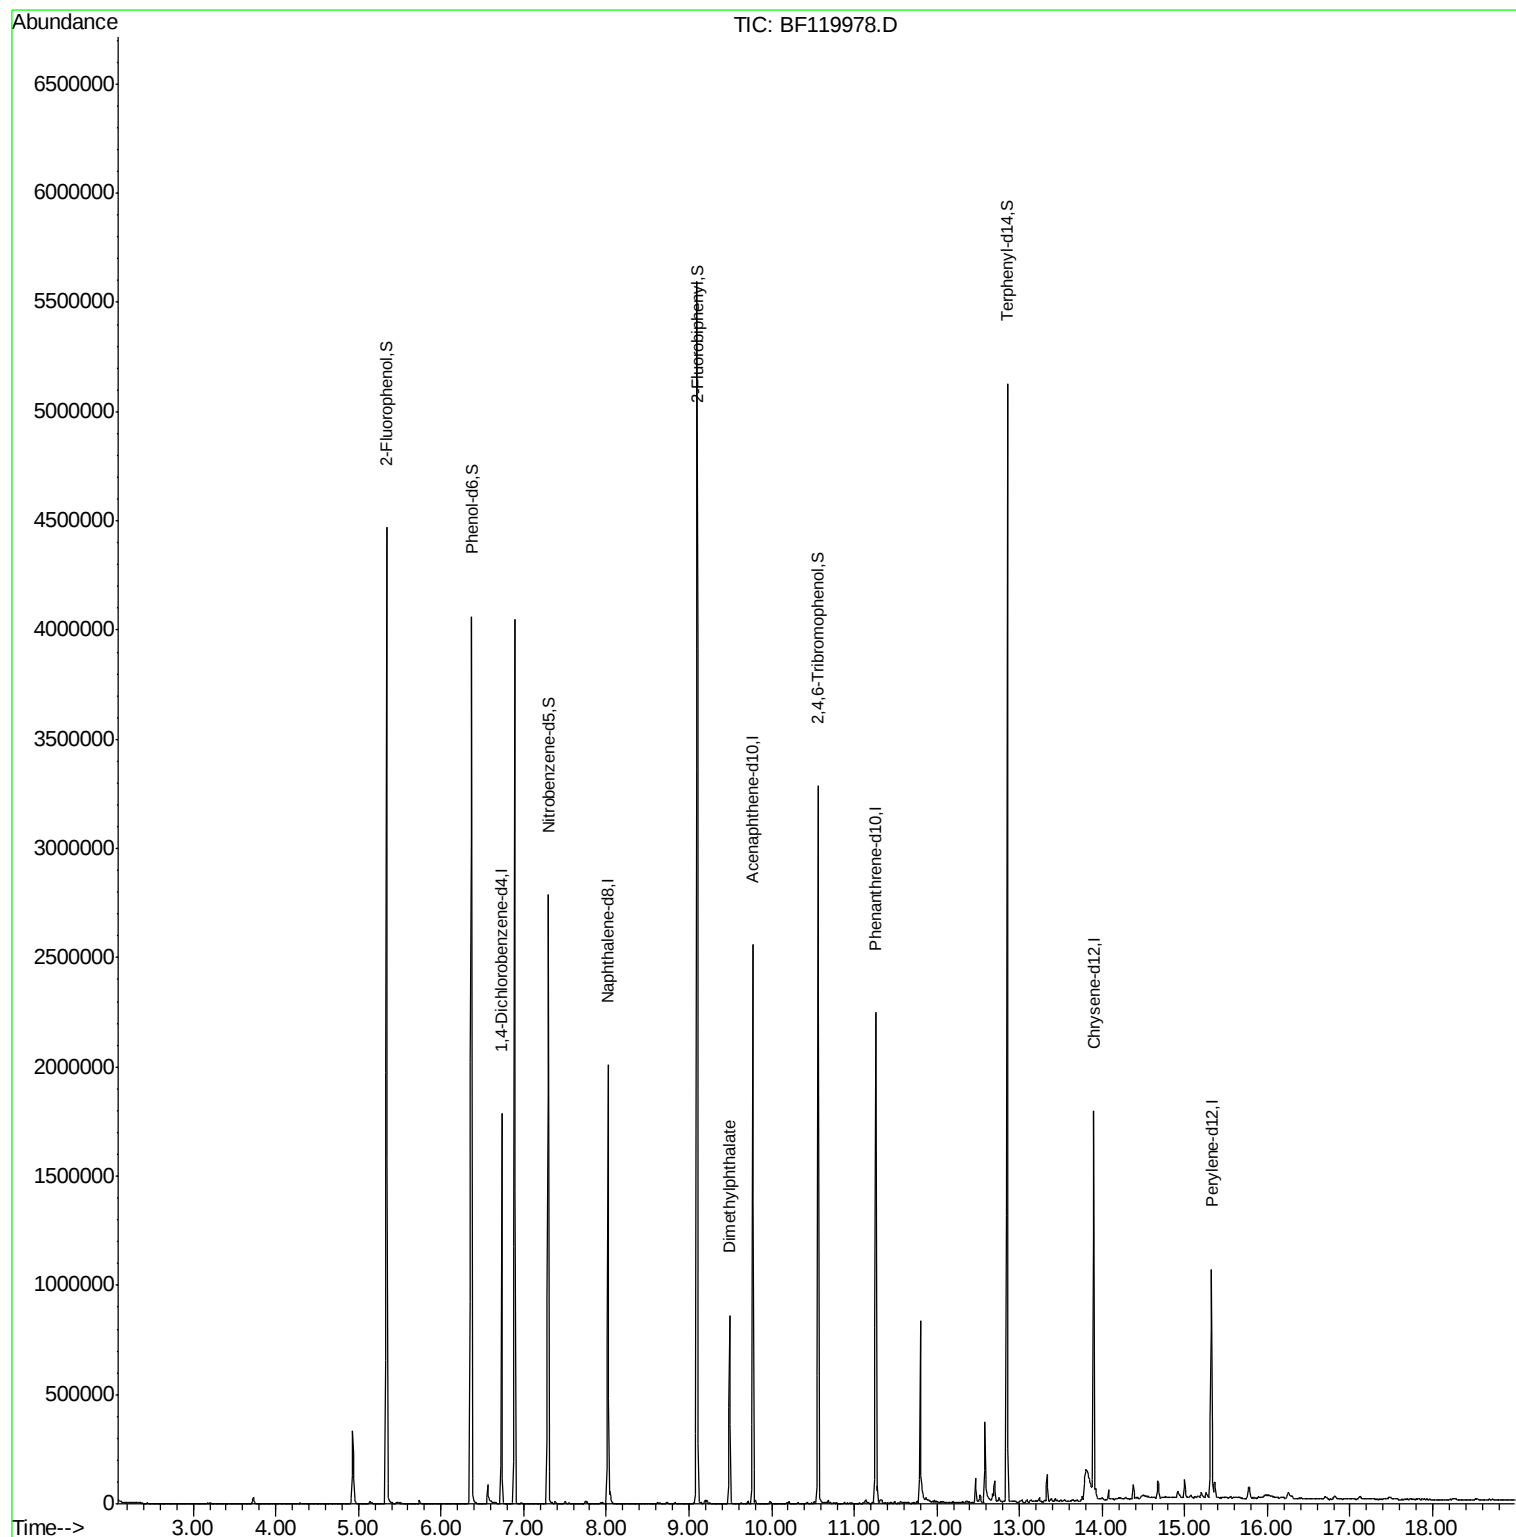




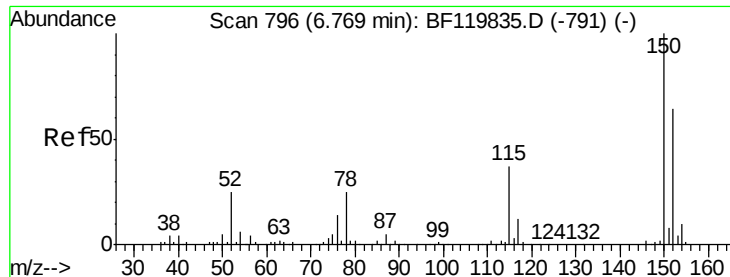


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 790
Delta R.T. -0.01 min
Lab File: BF119978.D
Acq: 15 Apr 2020 3:09

Instrument :
BNA_F
ClientSampleId :
TP-2




Tot Ion	Ratio	Lower	Upper
152	100		
150	154.6	124.8	187.2
115	60.2	46.5	69.7

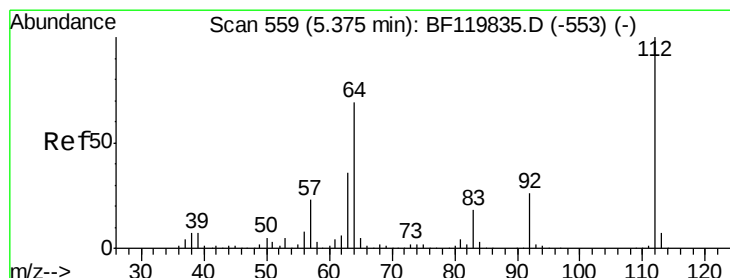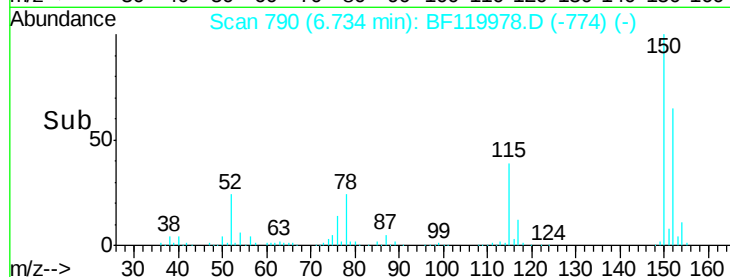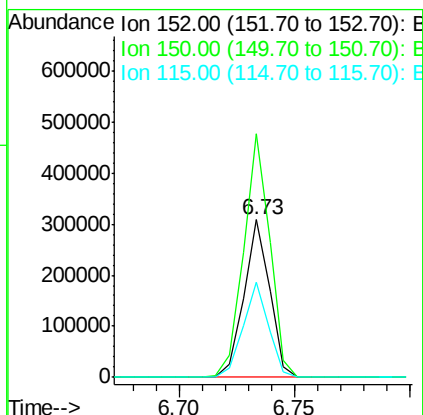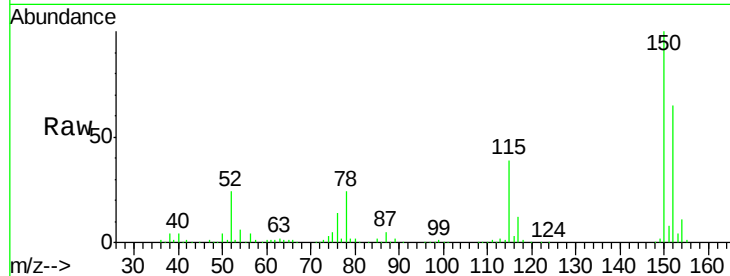

#5

2-Fluorophenol
Concen: 86.070 ng
RT: 5.35 min Scan# 554
Delta R.T. 0.01 min
Lab File: BF119978.D
Acq: 15 Apr 2020 3:09

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.0	55.5	83.3
63	35.6	29.1	43.7

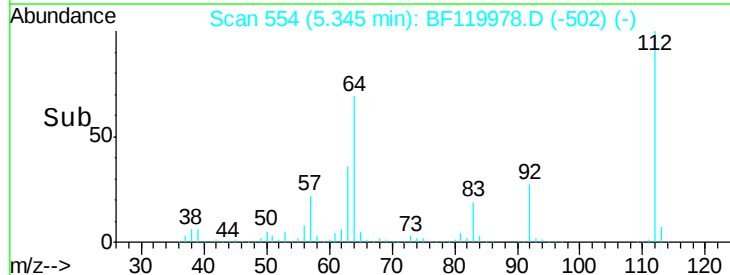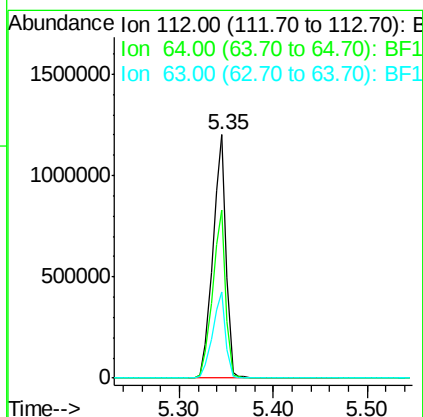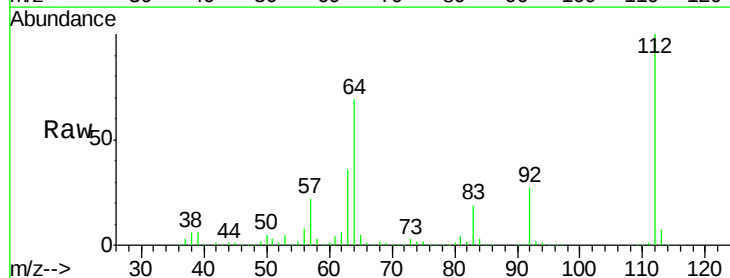



#7

Phenol-d6

Concen: 85.681 ng

RT: 6.37 min Scan# 728

Delta R.T. -0.01 min

Lab File: BF119978.D

Acq: 15 Apr 2020 3:09

Instrument :

BNA_F

ClientSampleId :

TP-2




Tot Ion: 99 Resp: 1534262

Ion Ratio Lower Upper

99 100

42 19.4 16.9 25.3

71 33.7 26.3 39.5

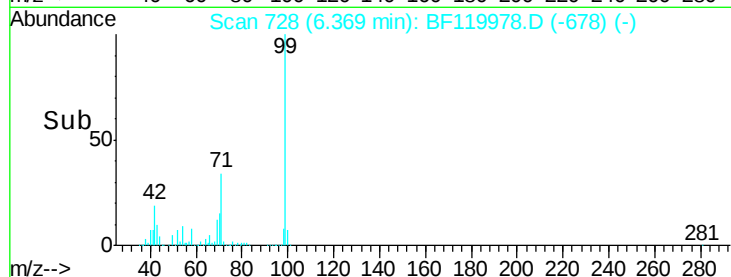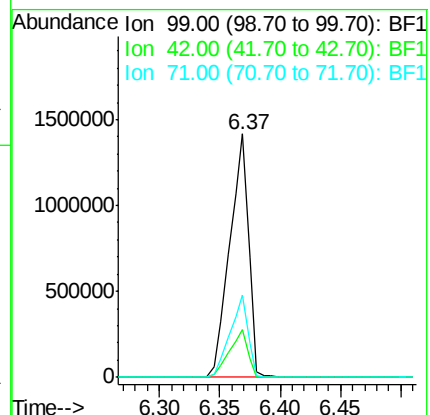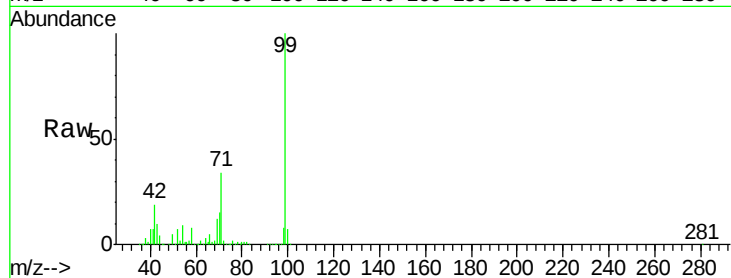

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 1009

Delta R.T. -0.01 min

Lab File: BF119978.D

Acq: 15 Apr 2020 3:09

Tgt Ion: 136 Resp: 939516




Ion Ratio Lower Upper

136 100

137 10.7 8.7 13.1

54 9.2 8.5 12.7

68 5.2 3.9 5.9


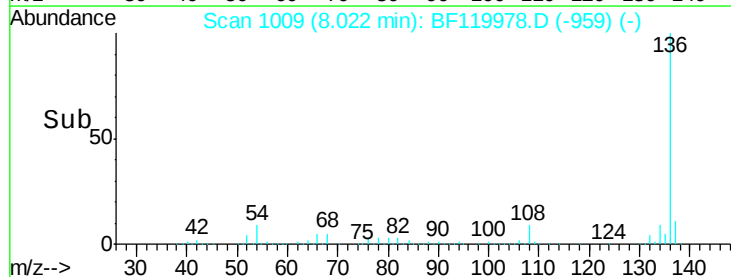
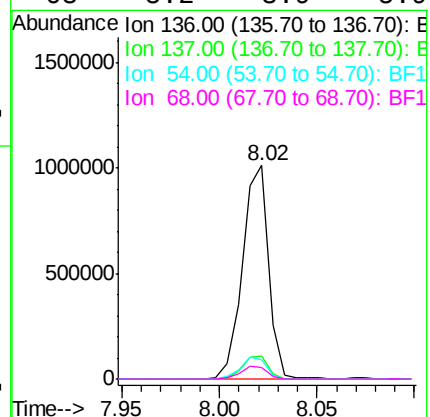
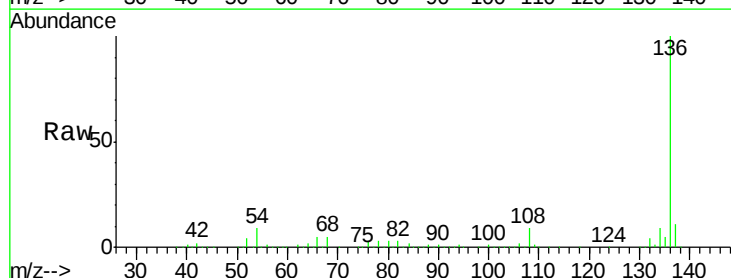




#23
 Nitrobenzene-d5
 Concen: 52.771 ng
 RT: 7.30 min Scan# 886
 Delta R.T. -0.01 min
 Lab File: BF119978.D
 Acq: 15 Apr 2020 3:09




Instrument :
 BNA_F
 ClientSampled :
 TP-2

Tot Ion: 82 Resp: 958364
 Ion Ratio Lower Upper
 82 100
 128 44.7 36.2 54.4
 54 60.1 50.4 75.6

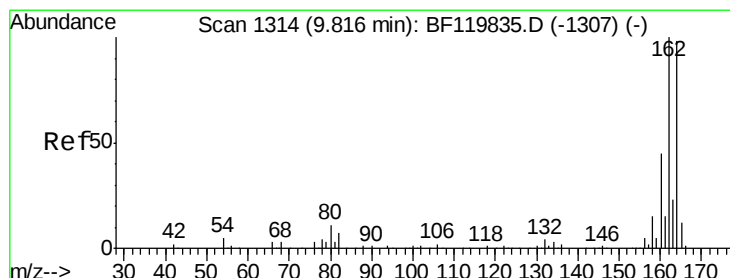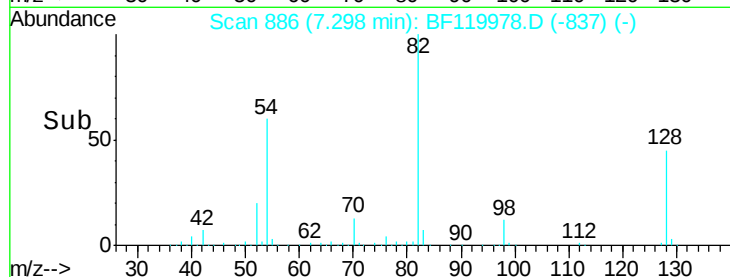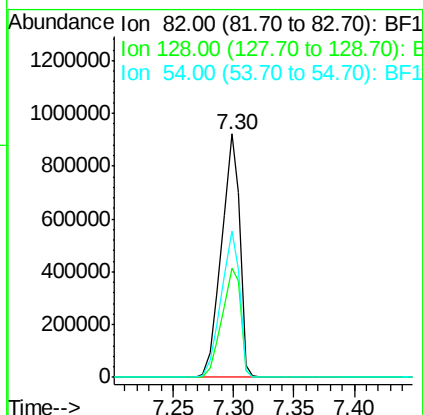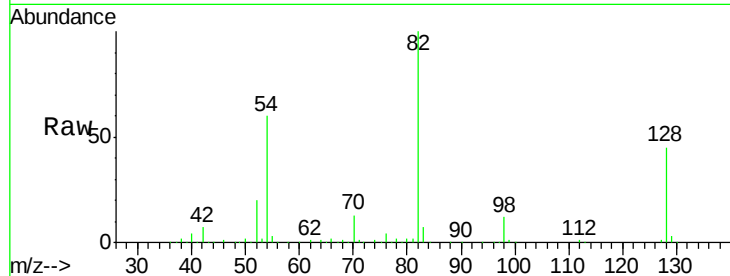

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.77 min Scan# 1307
 Delta R.T. -0.01 min
 Lab File: BF119978.D
 Acq: 15 Apr 2020 3:09

Tgt Ion: 164 Resp: 479489
 Ion Ratio Lower Upper
 164 100
 162 102.8 81.9 122.9
 160 45.4 36.6 54.8

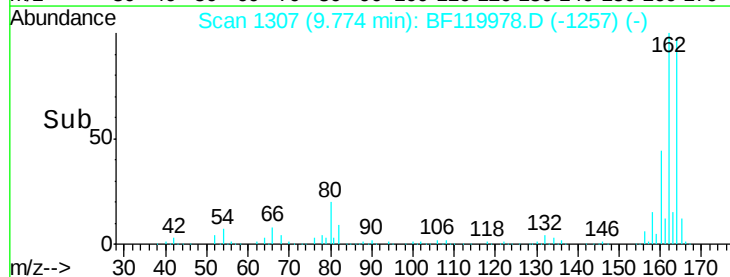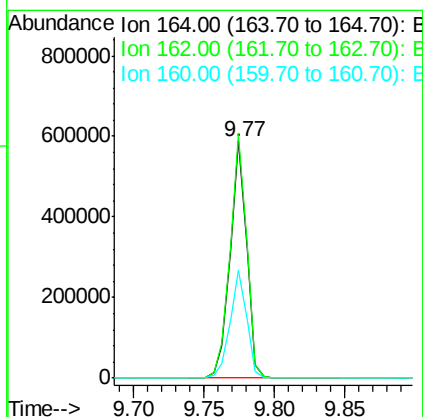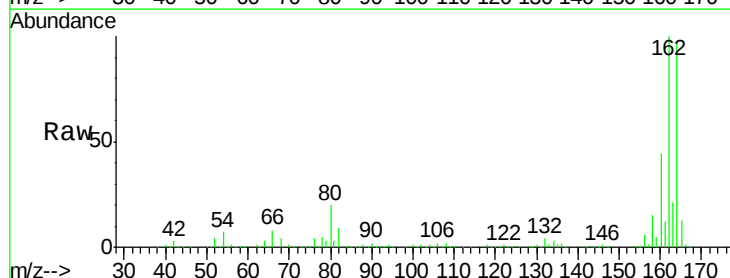







#42
 2,4,6-Tribromophenol
 Concen: 65.064 ng
 RT: 10.56 min Scan# 1441
 Delta R.T. -0.01 min
 Lab File: BF119978.D
 Acq: 15 Apr 2020 3:09

Instrument :
 BNA_F
 ClientSampleId :
 TP-2

Tot Ion:330 Resp: 381964
 Ion Ratio Lower Upper
 330 100
 332 96.5 76.8 115.2
 141 34.4 25.1 37.7

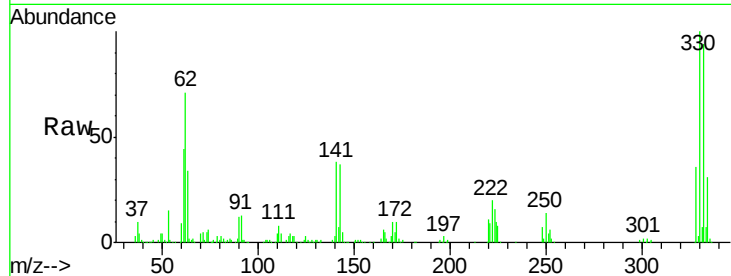


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

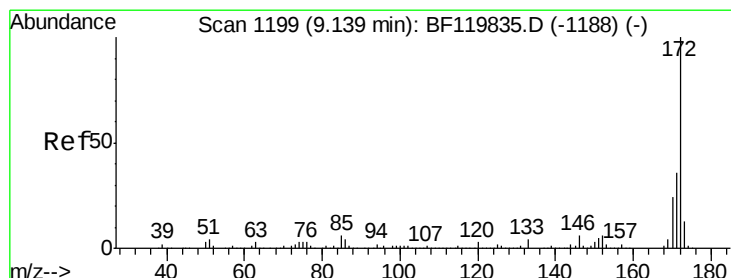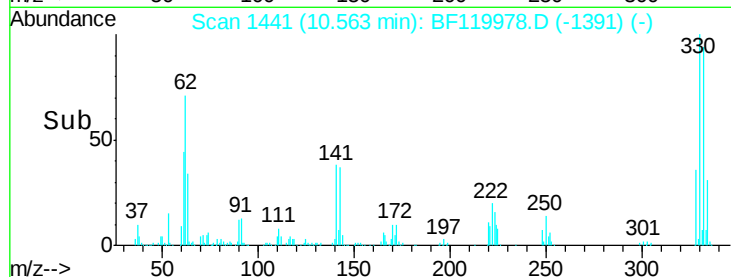
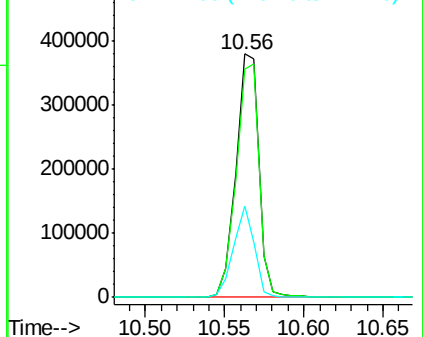



#45
 2-Fluorobiphenyl
 Concen: 53.444 ng
 RT: 9.10 min Scan# 1192
 Delta R.T. -0.01 min
 Lab File: BF119978.D
 Acq: 15 Apr 2020 3:09

Tgt Ion:172 Resp: 1804920
 Ion Ratio Lower Upper
 172 100
 171 36.5 28.9 43.3
 170 24.3 19.4 29.2

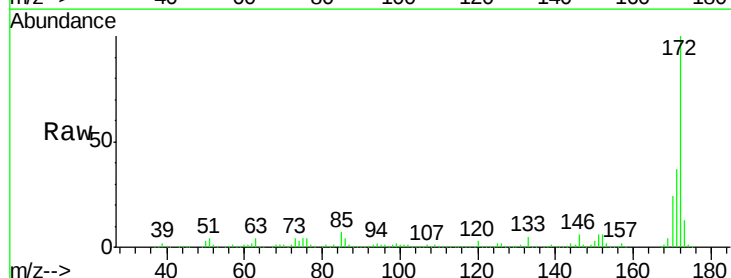

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

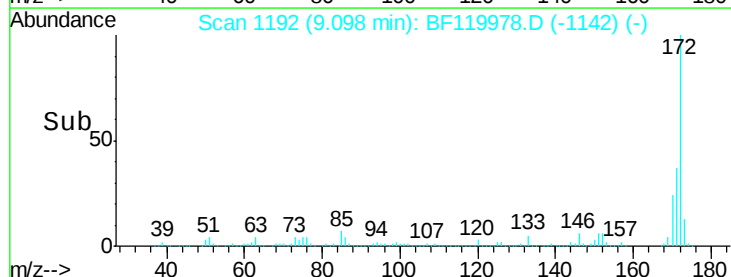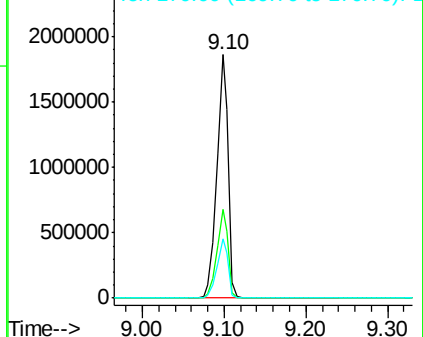

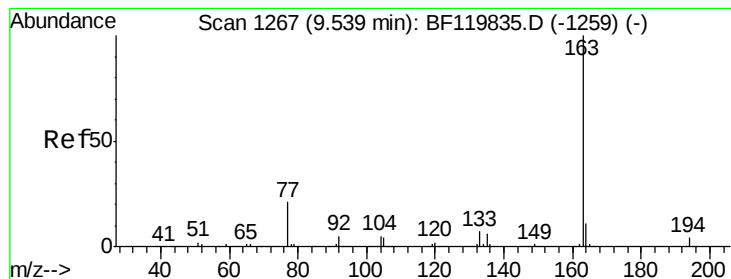

#50

Dimethylphthalate

Concen: 8.015 ng

RT: 9.49 min Scan# 1259

Delta R.T. -0.02 min

Lab File: BF119978.D

Acq: 15 Apr 2020 3:09

Instrument :

BNA_F

ClientSampleId :

TP-2


Tot Ion:163 Resp: 297263

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.4




164 10.0 8.4 12.6

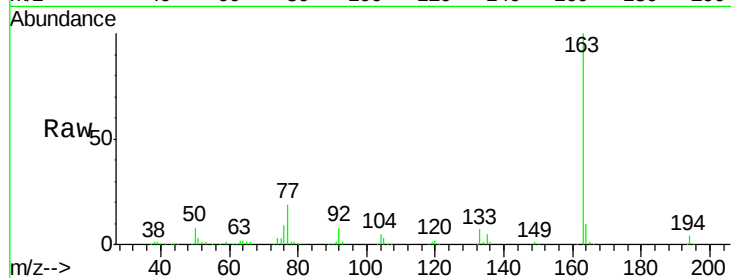

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

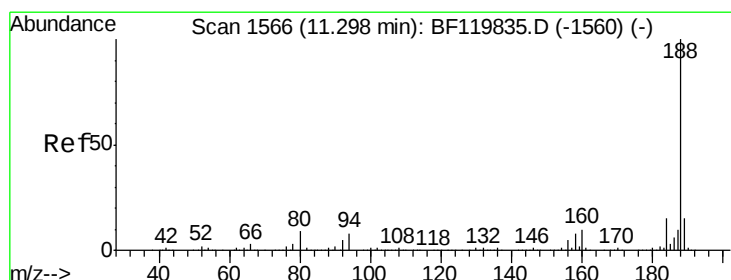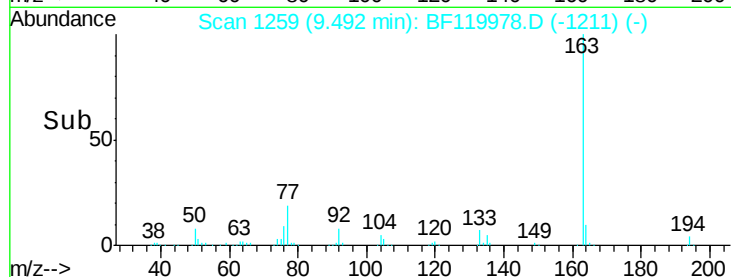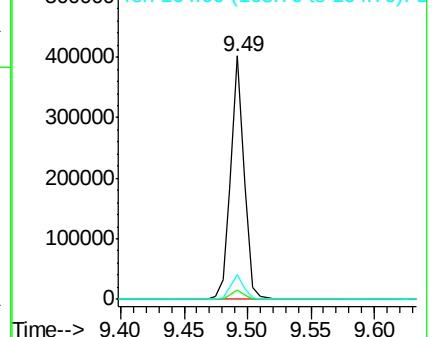

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.26 min Scan# 1559

Delta R.T. -0.01 min

Lab File: BF119978.D

Acq: 15 Apr 2020 3:09


Tgt Ion:188 Resp: 876684

Ion Ratio Lower Upper

188 100

94 10.1 6.7 10.1#



80 10.7 7.4 11.2

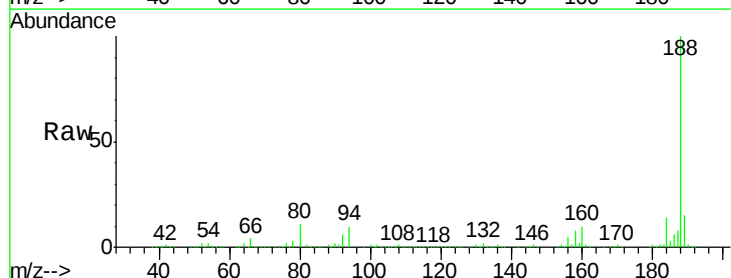


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

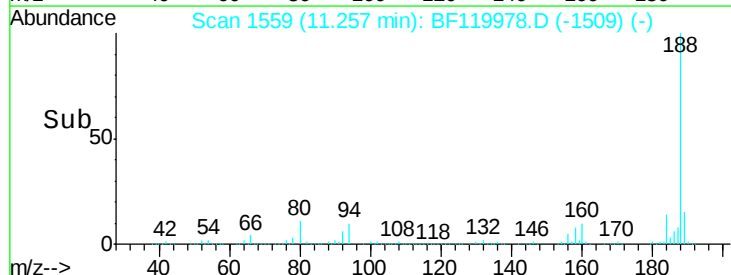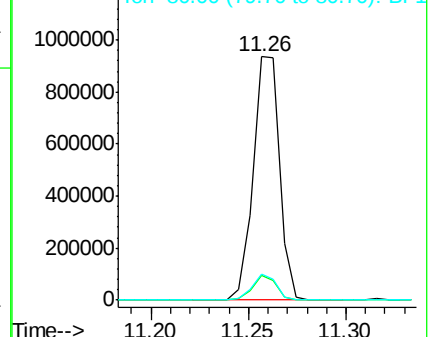

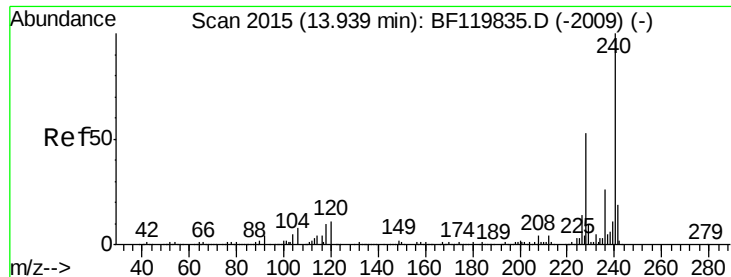

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.90 min Scan# 2008

Delta R.T. -0.01 min

Lab File: BF119978.D

Acq: 15 Apr 2020 3:09

Instrument :

BNA_F

ClientSampleId :

TP-2


Tot Ion:240 Resp: 561724

Ion Ratio Lower Upper

240 100

120 11.0 9.0 13.6




236 25.4 20.7 31.1

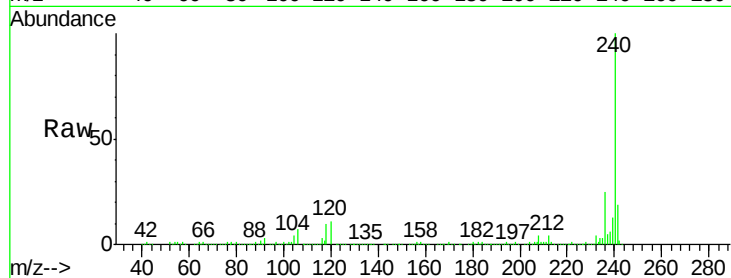

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

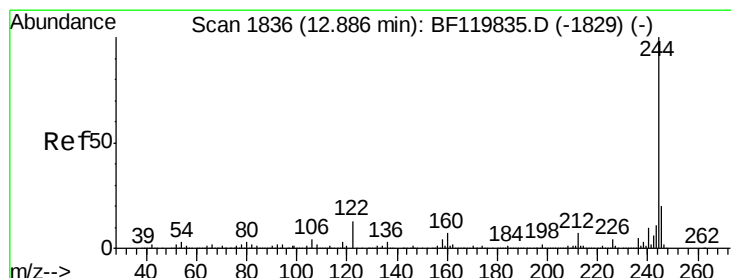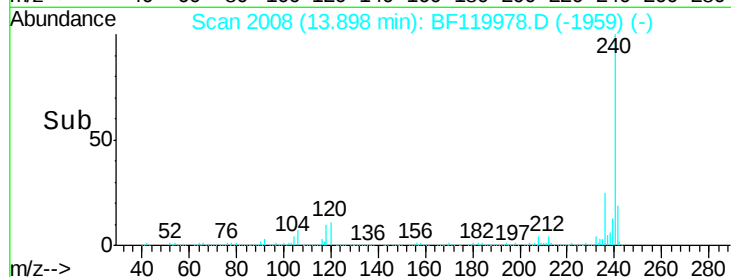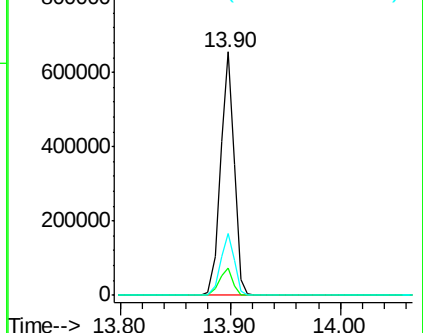

#79

Terphenyl-d14

Concen: 53.689 ng

RT: 12.85 min Scan# 1830

Delta R.T. -0.01 min

Lab File: BF119978.D

Acq: 15 Apr 2020 3:09


Tgt Ion:244 Resp: 1792319

Ion Ratio Lower Upper

244 100

212 6.8 5.4 8.0



122 13.2 10.3 15.5

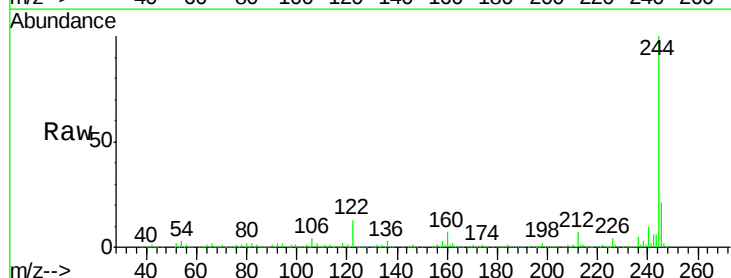


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

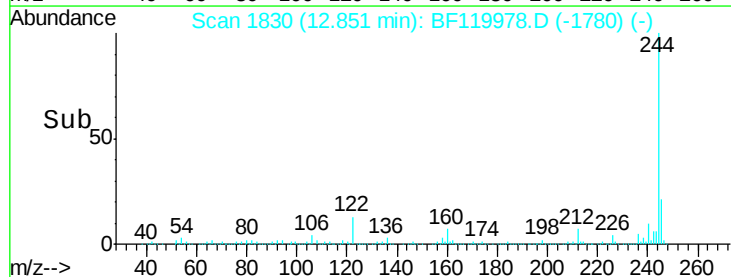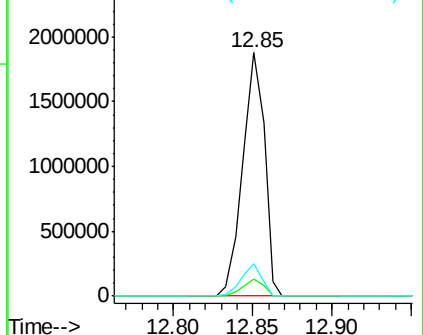


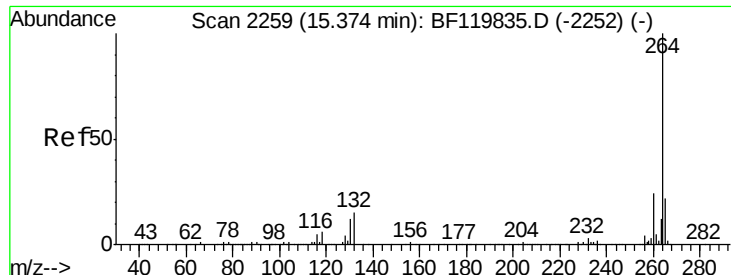

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.32 min Scan# 2250
Delta R.T. -0.01 min
Lab File: BF119978.D
Acq: 15 Apr 2020 3:09

Instrument :
BNA_F
ClientSampleId :
TP-2

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.3	28.9
265	21.6	17.6	26.4

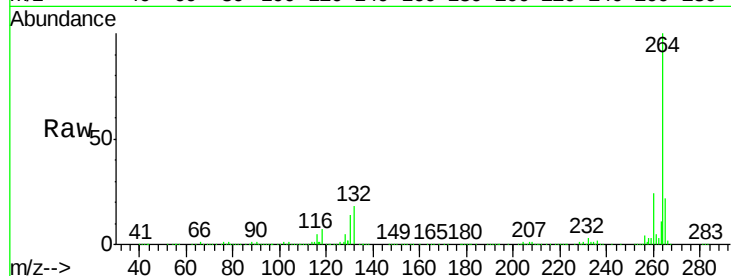

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

