


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041320\
 Data File : BF119911.D
 Acq On : 13 Apr 2020 11:22
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 13 13:37:50 2020

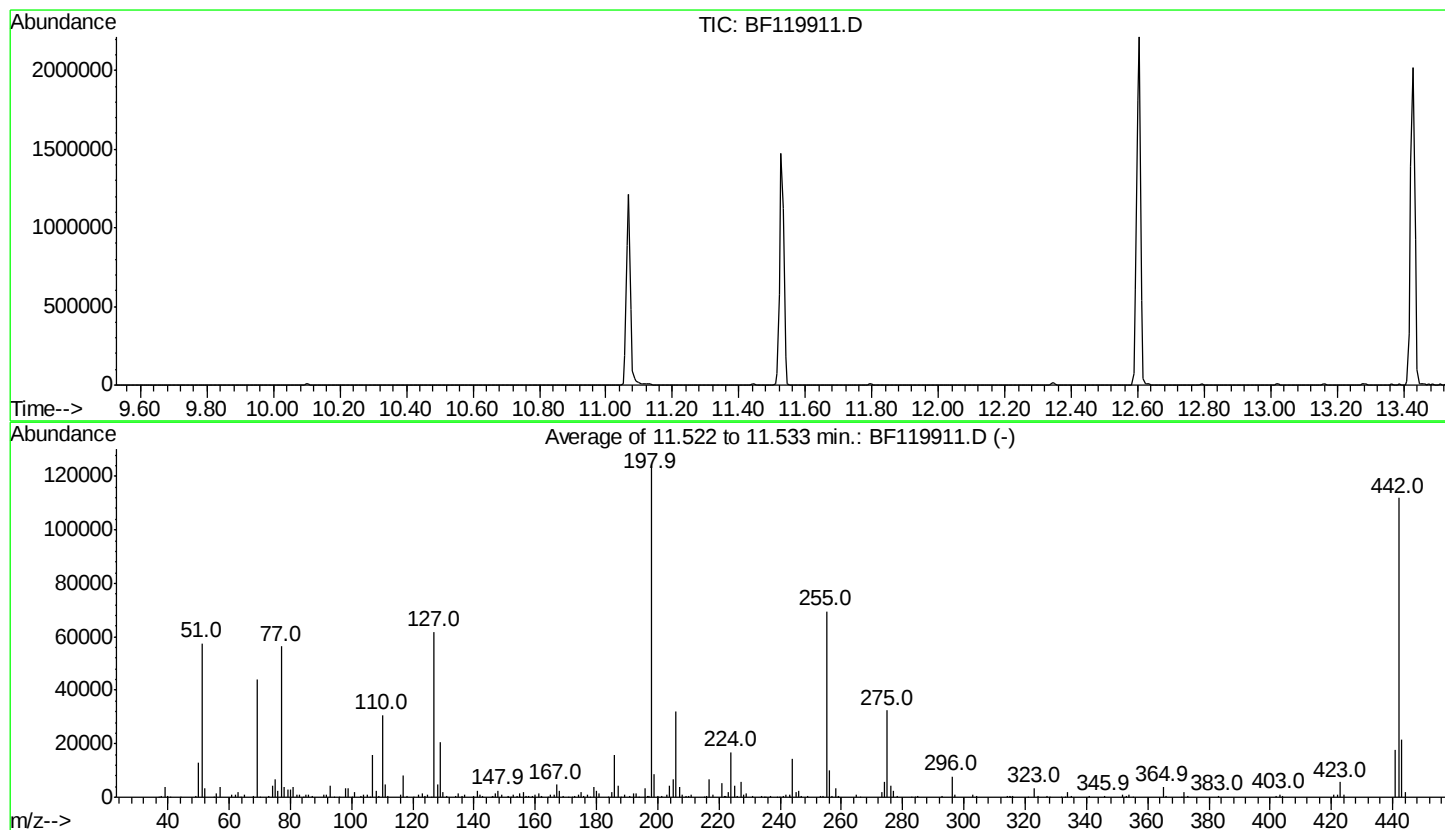

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	57637	PASS
68	69	0.00	2	1.5	642	PASS
69	198	0.00	100	35.6	44202	PASS
70	69	0.00	2	0.4	156	PASS
127	198	10	80	49.8	61778	PASS
197	198	0.00	2	0.5	601	PASS
198	198	100	100	100.0	124040	PASS
199	198	5	9	6.9	8595	PASS
275	198	10	60	26.1	32423	PASS
365	198	1	100	3.1	3902	PASS
441	198	0.01	100	14.3	17740	PASS
442	198	50	100	90.2	111848	PASS
443	442	15	24	19.1	21349	PASS