


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041320\
 Data File : BF119930.D
 Acq On : 14 Apr 2020 1:44
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 15 11:01:23 2020

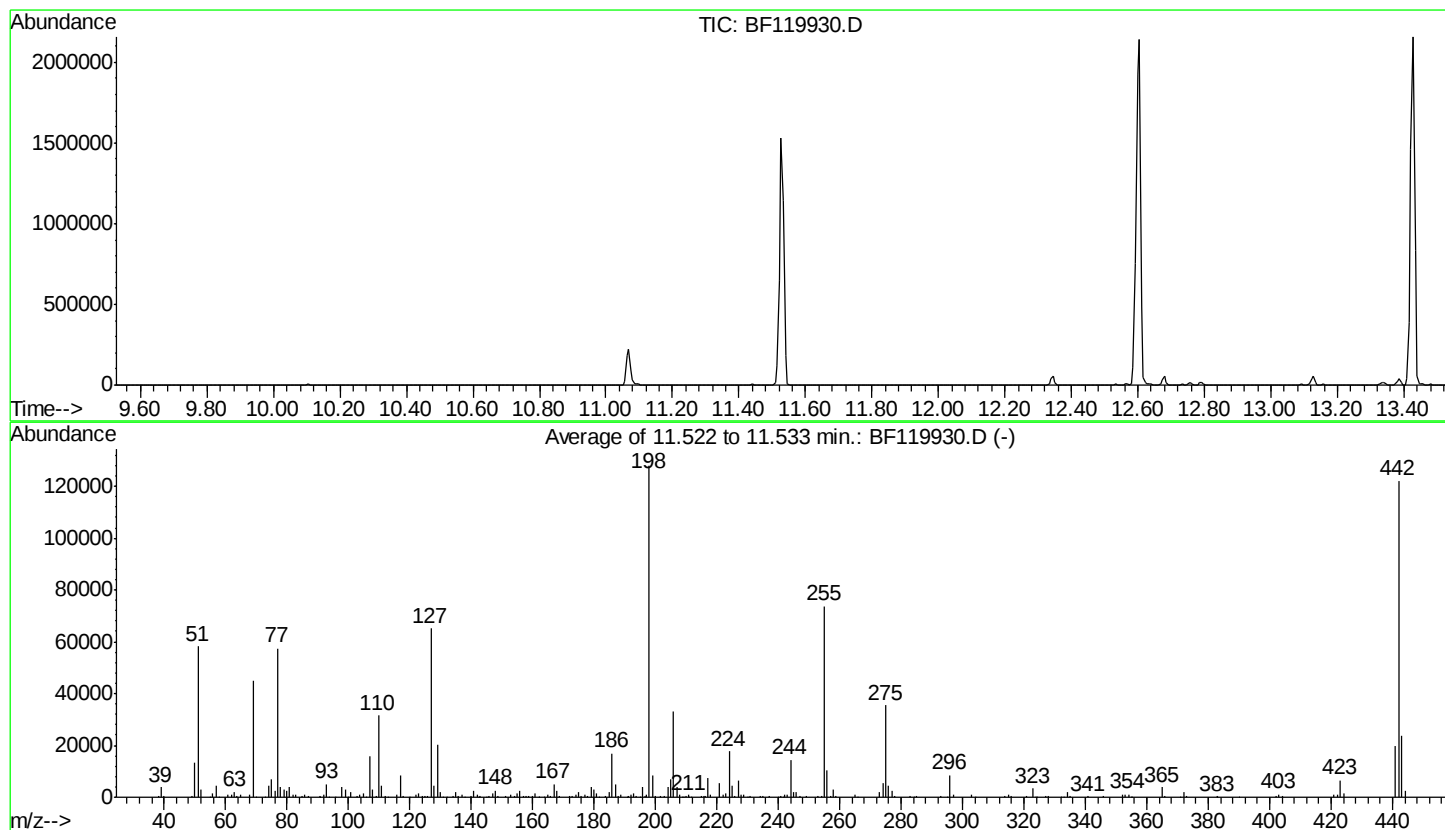

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	58258	PASS
68	69	0.00	2	1.9	864	PASS
69	198	0.00	100	35.2	45061	PASS
70	69	0.00	2	0.2	103	PASS
127	198	10	80	50.9	65152	PASS
197	198	0.00	2	0.7	878	PASS
198	198	100	100	100.0	127994	PASS
199	198	5	9	6.5	8331	PASS
275	198	10	60	27.7	35426	PASS
365	198	1	100	2.9	3728	PASS
441	198	0.01	100	15.3	19598	PASS
442	198	50	100	95.4	122149	PASS
443	442	15	24	19.6	23891	PASS