


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041320\
 Data File : BF119962.D
 Acq On : 14 Apr 2020 19:24
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 15 11:01:23 2020

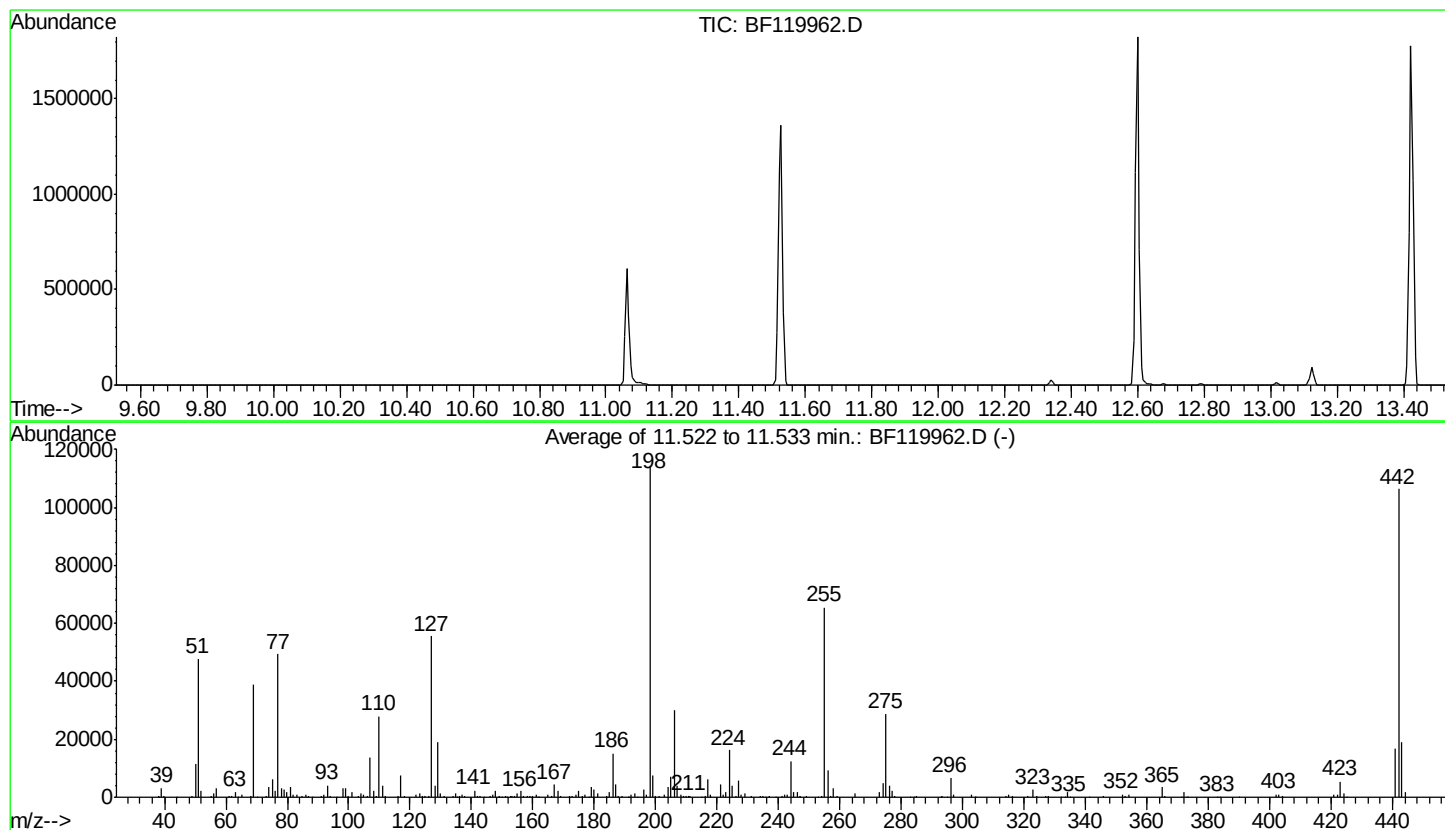

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	47871	PASS
68	69	0.00	2	1.7	654	PASS
69	198	0.00	100	34.0	38889	PASS
70	69	0.00	2	0.4	137	PASS
127	198	10	80	48.5	55527	PASS
197	198	0.00	2	0.6	726	PASS
198	198	100	100	100.0	114386	PASS
199	198	5	9	6.4	7357	PASS
275	198	10	60	25.2	28774	PASS
365	198	1	100	3.0	3435	PASS
441	198	0.01	100	14.8	16920	PASS
442	198	50	100	93.0	106328	PASS
443	442	15	24	18.0	19149	PASS