

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041519\
 Data File : BF113782.D
 Acq On : 16 Apr 2019 00:23
 Operator : JU/SJ
 Sample : K2359-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OIL-WATER-SEPERATOR-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.410	372	395	408	rBV3	62653	326439	1.09%	0.219%
2	5.304	543	547	573	rVB	1260653	2034091	6.80%	1.364%
3	6.340	720	723	732	rBV	1065646	1876247	6.27%	1.258%
4	6.451	739	742	749	rVB	1994163	2133211	7.13%	1.431%
5	6.675	776	780	782	rBV	674163	681994	2.28%	0.457%
6	6.751	789	793	797	rBV	3448887	3165018	10.58%	2.123%
7	6.792	797	800	803	rBV2	1491944	1451903	4.85%	0.974%
8	6.828	803	806	815	rVB	1759987	1799004	6.01%	1.207%
9	6.951	825	827	829	rVV	363433	322686	1.08%	0.216%
10	7.022	834	839	841	rBV	383499	401193	1.34%	0.269%
11	7.110	851	854	856	rBV	311822	353464	1.18%	0.237%
12	7.128	856	857	863	rVV2	306856	313440	1.05%	0.210%
13	7.239	870	876	880	rVV	1360285	1480482	4.95%	0.993%
14	7.686	948	952	958	rVV	1514665	1598187	5.34%	1.072%
15	7.798	964	971	972	rBV3	298697	502717	1.68%	0.337%
16	7.828	973	976	980	rVB	428020	452836	1.51%	0.304%
17	7.951	992	997	1001	rBV2	864105	962674	3.22%	0.646%
18	8.551	1096	1099	1102	rBV	605410	476541	1.59%	0.320%
19	8.910	1157	1160	1164	rVB2	304914	328602	1.10%	0.220%
20	9.028	1176	1180	1184	rVB	2547648	2188748	7.31%	1.468%
21	9.116	1191	1195	1199	rVB	625289	538553	1.80%	0.361%
22	9.433	1244	1249	1251	rVV2	636973	711065	2.38%	0.477%
23	9.645	1282	1285	1289	rVB	404140	360136	1.20%	0.242%
24	9.704	1292	1295	1298	rBV	861421	734735	2.46%	0.493%
25	9.951	1331	1337	1343	rBV	648188	958256	3.20%	0.643%
26	10.139	1362	1369	1372	rBV	519659	509385	1.70%	0.342%
27	10.498	1427	1430	1441	rVB2	1163106	1232645	4.12%	0.827%
28	10.610	1446	1449	1451	rBV	510333	526984	1.76%	0.353%
29	10.639	1451	1454	1458	rVB2	488684	632018	2.11%	0.424%
30	10.686	1458	1462	1465	rBV2	1456499	1766970	5.90%	1.185%
31	10.722	1465	1468	1471	rVV2	1379476	2002084	6.69%	1.343%
32	10.757	1471	1474	1476	rVV2	1491162	1734221	5.79%	1.163%
33	10.780	1476	1478	1481	rVV	874725	931792	3.11%	0.625%
34	10.822	1481	1485	1490	rVV2	573647	1214054	4.06%	0.814%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041519\
 Data File : BF113782.D
 Acq On : 16 Apr 2019 00:23
 Operator : JU/SJ
 Sample : K2359-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OIL-WATER-SEPERATOR-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.874	1490	1494	1495	rVV3	1274418	1834800	6.13%	1.231%
36	10.910	1495	1500	1501	rVV	3772628	5902202	19.72%	3.958%
37	10.945	1505	1506	1517	rVB	1096516	1283744	4.29%	0.861%
38	11.057	1523	1525	1528	rBV	412882	363653	1.22%	0.244%
39	11.092	1528	1531	1534	rVB2	353248	357779	1.20%	0.240%
40	11.192	1545	1548	1556	rVV	750978	1100398	3.68%	0.738%
41	11.322	1566	1570	1574	rBV2	646121	622789	2.08%	0.418%
42	11.492	1595	1599	1603	rVV2	493742	689273	2.30%	0.462%
43	11.586	1611	1615	1622	rBV2	206460	391403	1.31%	0.263%
44	11.816	1626	1654	1657	rBV2	6365294	26745411	89.37%	17.937%
45	11.892	1664	1667	1671	rVB	439394	437697	1.46%	0.294%
46	12.045	1690	1693	1697	rBV2	1156793	1259290	4.21%	0.845%
47	12.145	1707	1710	1719	rVB2	282834	410128	1.37%	0.275%
48	12.280	1728	1733	1737	rBV3	404903	627408	2.10%	0.421%
49	12.404	1750	1754	1756	rBV	884506	1129900	3.78%	0.758%
50	12.521	1757	1774	1780	rVV4	5848232	29928008	100.00%	20.072%
51	12.574	1780	1783	1789	rVV	3852743	5147507	17.20%	3.452%
52	12.651	1792	1796	1800	rVB2	616301	829389	2.77%	0.556%
53	12.774	1813	1817	1822	rVB	2649973	2682906	8.96%	1.799%
54	12.886	1830	1836	1838	rBV2	557392	783265	2.62%	0.525%
55	12.916	1838	1841	1846	rBV2	1338991	2681944	8.96%	1.799%
56	13.039	1859	1862	1870	rBV4	628257	1762375	5.89%	1.182%
57	13.098	1870	1872	1879	rVV	1143228	2211897	7.39%	1.483%
58	13.157	1879	1882	1890	rVV3	710806	1699222	5.68%	1.140%
59	13.216	1890	1892	1895	rVB3	350029	305549	1.02%	0.205%
60	13.345	1912	1914	1917	rVB	443875	470596	1.57%	0.316%
61	13.527	1942	1945	1948	rBV2	414046	501600	1.68%	0.336%
62	13.580	1948	1954	1957	rBV6	605451	1244643	4.16%	0.835%
63	13.833	1995	1997	2001	rVB	744265	717830	2.40%	0.481%
64	13.880	2001	2005	2007	rBV2	602402	922179	3.08%	0.618%
65	14.104	2040	2043	2047	rVB2	857640	962748	3.22%	0.646%
66	14.157	2047	2052	2055	rBV	840038	1440720	4.81%	0.966%
67	14.292	2071	2075	2082	rBV2	1217273	2476877	8.28%	1.661%
68	14.457	2099	2103	2109	rBV	2345424	4040634	13.50%	2.710%
69	14.510	2109	2112	2114	rVV2	789826	799876	2.67%	0.536%
70	14.804	2160	2162	2166	rVB2	849383	871897	2.91%	0.585%
71	14.857	2167	2171	2176	rBV4	594926	1144578	3.82%	0.768%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041519\
Data File : BF113782.D
Acq On : 16 Apr 2019 00:23
Operator : JU/SJ
Sample : K2359-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OIL-WATER-SEPERATOR-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	15.045	2199	2203	2207	rBV	1129626	2113323	7.06%	1.417%
73	15.133	2216	2218	2223	rVB	514482	650685	2.17%	0.436%
74	15.227	2230	2234	2237	rBV2	992281	1451651	4.85%	0.974%
75	15.780	2324	2328	2337	rVB	627899	1405530	4.70%	0.943%


Sum of corrected areas: 149105679

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041519\
Data File : BF113782.D
Acq On : 16 Apr 2019 00:23
Operator : JU/SJ
Sample : K2359-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OIL-WATER-SEPARATOR-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

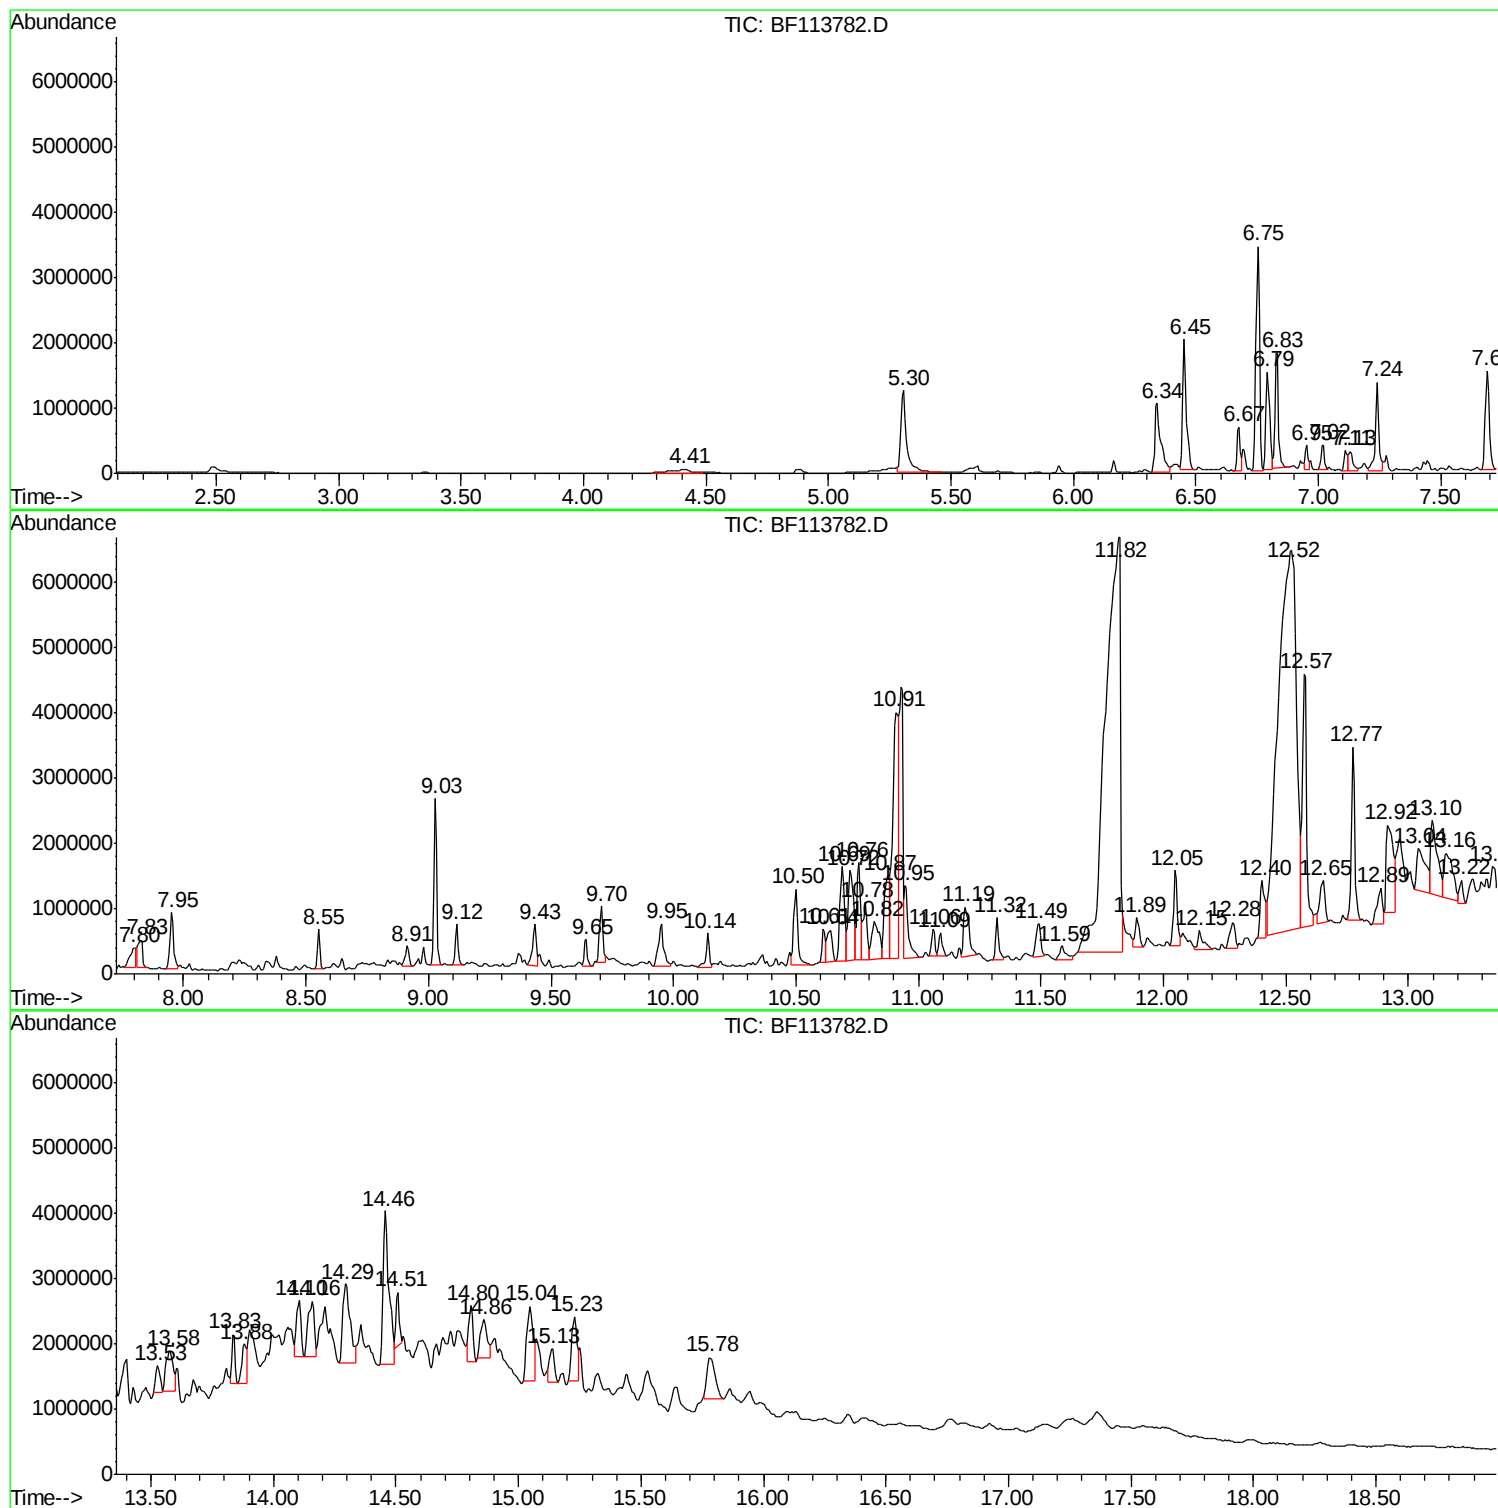

DbaaaPathh::ZZ\SS00SSRVNRP000001BBNAFNDATAAB0015599\
 DbaaaFile::BBE13382DD
 Aeqq00n ::166Apr2009 000233
 Oppaaaor ::JUUSJ
 Saaaphe ::K2599001
 MISC ::
 AASSVaal ::222 SaaapheMMuipheer:11

Instrument :
 BNA_F
 ClientSampleId :
 OIL-WATER-SEPERATOR-2

QqaantMebbdd::ZZ\SS00SSRVNRP000001BBNAFNMEEH00S82Z00BB000039MM
 QqaantTife ::ASBPBNASSANDABBSF00R55P000NTCAILBRATION

TICCLibbaay ::CC\DATAABASSEN0\$T11LL
 TICInteggaionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
