


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041519\
 Data File : BF113761.D
 Acq On : 15 Apr 2019 13:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

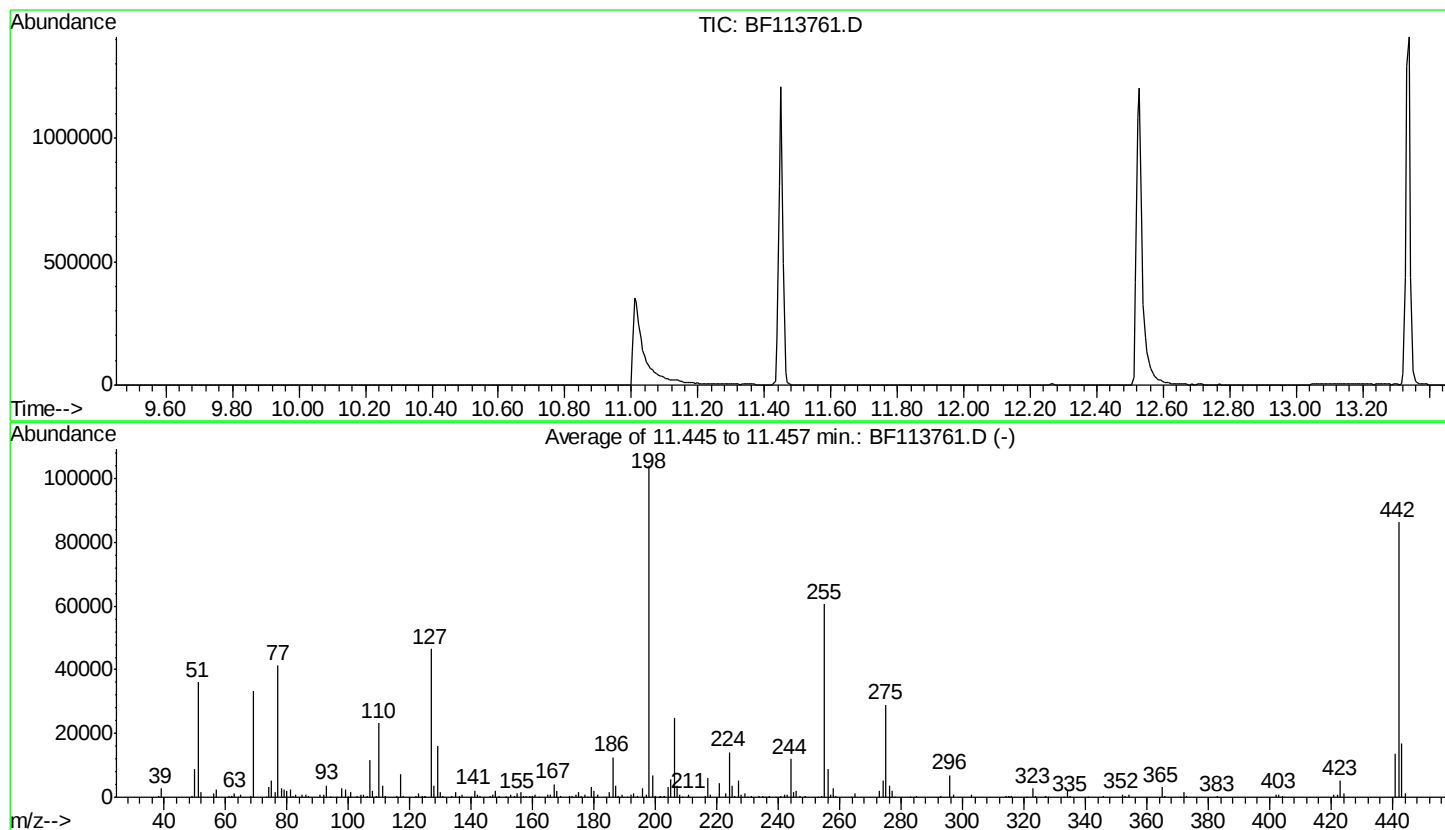

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	36064	PASS
68	69	0.00	2	1.3	430	PASS
69	198	0.00	100	32.0	33322	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.7	46525	PASS
197	198	0.00	2	0.6	650	PASS
198	198	100	100	100.0	104106	PASS
199	198	5	9	6.8	7034	PASS
275	198	10	60	27.8	28978	PASS
365	198	1	100	3.1	3208	PASS
441	198	0.01	100	13.2	13705	PASS
442	198	50	100	83.0	86368	PASS
443	442	15	24	19.4	16750	PASS