

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041520\
 Data File : BF120014.D
 Acq On : 16 Apr 2020 1:31
 Operator : MA/SJ
 Sample : L2115-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-041020

Quant Time: Apr 16 05:11:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 15 11:01:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	168201	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	640645	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	352259	20.00	ng	0.00
64) Phenanthrene-d10	11.25	188	693196	20.00	ng	0.00
76) Chrysene-d12	13.89	240	518013	20.00	ng	-0.01
87) Perylene-d12	15.31	264	381696	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	1311105	134.71	ng	0.00
7) Phenol-d6	6.36	99	1522543	121.40	ng	0.00
23) Nitrobenzene-d5	7.29	82	1167099	94.25	ng	0.00
42) 2,4,6-Tribromophenol	10.56	330	520791	120.75	ng	0.00
45) 2-Fluorobiphenyl	9.09	172	2205795	88.90	ng	0.00
79) Terphenyl-d14	12.84	244	2648943	86.05	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041520\
Data File : BF120014.D
Acq On : 16 Apr 2020 1:31
Operator : MA/SJ
Sample : L2115-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-041020

Quant Time: Apr 16 05:11:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 15 11:01:23 2020
Response via : Initial Calibration

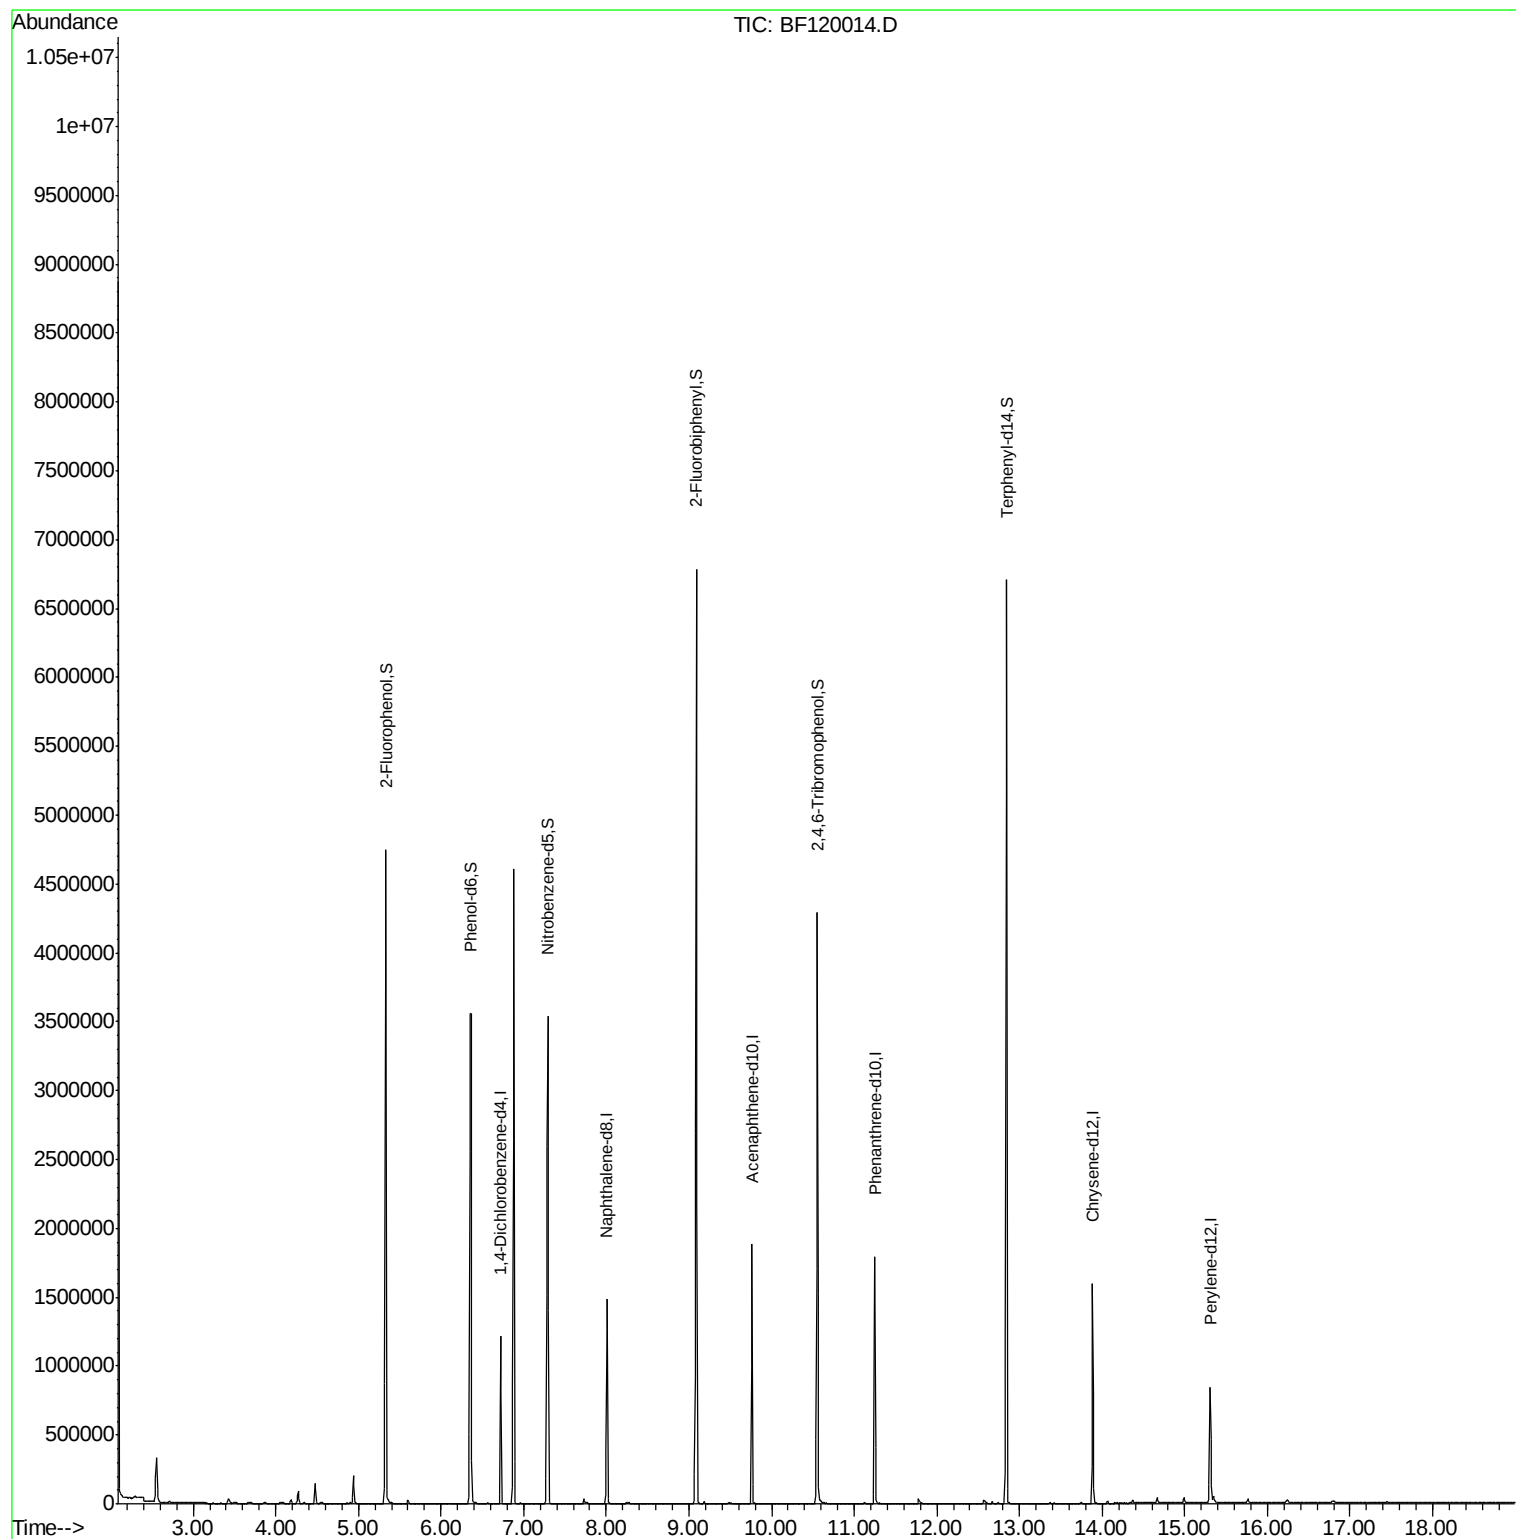







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 788
Delta R.T. -0.01 min
Lab File: BF120014.D
Acq: 16 Apr 2020 1:31

Instrument :
BNA_F
ClientSampleId :
CL-01-041020




Tot Ion:152 Resp: 168201
Ion Ratio Lower Upper
152 100
150 153.5 124.8 187.2
115 58.6 46.5 69.7

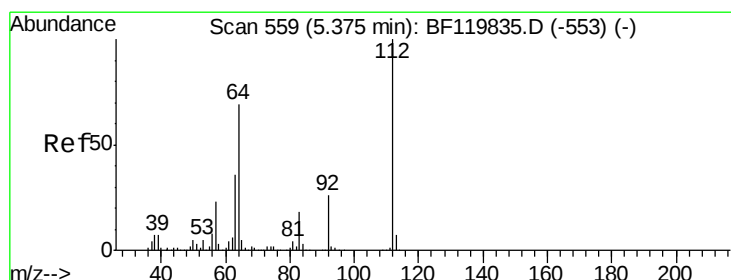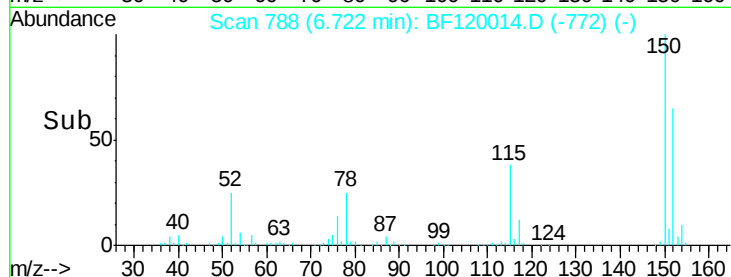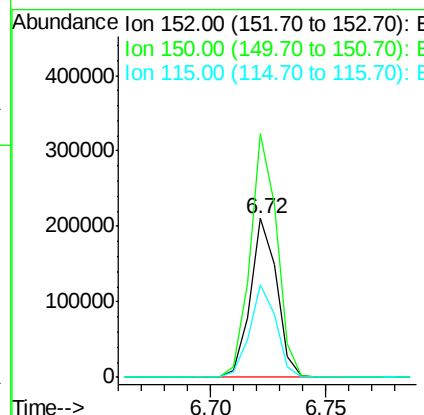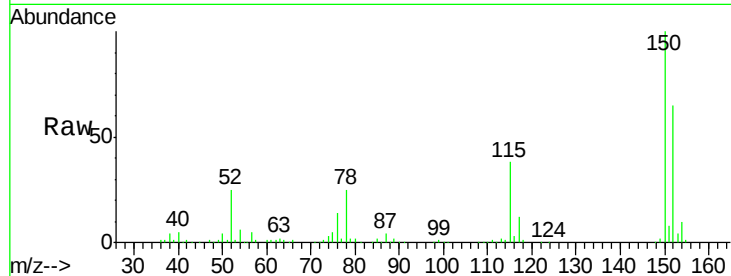

#5

2-Fluorophenol
Concen: 134.710 ng
RT: 5.33 min Scan# 552
Delta R.T. 0.01 min
Lab File: BF120014.D
Acq: 16 Apr 2020 1:31

Tgt Ion:112 Resp: 1311105
Ion Ratio Lower Upper
112 100
64 67.8 55.5 83.3
63 34.5 29.1 43.7

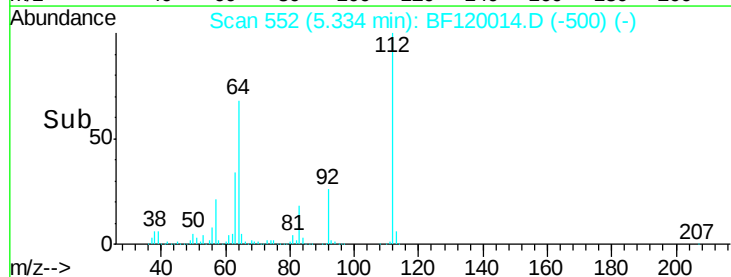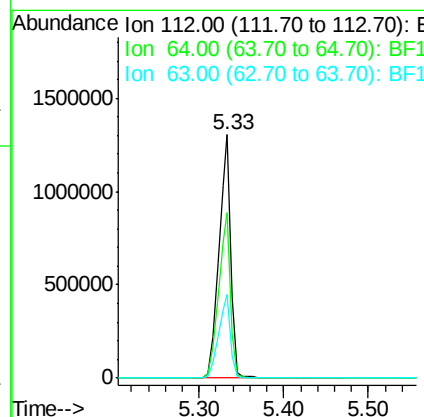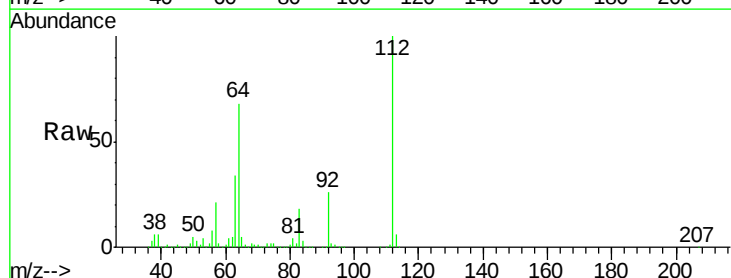



#7

Phenol-d6

Concen: 121.403 ng

RT: 6.36 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF120014.D

Acq: 16 Apr 2020 1:31

Instrument :

BNA_F

ClientSampleId :

CL-01-041020




Tot Ion: 99 Resp: 1522543

Ion Ratio Lower Upper

99 100

42 17.5 16.9 25.3

71 31.2 26.3 39.5

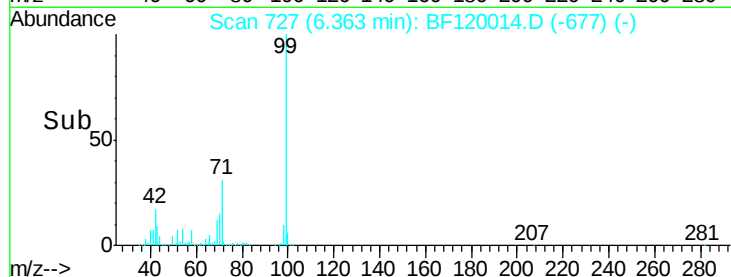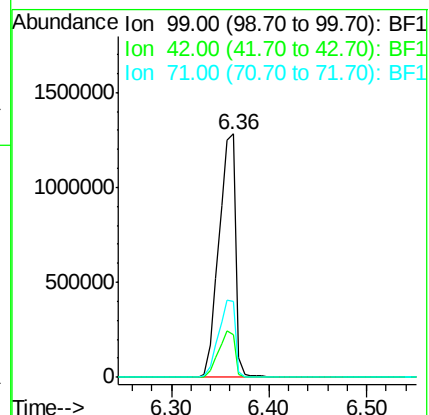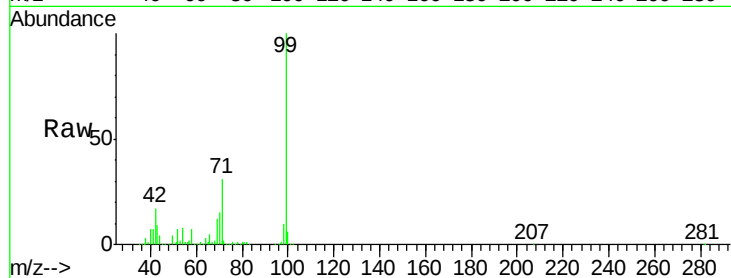

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007

Delta R.T. -0.01 min

Lab File: BF120014.D

Acq: 16 Apr 2020 1:31

Tgt Ion: 136 Resp: 640645




Ion Ratio Lower Upper

136 100

137 10.8 8.7 13.1

54 9.4 8.5 12.7

68 5.5 3.9 5.9

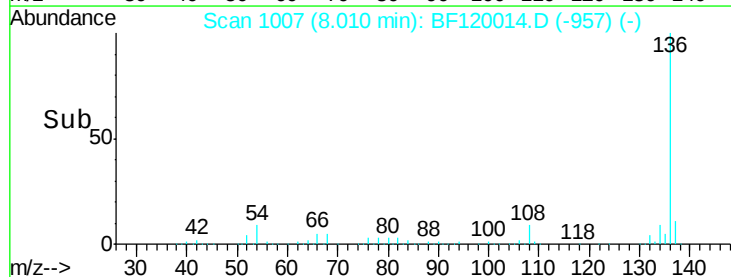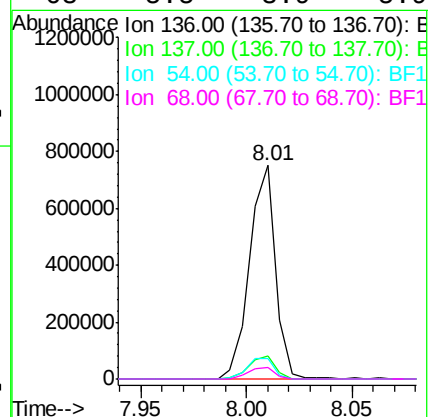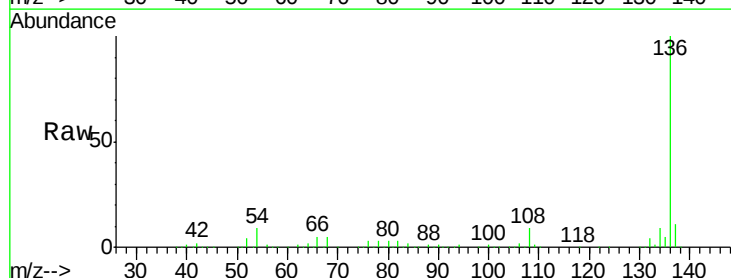







#23
 Nitrobenzene-d5
 Concen: 94.246 ng
 RT: 7.29 min Scan# 885
 Delta R.T. -0.01 min
 Lab File: BF120014.D
 Acq: 16 Apr 2020 1:31

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-041020

Tot Ion: 82 Resp: 1167099
 Ion Ratio Lower Upper
 82 100
 128 45.3 36.2 54.4
 54 60.6 50.4 75.6

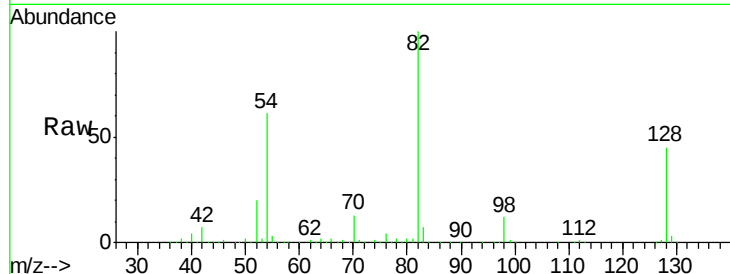


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

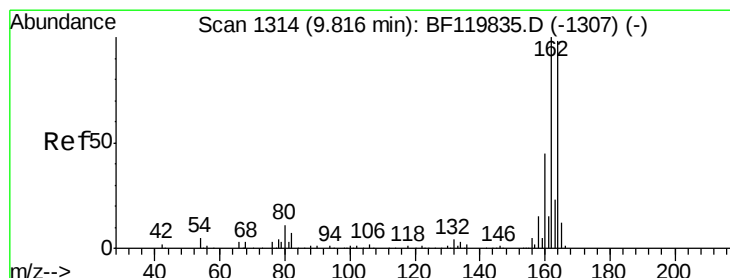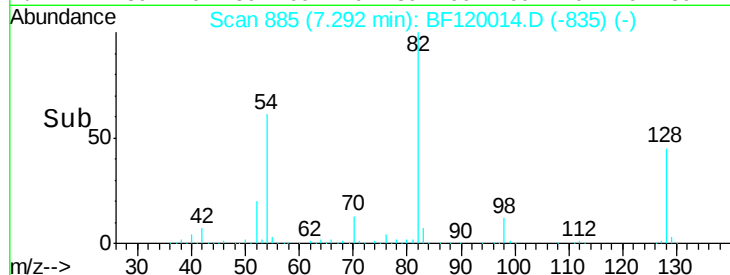
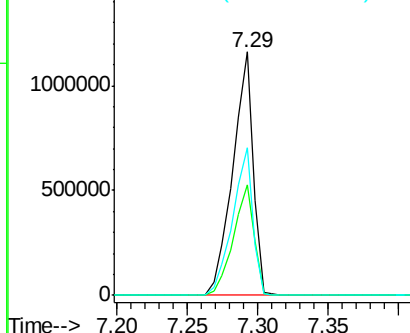



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.76 min Scan# 1305
 Delta R.T. -0.01 min
 Lab File: BF120014.D
 Acq: 16 Apr 2020 1:31

Tgt Ion: 164 Resp: 352259
 Ion Ratio Lower Upper
 164 100
 162 101.5 81.9 122.9
 160 46.1 36.6 54.8

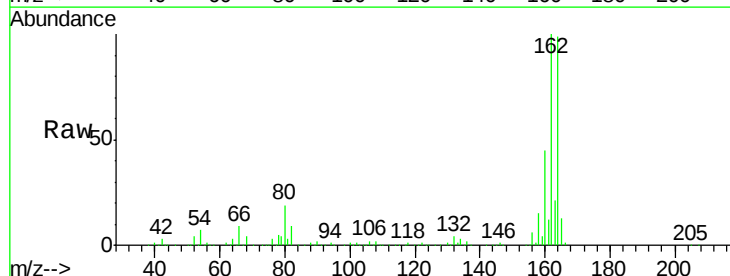

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1

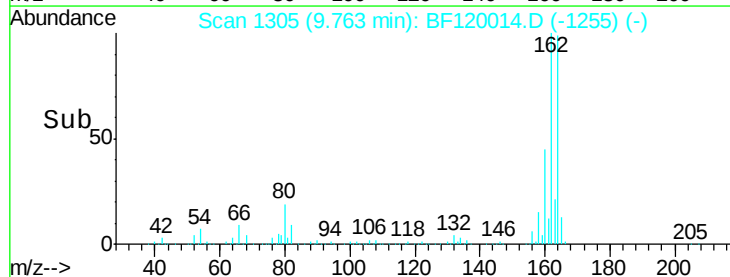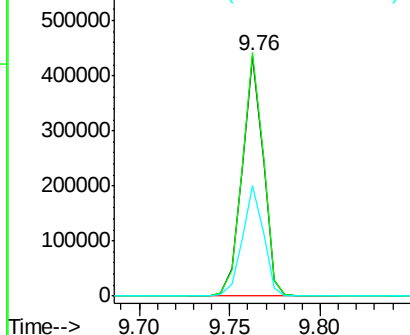


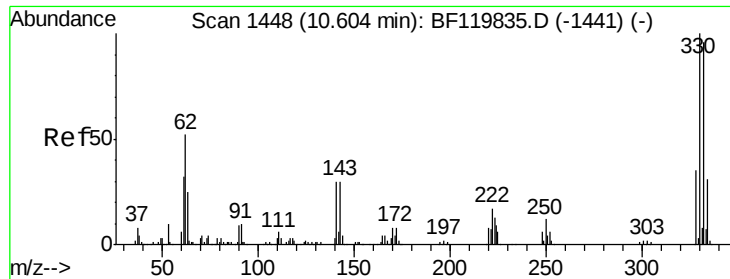




#42
 2,4,6-Tribromophenol
 Concen: 120.753 ng
 RT: 10.56 min Scan# 1440
 Delta R.T. -0.01 min
 Lab File: BF120014.D
 Acq: 16 Apr 2020 1:31

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-041020

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	76.8	115.2
141	33.6	25.1	37.7

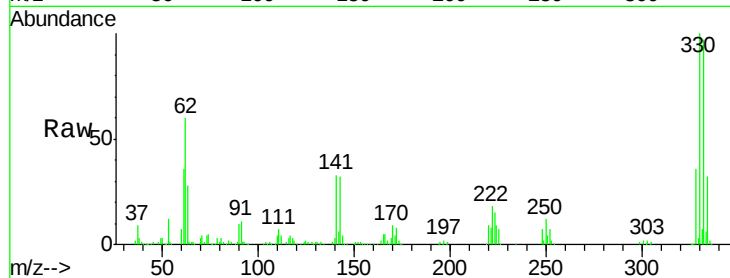


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

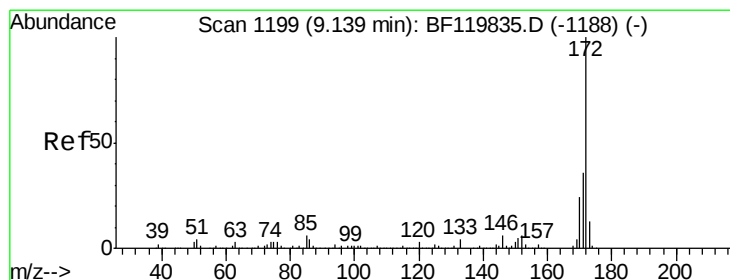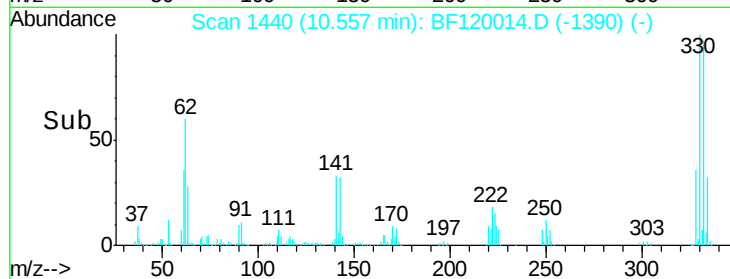
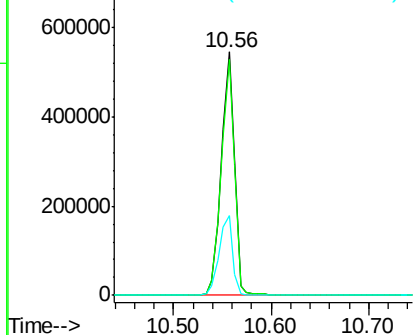



#45
 2-Fluorobiphenyl
 Concen: 88.905 ng
 RT: 9.09 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: BF120014.D
 Acq: 16 Apr 2020 1:31

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	28.9	43.3
170	24.4	19.4	29.2

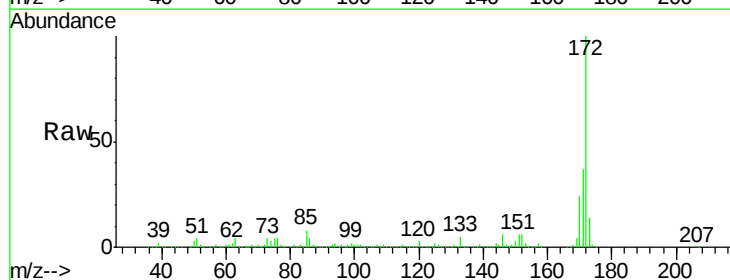

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



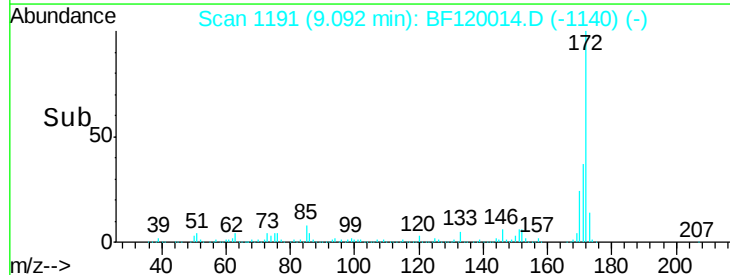
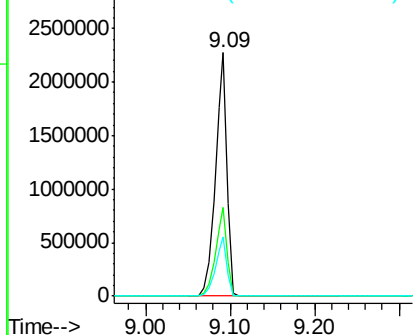


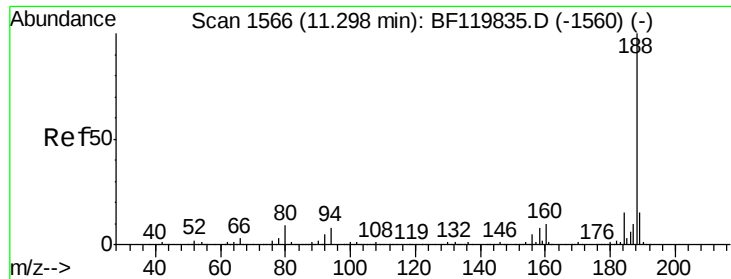

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.25 min Scan# 1558
Delta R.T. -0.01 min
Lab File: BF120014.D
Acq: 16 Apr 2020 1:31




Instrument :
BNA_F
ClientSampleId :
CL-01-041020


Tot Ion:188 Resp: 693196
Ion Ratio Lower Upper
188 100
94 8.1 6.7 10.1
80 8.2 7.4 11.2

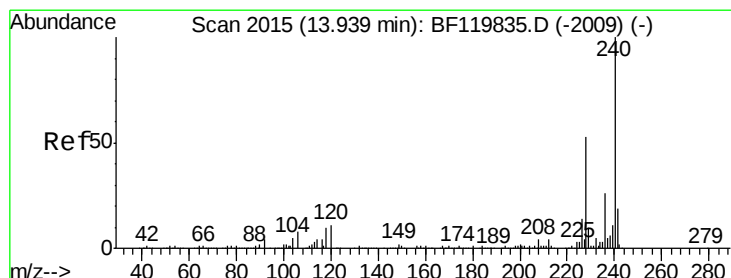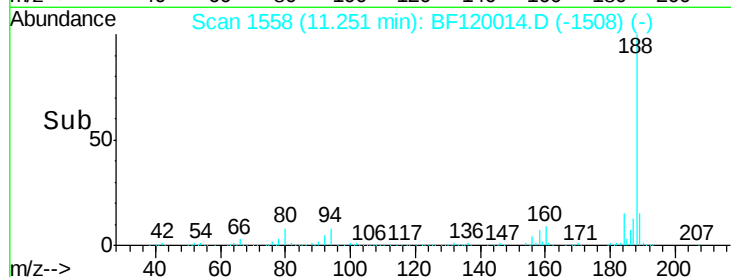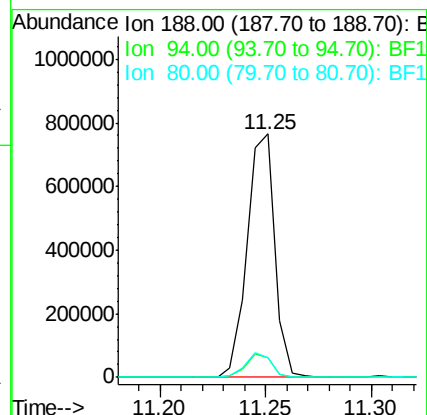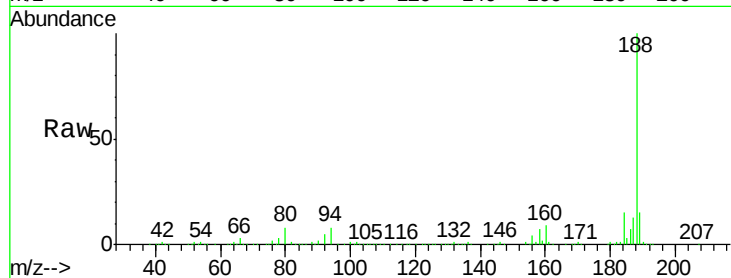

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.89 min Scan# 2006
Delta R.T. -0.01 min
Lab File: BF120014.D
Acq: 16 Apr 2020 1:31

Tgt Ion:240 Resp: 518013
Ion Ratio Lower Upper
240 100
120 10.9 9.0 13.6
236 25.6 20.7 31.1

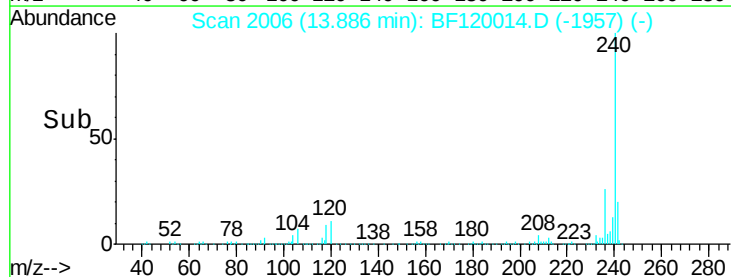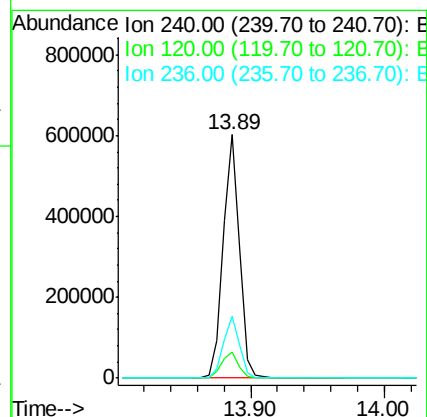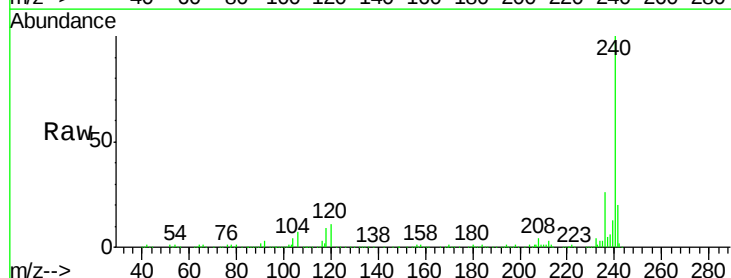

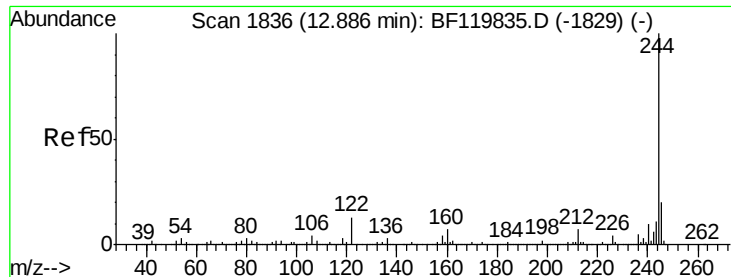

#79

Terphenyl-d14

Concen: 86.045 ng

RT: 12.84 min Scan# 1829

Delta R.T. -0.00 min

Lab File: BF120014.D

Acq: 16 Apr 2020 1:31

Instrument :

BNA_F

ClientSampleId :

CL-01-041020


Tot Ion:244 Resp: 2648943

Ion Ratio Lower Upper

244 100

212 7.4 5.4 8.0




122 13.8 10.3 15.5

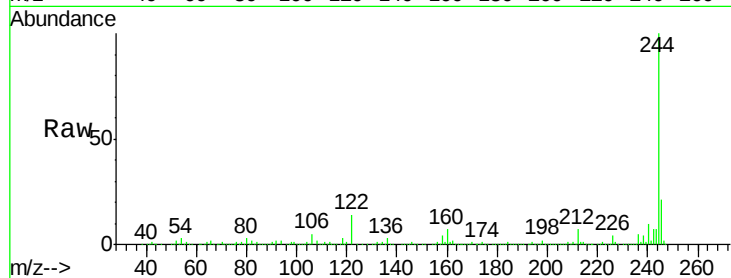

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

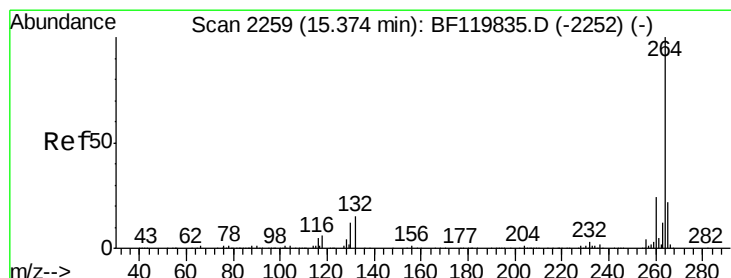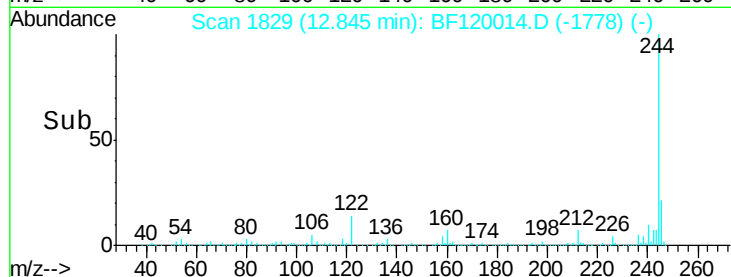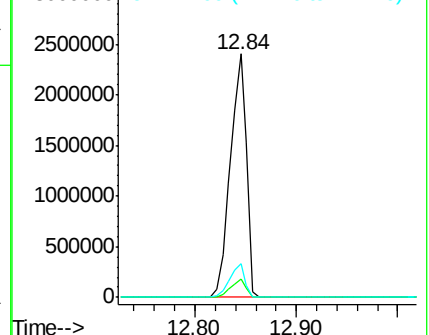

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.31 min Scan# 2248

Delta R.T. -0.00 min

Lab File: BF120014.D

Acq: 16 Apr 2020 1:31


Tgt Ion:264 Resp: 381696

Ion Ratio Lower Upper

264 100

260 24.2 19.3 28.9

265 21.1 17.6 26.4

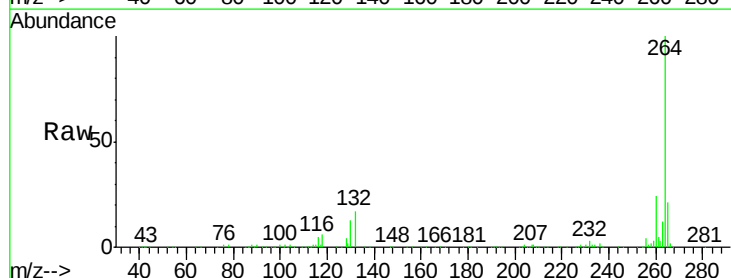

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

