

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041520\
Data File : BF119987.D
Acq On : 15 Apr 2020 12:19
Operator : MA/SJ
Sample : PB128205BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128205BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.328	545	551	554	rBV	5128469	5454804	74.08%	11.748%
2	6.363	720	727	730	rBV	4465638	5374467	72.99%	11.575%
3	6.722	784	788	792	rBV	1272298	1072035	14.56%	2.309%
4	6.881	810	815	818	rBV	4654257	4474325	60.76%	9.636%
5	7.292	878	885	888	rBV	3613674	3661020	49.72%	7.885%
6	8.010	1002	1007	1010	rBV	1602113	1420499	19.29%	3.059%
7	9.092	1184	1191	1194	rBV	7117099	6643445	90.22%	14.308%
8	9.763	1300	1305	1309	rBV	2052869	1680650	22.82%	3.620%
9	10.557	1434	1440	1443	rBV	4469065	4402168	59.78%	9.481%
10	11.251	1554	1558	1561	rBV	2203893	1808818	24.56%	3.896%
11	12.845	1823	1829	1832	rBV	6400031	7363559	100.00%	15.859%
12	13.886	2002	2006	2010	rBV	1760154	1642409	22.30%	3.537%
13	15.310	2243	2248	2253	rBV	1211221	1434455	19.48%	3.089%


Sum of corrected areas: 46432654

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041520\
Data File : BF119987.D
Acq On : 15 Apr 2020 12:19
Operator : MA/SJ
Sample : PB128205BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128205BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

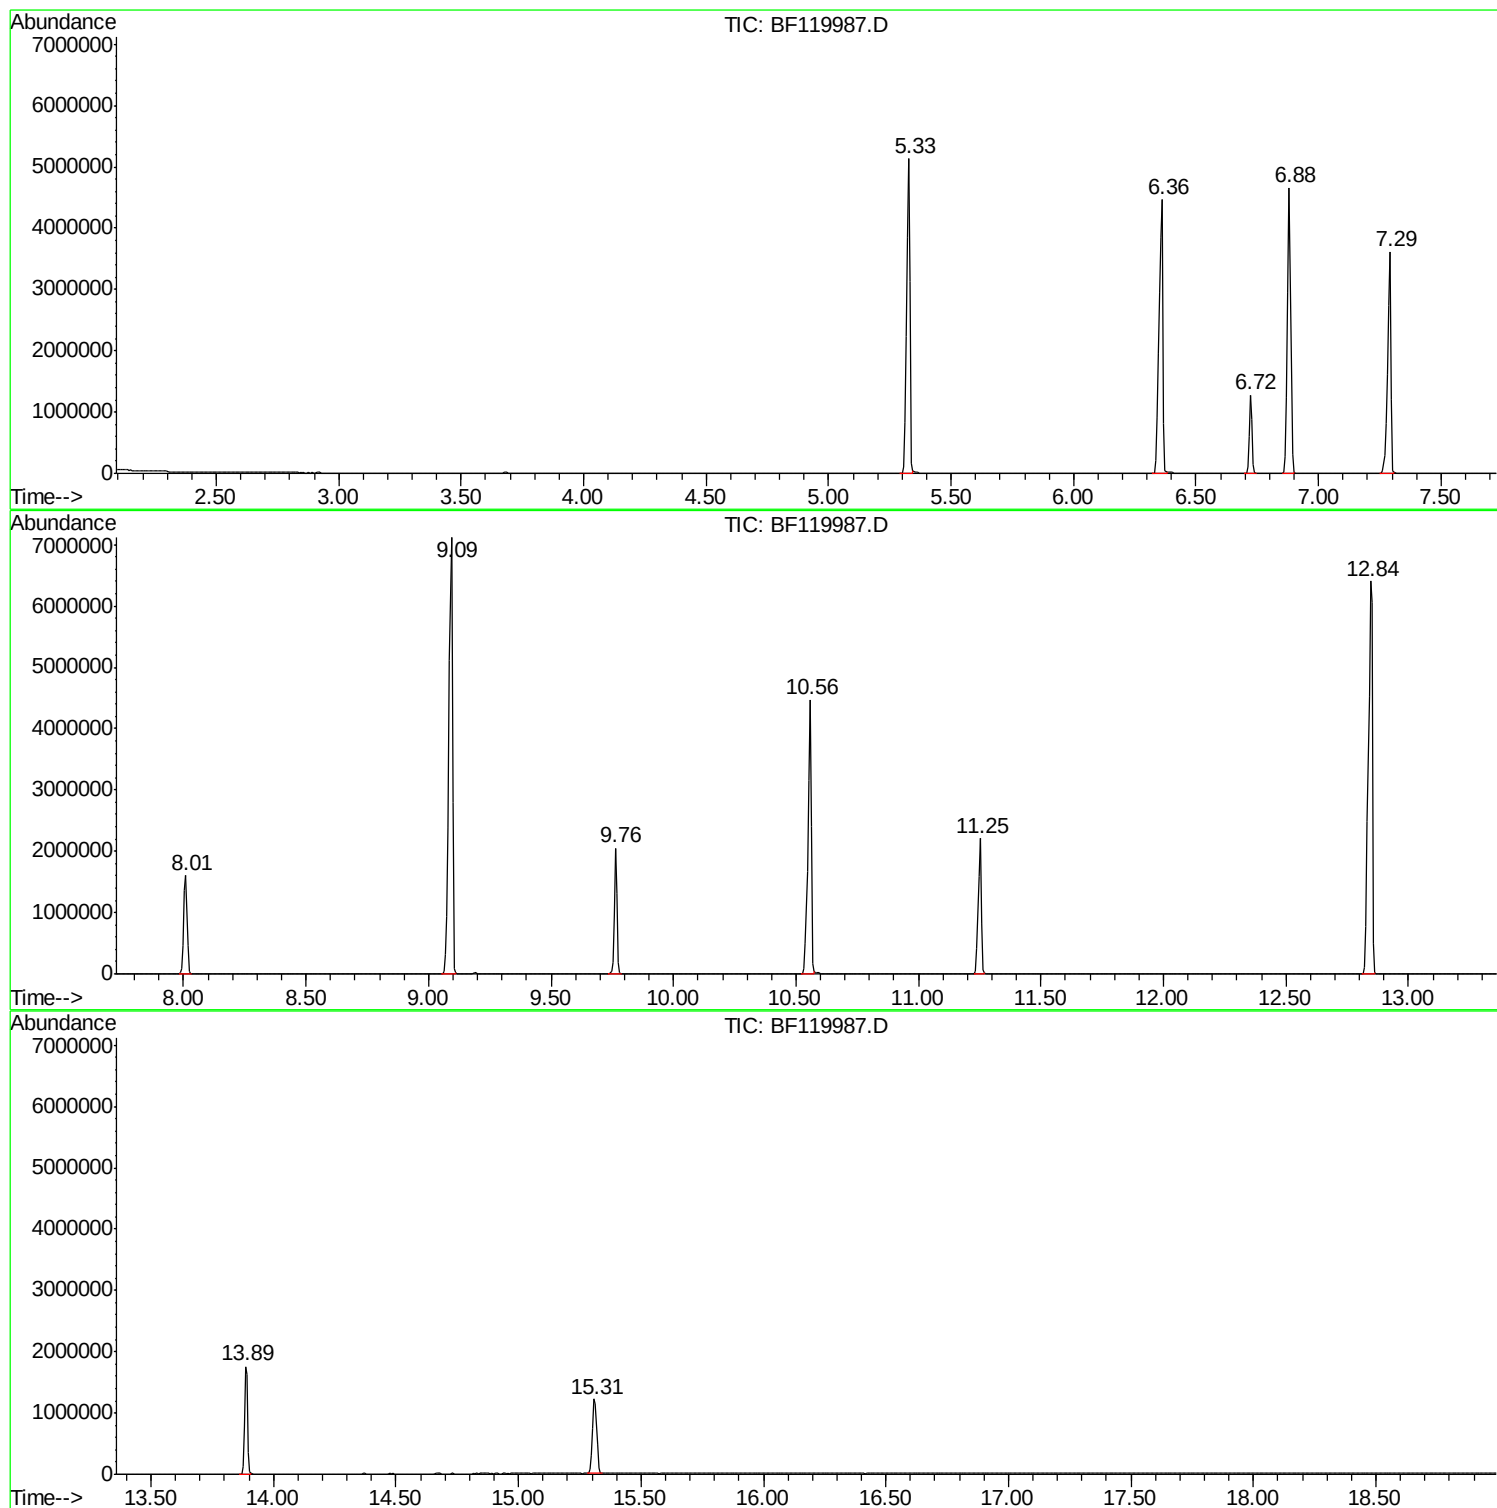

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041520\
Data File : BF119987.D
Acq On : 15 Apr 2020 12:19
Operator : MA/SJ
Sample : PB128205BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128205BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041520\
Data File : BF119987.D
Acq On : 15 Apr 2020 12:19
Operator : MA/SJ
Sample : PB128205BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128205BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc