

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041520\
 Data File : BF120016.D
 Acq On : 16 Apr 2020 2:25
 Operator : MA/SJ
 Sample : PB128243BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128243BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.940	481	485	493	rBV	53800	72289	1.04%	0.187%
2	5.340	548	553	556	rBV	3735347	3761551	54.03%	9.742%
3	6.357	720	726	729	rBV	3649758	3630837	52.15%	9.403%
4	6.722	784	788	792	rBV	1208260	953873	13.70%	2.470%
5	6.881	810	815	818	rBV	4728966	4285292	61.55%	11.098%
6	7.287	878	884	887	rBV	2979634	3527736	50.67%	9.136%
7	8.004	1001	1006	1010	rBV	1290787	1255560	18.03%	3.252%
8	9.092	1184	1191	1194	rBV	5600880	6445645	92.58%	16.693%
9	9.763	1299	1305	1308	rBV	1667435	1467853	21.08%	3.801%
10	10.551	1434	1439	1442	rBV	2601319	2242375	32.21%	5.807%
11	11.251	1553	1558	1561	rBV	1721995	1594696	22.91%	4.130%
12	12.845	1823	1829	1832	rBV	6701793	6962033	100.00%	18.030%
13	13.886	2002	2006	2010	rBV	1599051	1375313	19.75%	3.562%
14	15.310	2242	2248	2252	rBV	903960	1038253	14.91%	2.689%


Sum of corrected areas: 38613306

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041520\
Data File : BF120016.D
Acq On : 16 Apr 2020 2:25
Operator : MA/SJ
Sample : PB128243BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128243BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

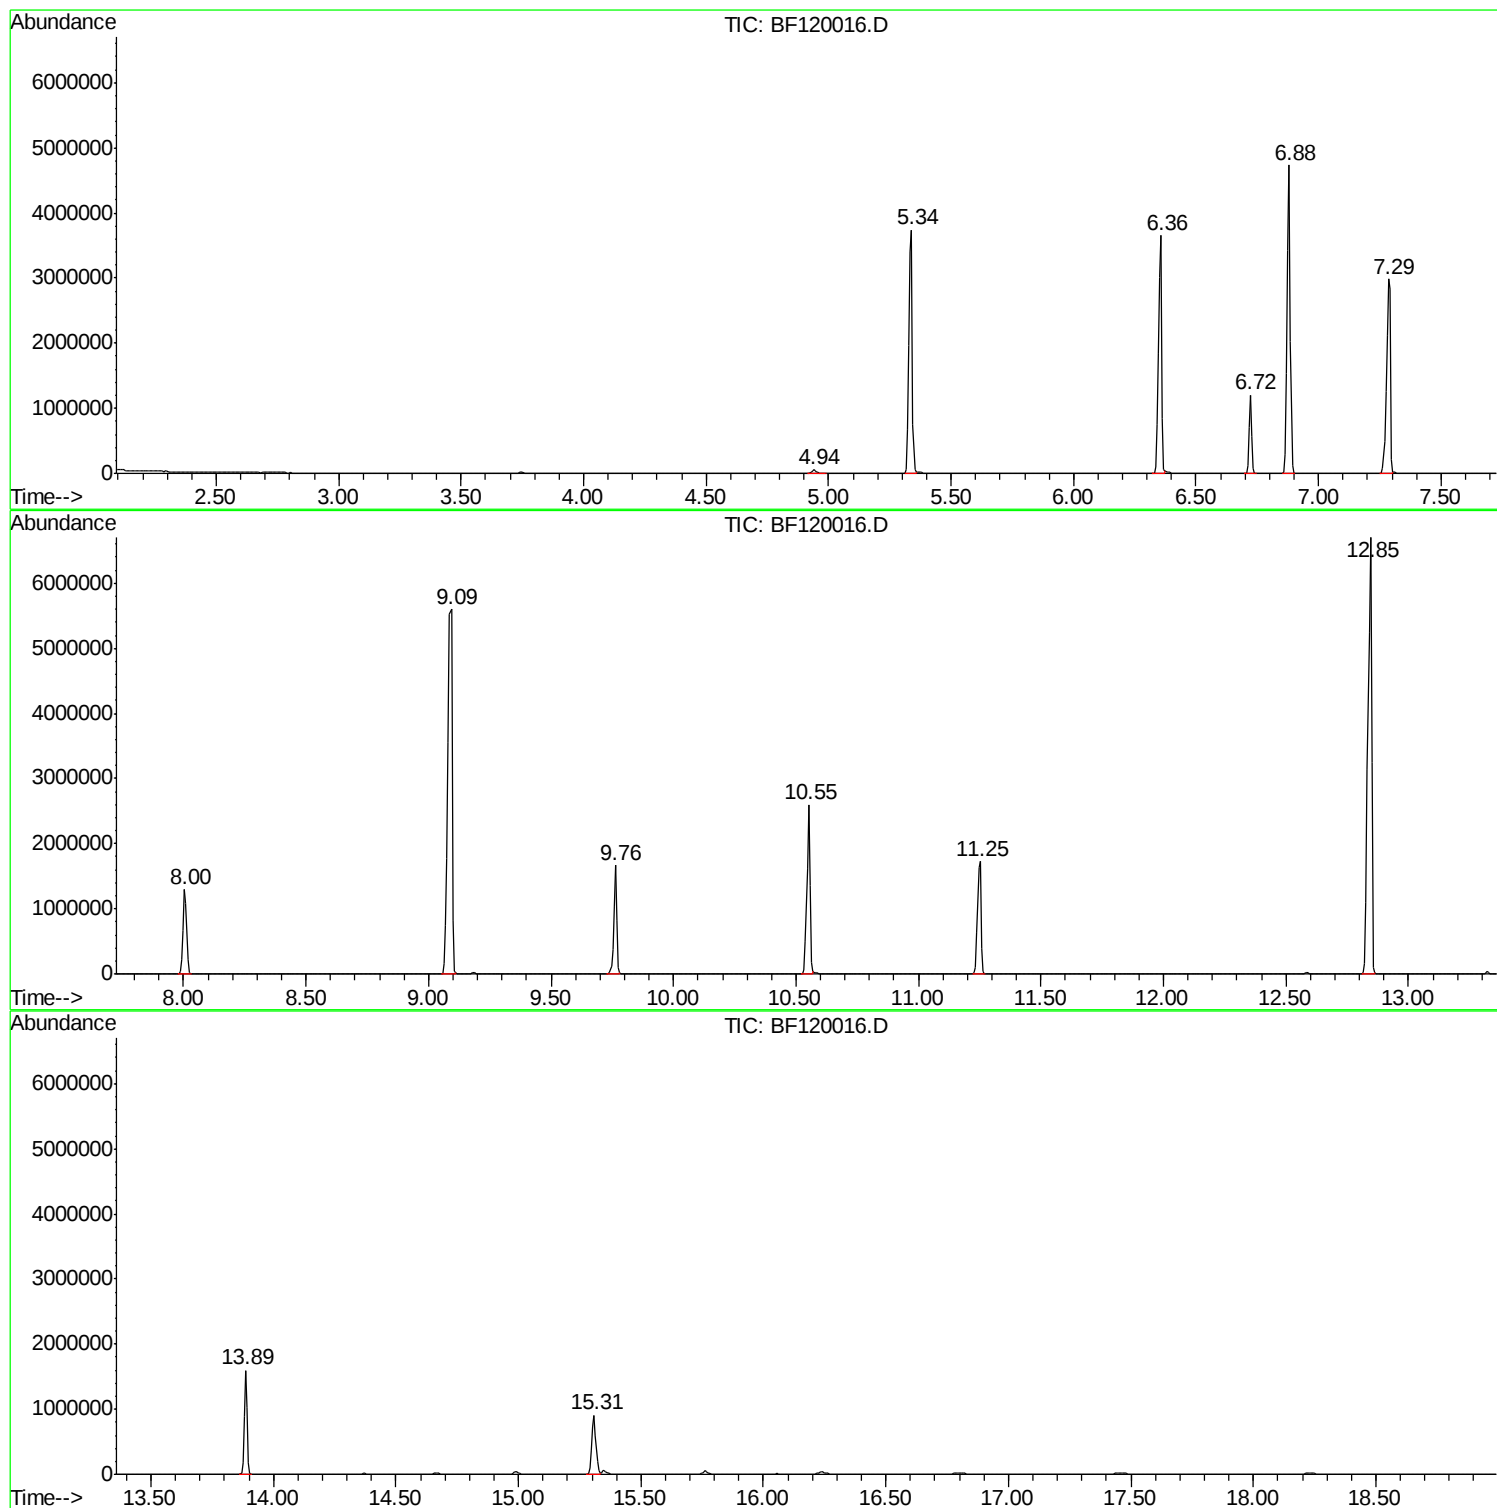

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041520\
Data File : BF120016.D
Acq On : 16 Apr 2020 2:25
Operator : MA/SJ
Sample : PB128243BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128243BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041520\
Data File : BF120016.D
Acq On : 16 Apr 2020 2:25
Operator : MA/SJ
Sample : PB128243BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128243BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc