


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041520\
 Data File : BF119981.D
 Acq On : 15 Apr 2020 9:37
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 16 10:48:04 2020

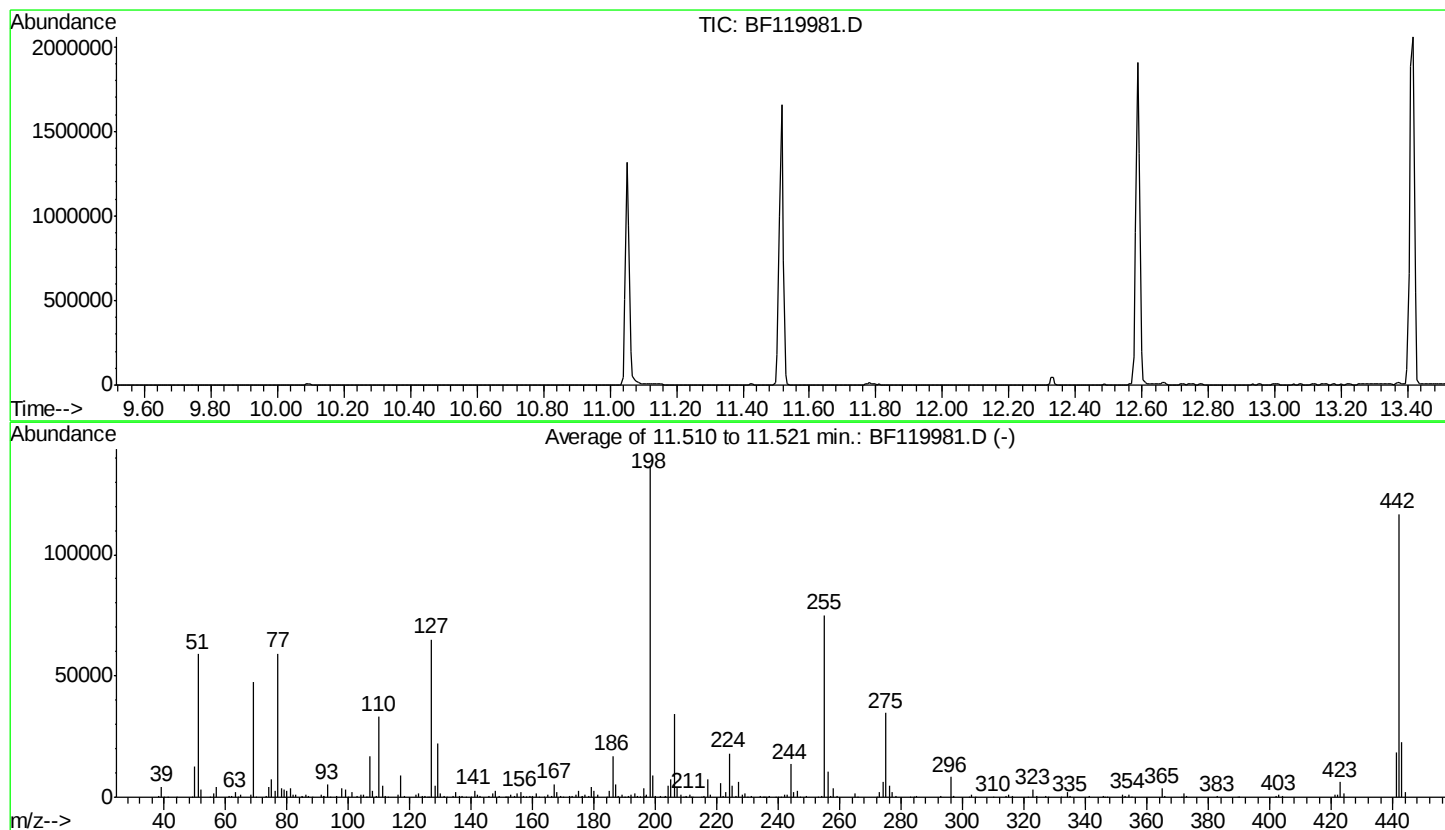

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	58951	PASS
68	69	0.00	2	1.7	829	PASS
69	198	0.00	100	34.9	47664	PASS
70	69	0.00	2	0.3	139	PASS
127	198	10	80	47.6	65066	PASS
197	198	0.00	2	0.7	901	PASS
198	198	100	100	100.0	136690	PASS
199	198	5	9	6.4	8729	PASS
275	198	10	60	25.4	34765	PASS
365	198	1	100	2.6	3534	PASS
441	198	0.01	100	13.7	18739	PASS
442	198	50	100	85.4	116712	PASS
443	442	15	24	19.5	22739	PASS