


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041520\
 Data File : BF120005.D
 Acq On : 15 Apr 2020 20:59
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 16 10:48:04 2020

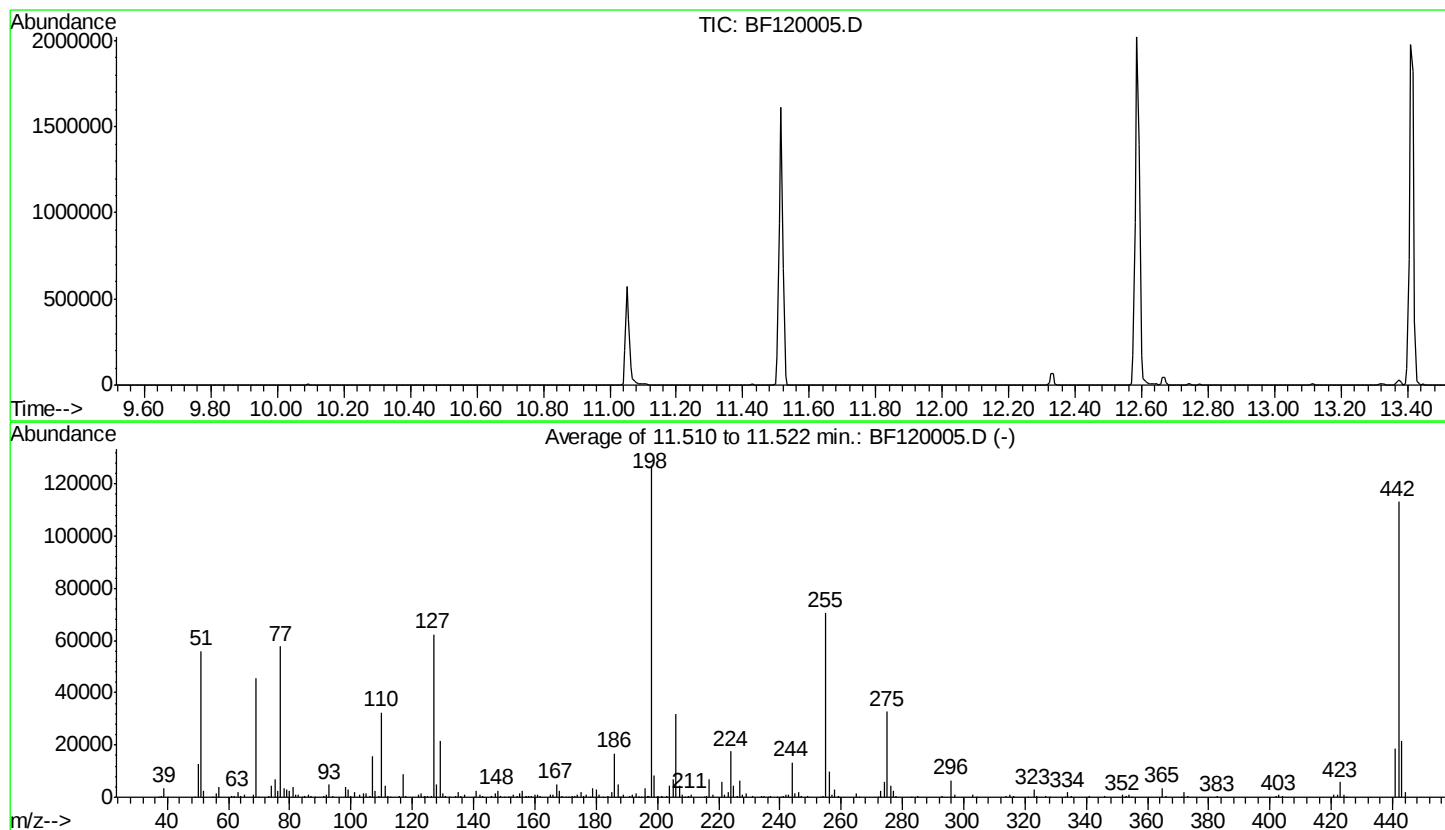

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	55912	PASS
68	69	0.00	2	1.7	791	PASS
69	198	0.00	100	35.9	45653	PASS
70	69	0.00	2	0.3	145	PASS
127	198	10	80	49.2	62450	PASS
197	198	0.00	2	0.4	500	PASS
198	198	100	100	100.0	126992	PASS
199	198	5	9	6.7	8526	PASS
275	198	10	60	25.8	32760	PASS
365	198	1	100	2.8	3567	PASS
441	198	0.01	100	14.5	18469	PASS
442	198	50	100	89.1	113202	PASS
443	442	15	24	18.9	21410	PASS