
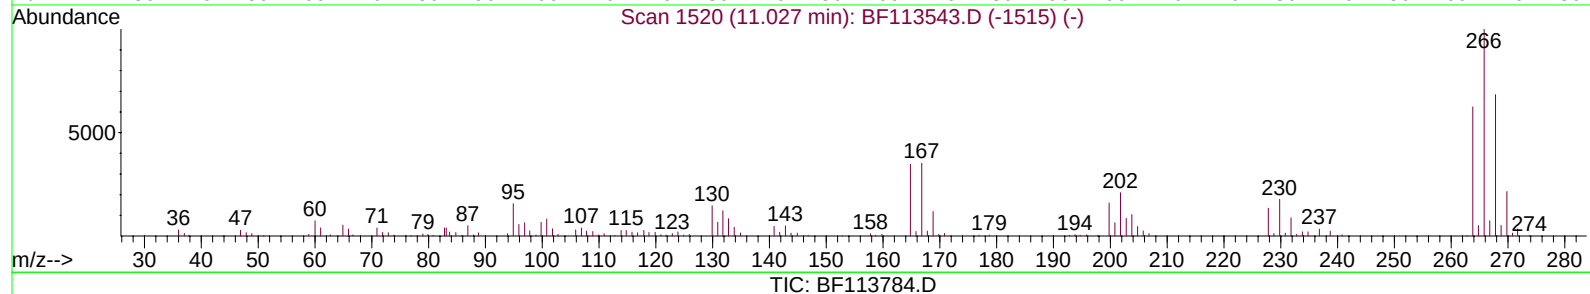
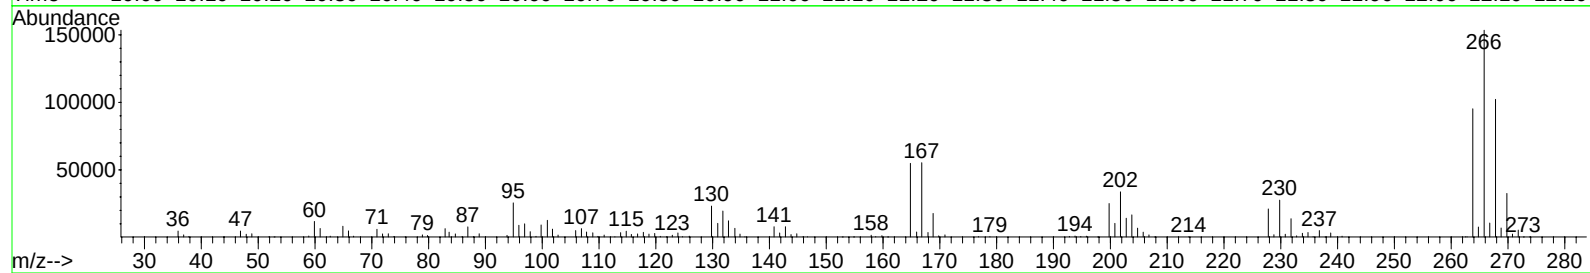


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF041619\
Data File : BF113784.D
Acq On : 16 Apr 2019 10:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 19:19:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

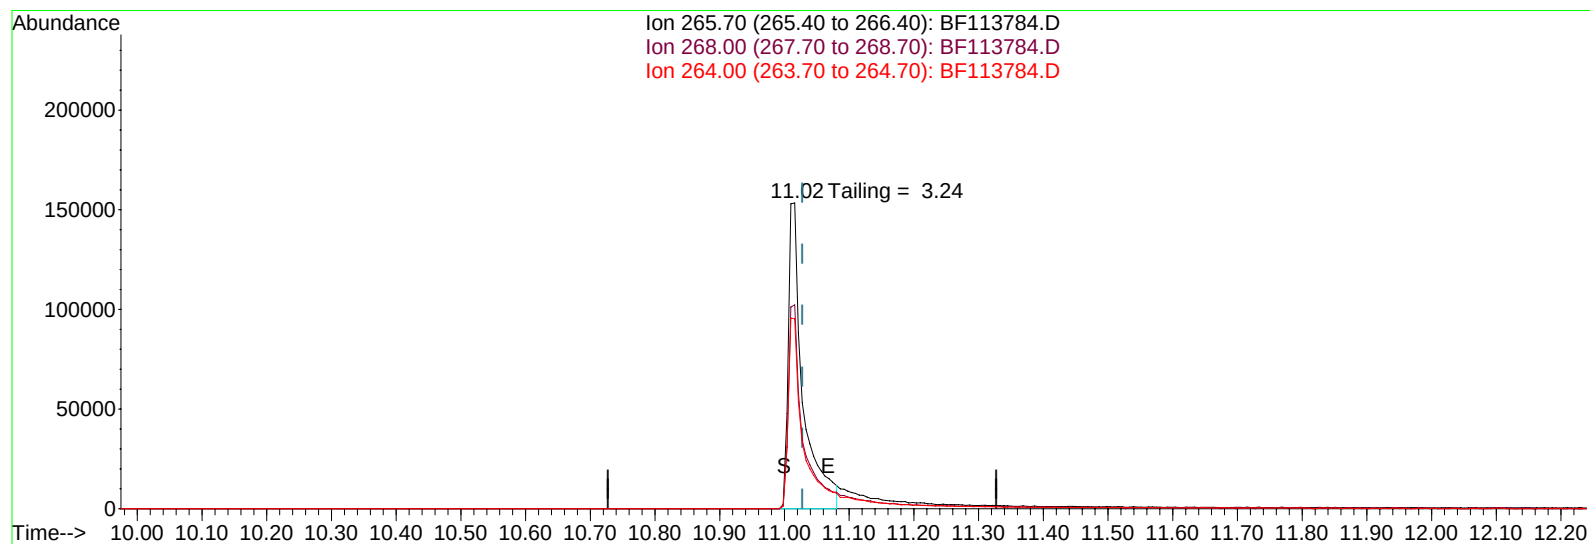

(70) Pentachlorophenol (C)




11.016min (-0.012) 82794.67ng

response 290789

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	66.67
264.00	61.50	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF041619\
 Data File : BF113784.D
 Acq On : 16 Apr 2019 10:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 19:19:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration

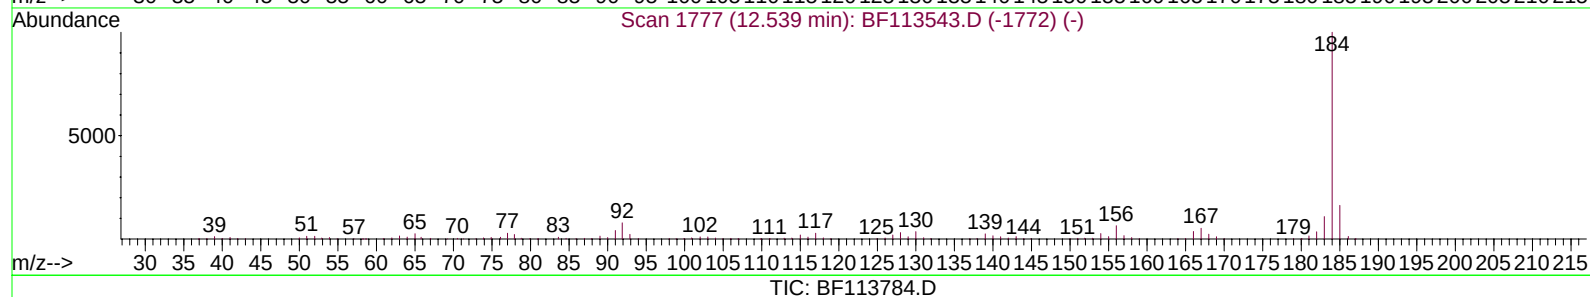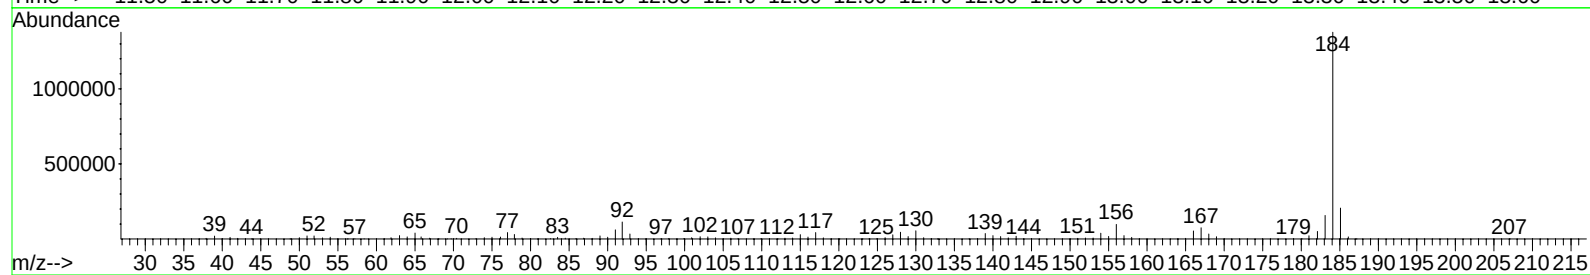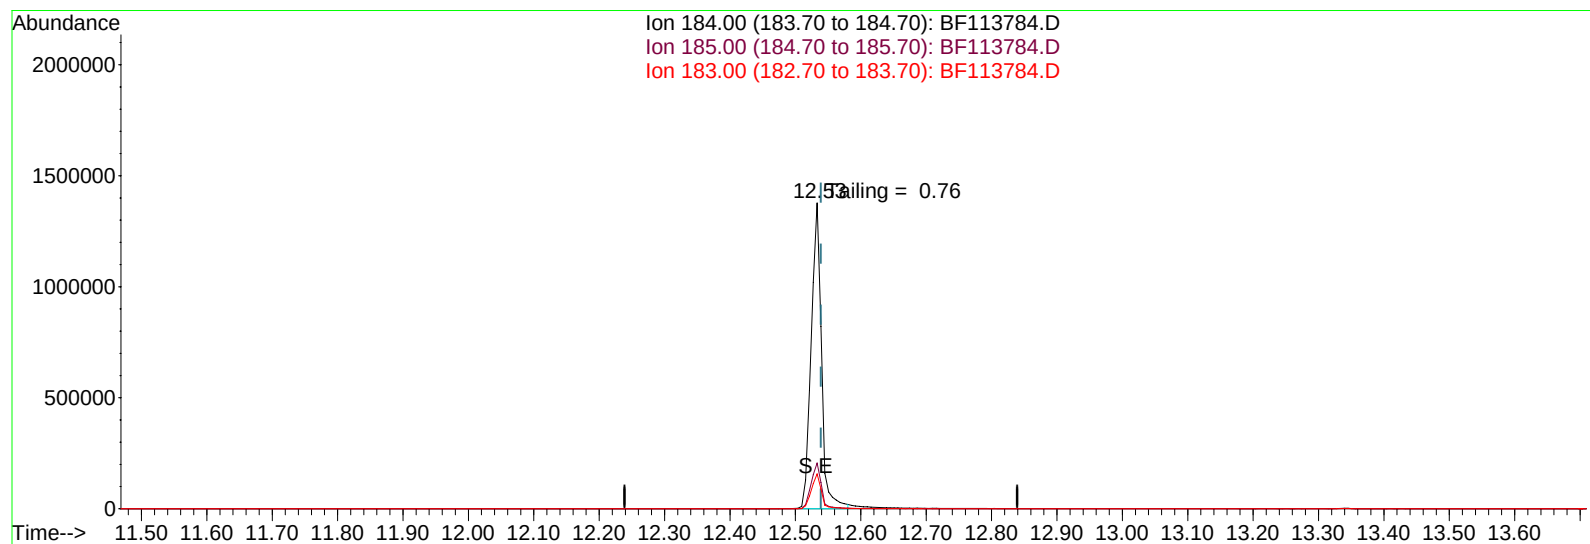

(77) Benzidine

12.533min (-0.006) 42002.02ng

response 1557233

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.99
183.00	11.20	11.41
0.00	0.00	0.00