

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041619\
 Data File : BF113803.D
 Acq On : 16 Apr 2019 19:51
 Operator : JU/SJ
 Sample : K2411-03 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-16-S

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.298	542	546	577	rBV	571789	1201206	81.59%	7.204%
2	6.334	719	722	738	rBV	681772	1218136	82.74%	7.305%
3	6.451	738	742	764	rVB	1121319	1397318	94.91%	8.380%
4	6.669	776	779	796	rVB	783715	743486	50.50%	4.459%
5	6.828	802	806	824	rBV	1043955	1072711	72.86%	6.433%
6	7.240	873	876	904	rBV	495577	808376	54.91%	4.848%
7	7.957	994	998	1023	rBV	689896	933575	63.41%	5.599%
8	9.028	1176	1180	1193	rBV	1449472	1472290	100.00%	8.829%
9	9.434	1246	1249	1256	rBV	73200	92180	6.26%	0.553%
10	9.575	1268	1273	1281	rBV	30092	33968	2.31%	0.204%
11	9.704	1291	1295	1309	rBV	884253	884377	60.07%	5.304%
12	10.498	1427	1430	1446	rBV	439027	645968	43.88%	3.874%
13	11.186	1544	1547	1560	rBV	722681	879198	59.72%	5.273%
14	11.280	1560	1563	1569	rVB	15935	22787	1.55%	0.137%
15	11.727	1636	1639	1645	rBV3	50357	78600	5.34%	0.471%
16	12.404	1750	1754	1761	rBV	148256	149262	10.14%	0.895%
17	12.504	1769	1771	1778	rBV	18566	29406	2.00%	0.176%
18	12.633	1788	1793	1800	rBV	136110	166099	11.28%	0.996%
19	12.763	1811	1815	1823	rBV	1350050	1286068	87.35%	7.713%
20	12.857	1827	1831	1835	rVB2	12421	17424	1.18%	0.104%
21	12.963	1847	1849	1853	rVB2	16747	16411	1.11%	0.098%
22	13.027	1858	1860	1863	rBV	16342	15055	1.02%	0.090%
23	13.069	1864	1867	1872	rVB3	17272	19000	1.29%	0.114%
24	13.339	1909	1913	1915	rBV3	23109	21888	1.49%	0.131%
25	13.604	1952	1958	1961	rBV3	15311	26985	1.83%	0.162%
26	13.663	1965	1968	1971	rVB4	21978	23295	1.58%	0.140%
27	13.827	1988	1996	2008	rBV2	893516	1354658	92.01%	8.124%
28	13.980	2019	2022	2024	rBV2	36854	32826	2.23%	0.197%
29	14.045	2031	2033	2037	rBV4	12110	17589	1.19%	0.105%
30	14.221	2061	2063	2066	rVB2	21988	18638	1.27%	0.112%
31	14.280	2071	2073	2077	rVB2	57391	55765	3.79%	0.334%
32	14.574	2120	2123	2126	rVB	77464	74646	5.07%	0.448%
33	14.845	2165	2169	2172	rBV	119386	165244	11.22%	0.991%
34	14.880	2172	2175	2180	rVV2	109659	163464	11.10%	0.980%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041619\
Data File : BF113803.D
Acq On : 16 Apr 2019 19:51
Operator : JU/SJ
Sample : K2411-03 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-16-S

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.951	2184	2187	2192	rVB	41586	49371	3.35%	0.296%
36	15.121	2213	2216	2220	rBV	72547	79799	5.42%	0.479%
37	15.186	2223	2227	2230	rVV	91625	113187	7.69%	0.679%
38	15.233	2230	2235	2248	rVB	762125	1124025	76.35%	6.741%
39	15.621	2297	2301	2305	rVB	72277	94711	6.43%	0.568%
40	16.074	2374	2378	2382	rVB	50354	75885	5.15%	0.455%


Sum of corrected areas: 16674877

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041619\
Data File : BF113803.D
Acq On : 16 Apr 2019 19:51
Operator : JU/SJ
Sample : K2411-03 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-16-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

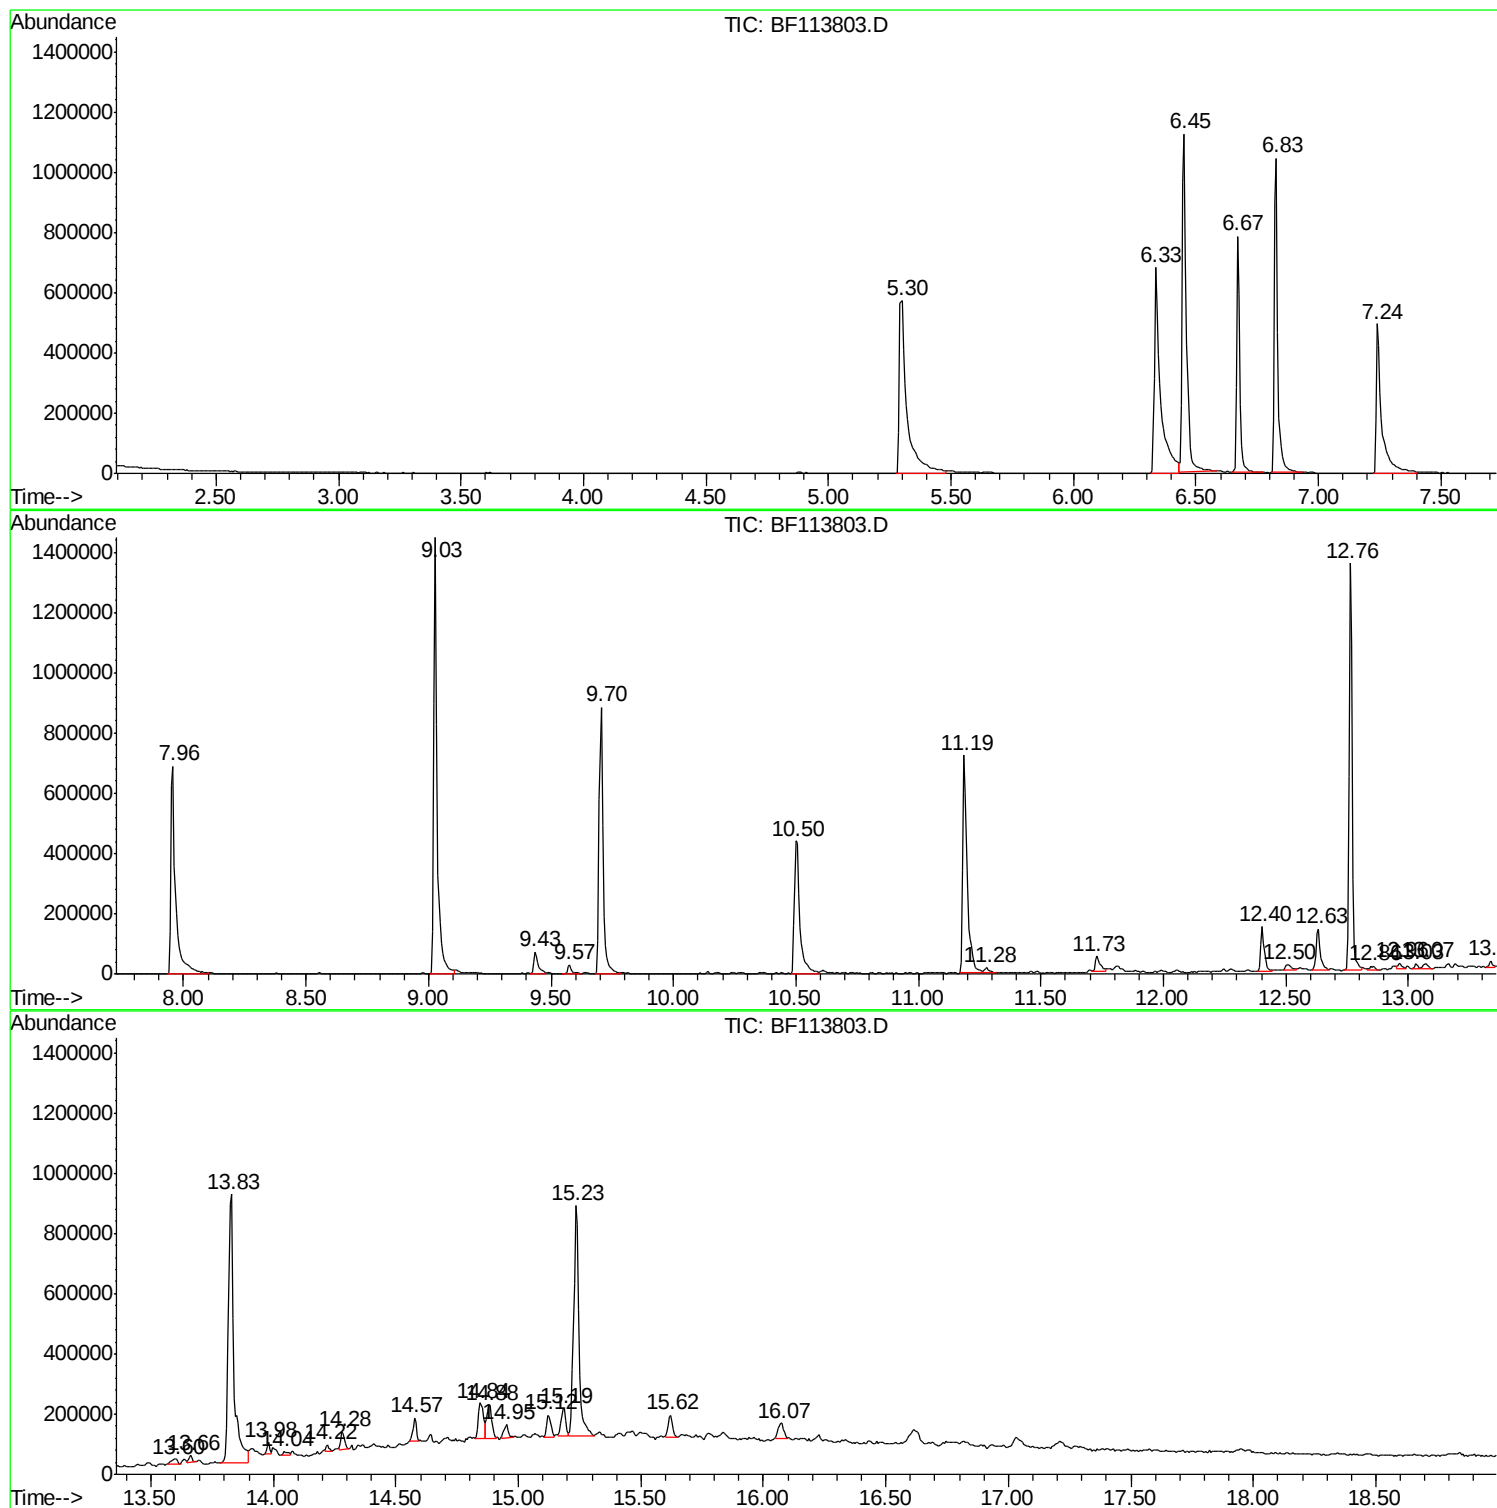

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041619\
Data File : BF113803.D
Acq On : 16 Apr 2019 19:51
Operator : JU/SJ
Sample : K2411-03 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-16-S







Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.45 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.45	37.59 ng	1397320	1,4-Dichlorobenzene-d4	6.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	16
4		5-Aminoindole	132	C8H8N2	005192-03-0	16
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

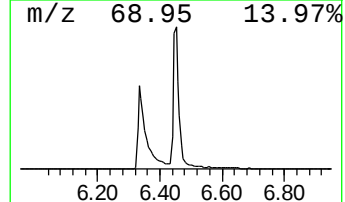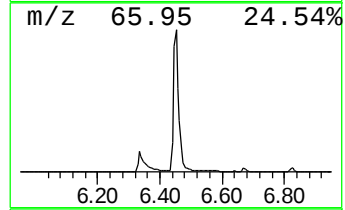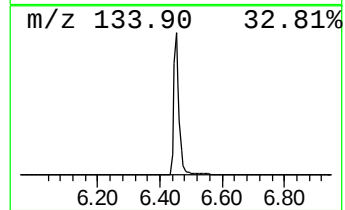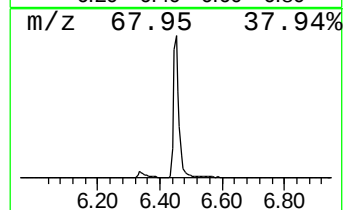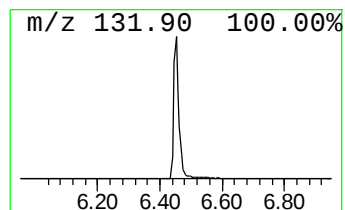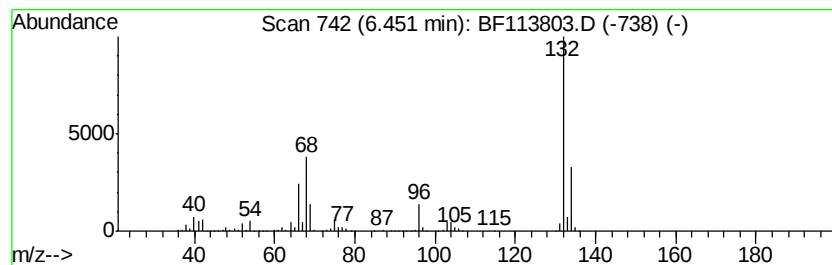

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041619\
Data File : BF113803.D
Acq On : 16 Apr 2019 19:51
Operator : JU/SJ
Sample : K2411-03 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-16-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.45	6.45	37.6	ng	1397320	1	6.67	743486	20.0