


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041619\
 Data File : BF113784.D
 Acq On : 16 Apr 2019 10:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

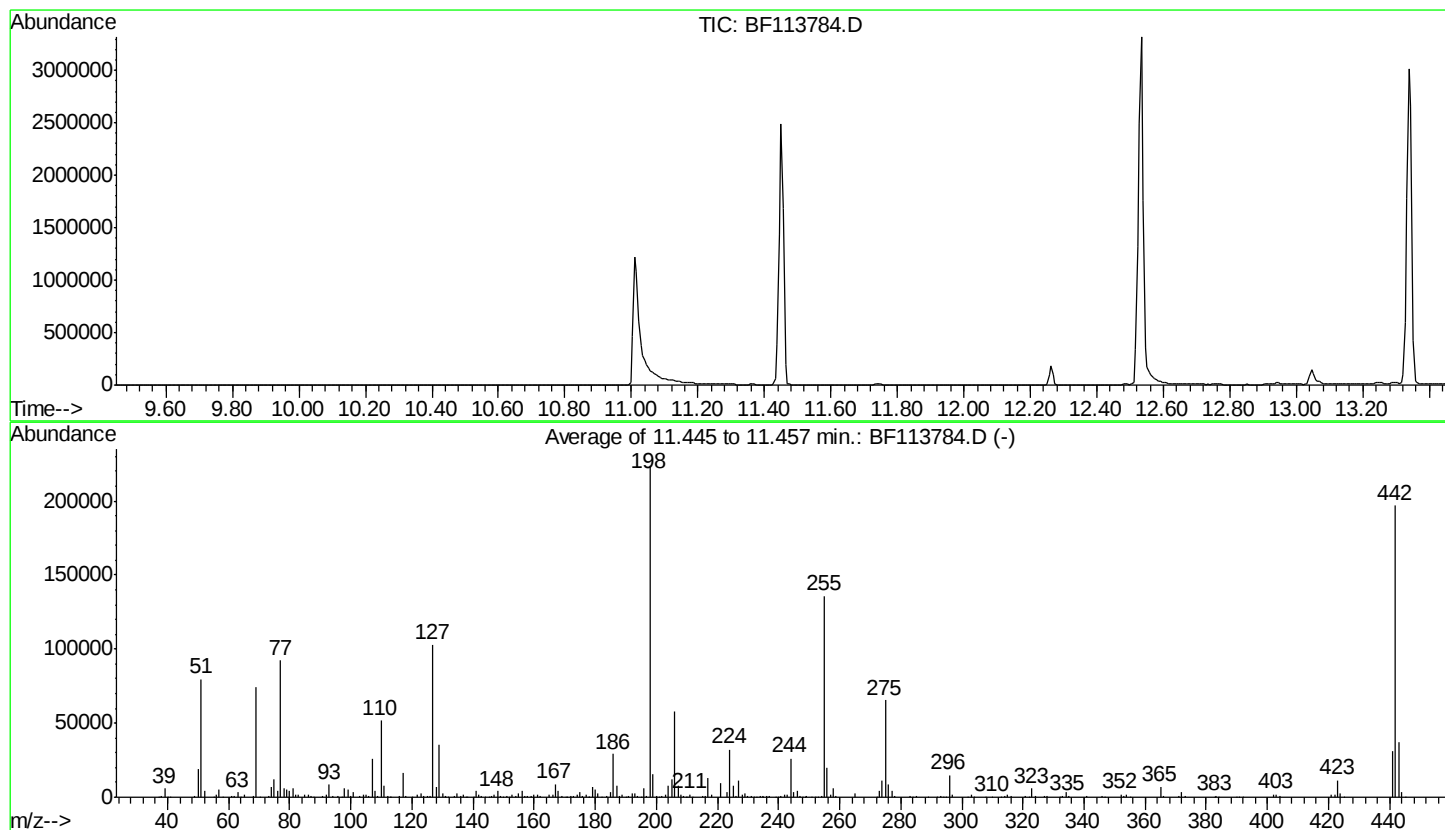

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	79664	PASS
68	69	0.00	2	1.5	1134	PASS
69	198	0.00	100	33.1	74112	PASS
70	69	0.00	2	0.4	282	PASS
127	198	10	80	46.0	102858	PASS
197	198	0.00	2	0.4	893	PASS
198	198	100	100	100.0	223829	PASS
199	198	5	9	6.9	15381	PASS
275	198	10	60	29.3	65568	PASS
365	198	1	100	3.2	7182	PASS
441	198	0.01	100	14.0	31334	PASS
442	198	50	100	87.9	196666	PASS
443	442	15	24	19.0	37426	PASS