

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041620\
 Data File : BF120045.D
 Acq On : 16 Apr 2020 19:20
 Operator : MA/SJ
 Sample : L2230-49 5X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CONCRETE-4-9-2020

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.357	723	726	732	rBV2	82429	93460	9.17%	0.998%
2	6.722	785	788	792	rBV	1020727	819739	80.44%	8.753%
3	6.881	811	815	818	rBV	731230	595369	58.43%	6.357%
4	7.287	880	884	887	rBV	519141	425554	41.76%	4.544%
5	8.010	1003	1007	1010	rBV	1360788	1019022	100.00%	10.881%
6	9.086	1187	1190	1203	rVB	1061085	808972	79.39%	8.638%
7	9.251	1215	1218	1222	rVB	20084	14883	1.46%	0.159%
8	9.486	1255	1258	1267	rVB	88468	81497	8.00%	0.870%
9	9.769	1302	1306	1309	rBV	1085655	969021	95.09%	10.347%
10	11.251	1554	1558	1561	rBV	1004113	791236	77.65%	8.448%
11	11.275	1561	1562	1565	rVB	31161	15514	1.52%	0.166%
12	11.969	1674	1680	1684	rBV3	14571	27566	2.71%	0.294%
13	12.351	1740	1745	1749	rBV3	12528	15899	1.56%	0.170%
14	12.463	1760	1764	1767	rBV	34953	29376	2.88%	0.314%
15	12.669	1795	1799	1802	rBV	377388	313444	30.76%	3.347%
16	12.692	1802	1803	1805	rVV	34888	17881	1.75%	0.191%
17	12.722	1805	1808	1810	rVV	31841	29042	2.85%	0.310%
18	12.745	1810	1812	1815	rVB	73393	55183	5.42%	0.589%
19	12.839	1824	1828	1831	rBV	641895	548641	53.84%	5.858%
20	12.933	1842	1844	1850	rVB6	11437	13274	1.30%	0.142%
21	13.080	1865	1869	1873	rBV2	40060	39924	3.92%	0.426%
22	13.327	1907	1911	1914	rBV	115379	103892	10.20%	1.109%
23	13.374	1916	1919	1923	rVV	272471	219728	21.56%	2.346%
24	13.421	1924	1927	1929	rBV	64356	51288	5.03%	0.548%
25	13.445	1929	1931	1934	rVB3	29835	22993	2.26%	0.246%
26	13.545	1943	1948	1951	rBV7	13673	18501	1.82%	0.198%
27	13.610	1956	1959	1961	rBV	14601	16596	1.63%	0.177%
28	13.751	1980	1983	1986	rBV	68760	70202	6.89%	0.750%
29	13.892	2002	2007	2010	rBV	811332	743496	72.96%	7.939%
30	14.068	2033	2037	2040	rBV	98118	85395	8.38%	0.912%
31	14.374	2085	2089	2092	rBV	111519	106988	10.50%	1.142%
32	14.668	2136	2139	2145	rBV	119081	125459	12.31%	1.340%
33	14.910	2177	2180	2184	rBV5	24825	34258	3.36%	0.366%
34	14.992	2191	2194	2198	rBV	113188	120026	11.78%	1.282%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041620\
Data File : BF120045.D
Acq On : 16 Apr 2020 19:20
Operator : MA/SJ
Sample : L2230-49 5X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONCRETE-4-9-2020

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.315	2244	2249	2253	rBV	478064	566394	55.58%	6.048%
36	15.357	2253	2256	2260	rVB	110352	129464	12.70%	1.382%
37	15.768	2322	2326	2331	rBV2	78750	109310	10.73%	1.167%
38	16.251	2402	2408	2413	rBV3	58230	117007	11.48%	1.249%


Sum of corrected areas: 9365494

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041620\
Data File : BF120045.D
Acq On : 16 Apr 2020 19:20
Operator : MA/SJ
Sample : L2230-49 5X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONCRETE-4-9-2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

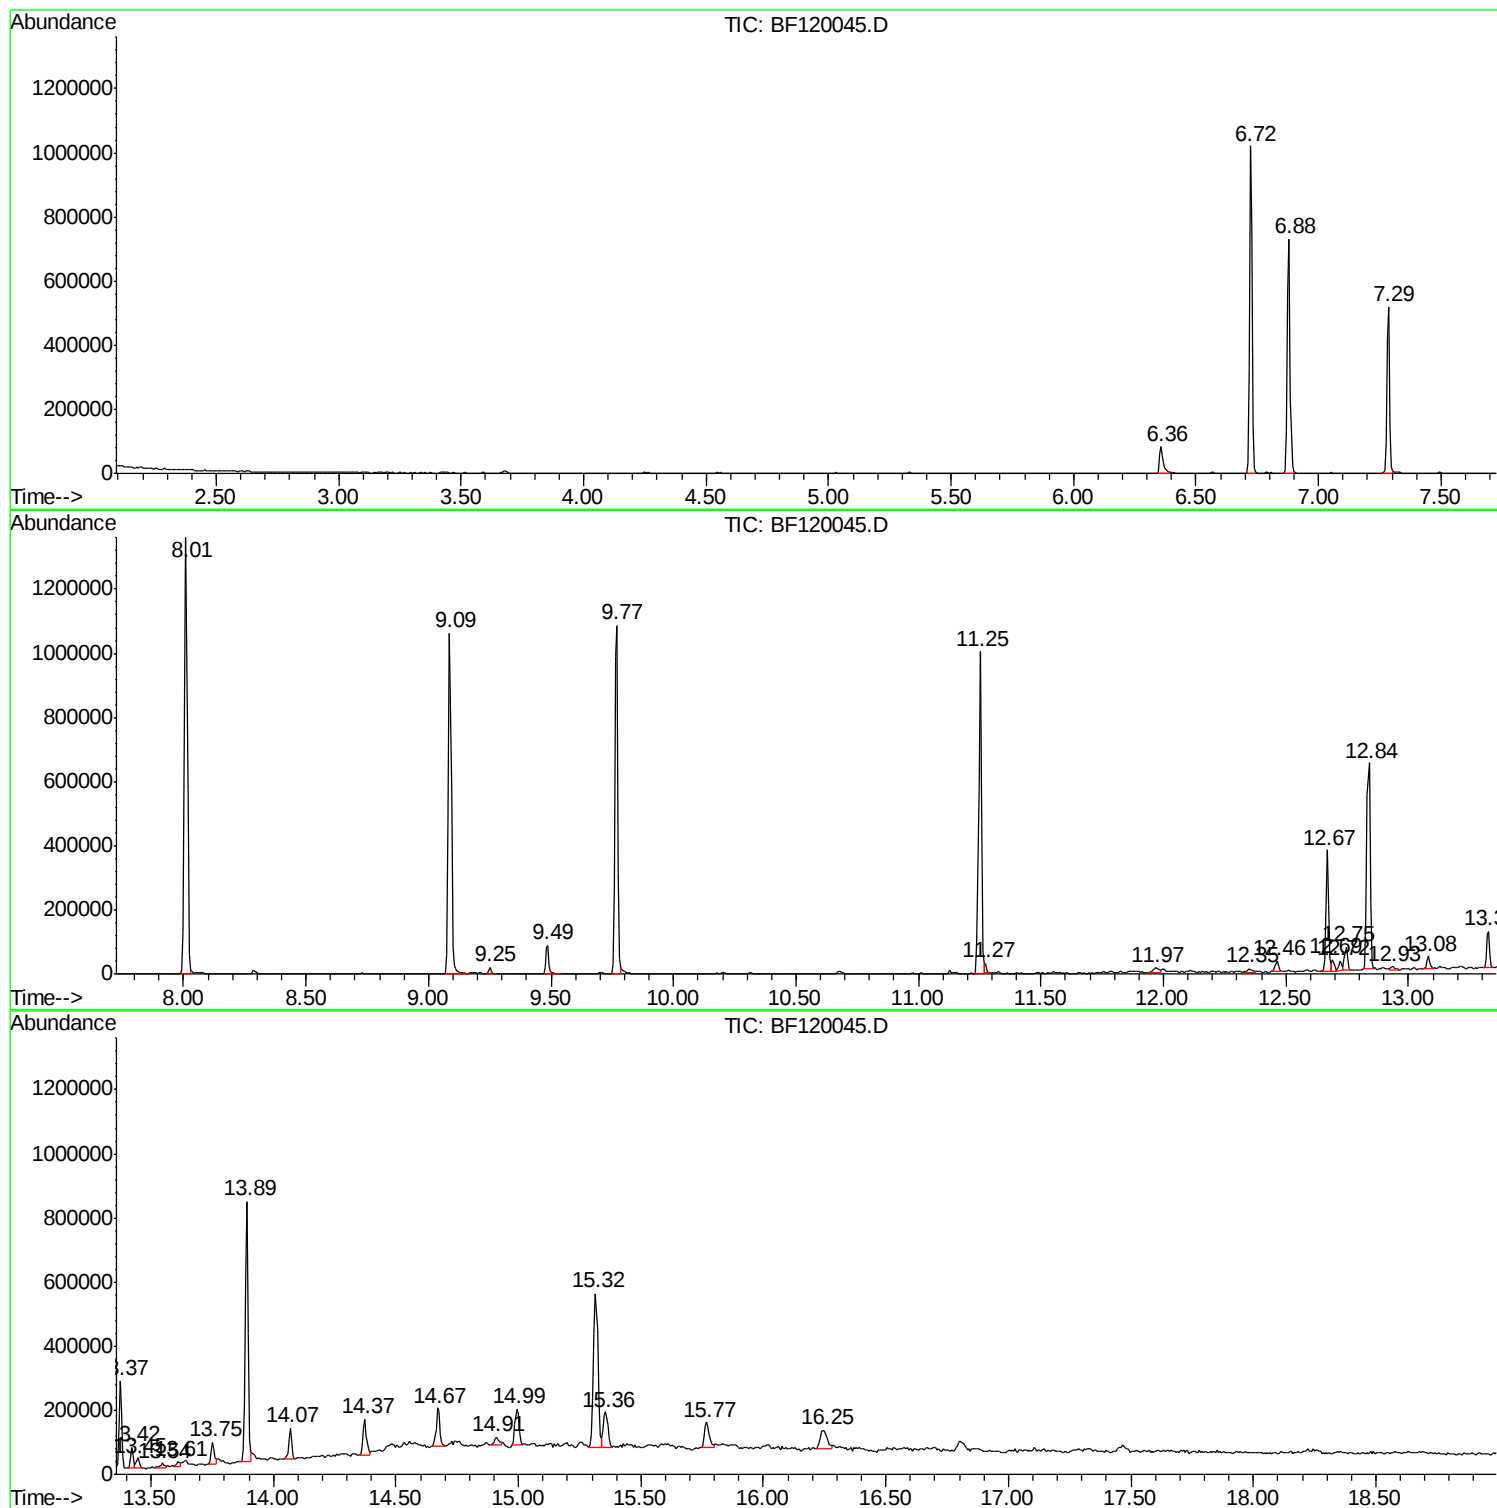

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041620\
Data File : BF120045.D
Acq On : 16 Apr 2020 19:20
Operator : MA/SJ
Sample : L2230-49 5X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONCRETE-4-9-2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041620\
Data File : BF120045.D
Acq On : 16 Apr 2020 19:20
Operator : MA/SJ
Sample : L2230-49 5X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONCRETE-4-9-2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc