


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041620\
 Data File : BF120024.D
 Acq On : 16 Apr 2020 8:13
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 17 10:51:37 2020

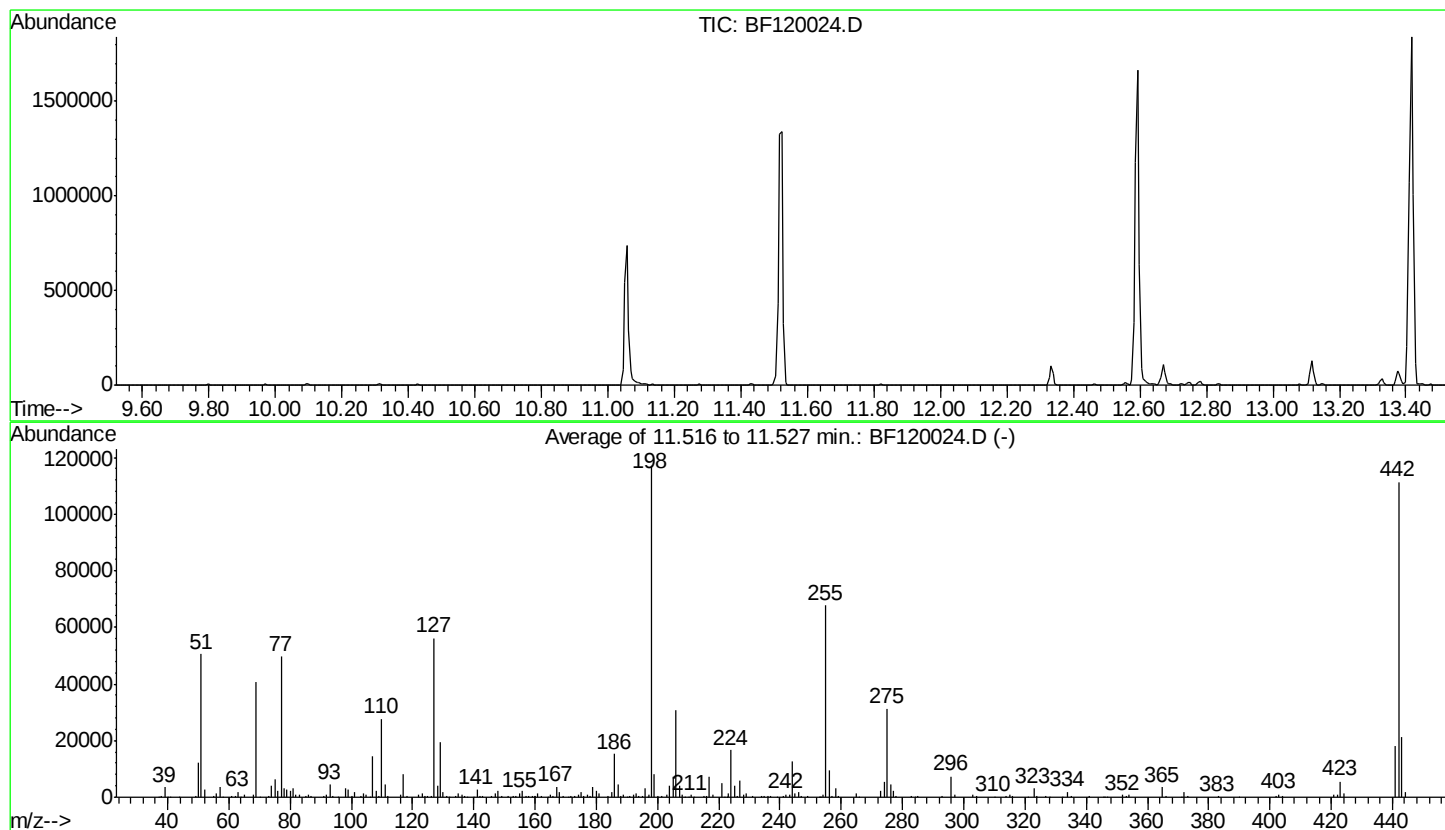

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	50546	PASS
68	69	0.00	2	2.0	823	PASS
69	198	0.00	100	34.6	40580	PASS
70	69	0.00	2	0.3	116	PASS
127	198	10	80	48.0	56169	PASS
197	198	0.00	2	0.6	738	PASS
198	198	100	100	100.0	117114	PASS
199	198	5	9	6.8	7985	PASS
275	198	10	60	26.8	31398	PASS
365	198	1	100	3.0	3555	PASS
441	198	0.01	100	15.5	18127	PASS
442	198	50	100	95.0	111245	PASS
443	442	15	24	19.1	21277	PASS