

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041720\
 Data File : BF120067.D
 Acq On : 17 Apr 2020 18:53
 Operator : MA/SJ
 Sample : L2279-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OILY-STONE-REGULATORS

Quant Time: Apr 18 04:27:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 17 10:51:37 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	157654	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	566333	20.00	ng	0.00
39) Acenaphthene-d10	9.77	164	244438	20.00	ng	0.00
64) Phenanthrene-d10	11.27	188	311670	20.00	ng	0.01
76) Chrysene-d12	13.92	240	249450	20.00	ng	0.01
87) Perylene-d12	15.34	264	187539	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	991919	108.73	ng	0.00
7) Phenol-d6	6.37	99	1246632	106.05	ng	0.00
23) Nitrobenzene-d5	7.29	82	677635	61.90	ng	0.00
42) 2,4,6-Tribromophenol	10.56	330	207512	69.34	ng	0.00
45) 2-Fluorobiphenyl	9.09	172	1402033	81.44	ng	0.00
79) Terphenyl-d14	12.87	244	765416	51.63	ng	0.02
Target Compounds						
50) Dimethylphthalate	9.49	163	270662	14.315	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041720\
Data File : BF120067.D
Acq On : 17 Apr 2020 18:53
Operator : MA/SJ
Sample : L2279-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OILY-STONE-REGULATORS

Quant Time: Apr 18 04:27:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 10:51:37 2020
Response via : Initial Calibration

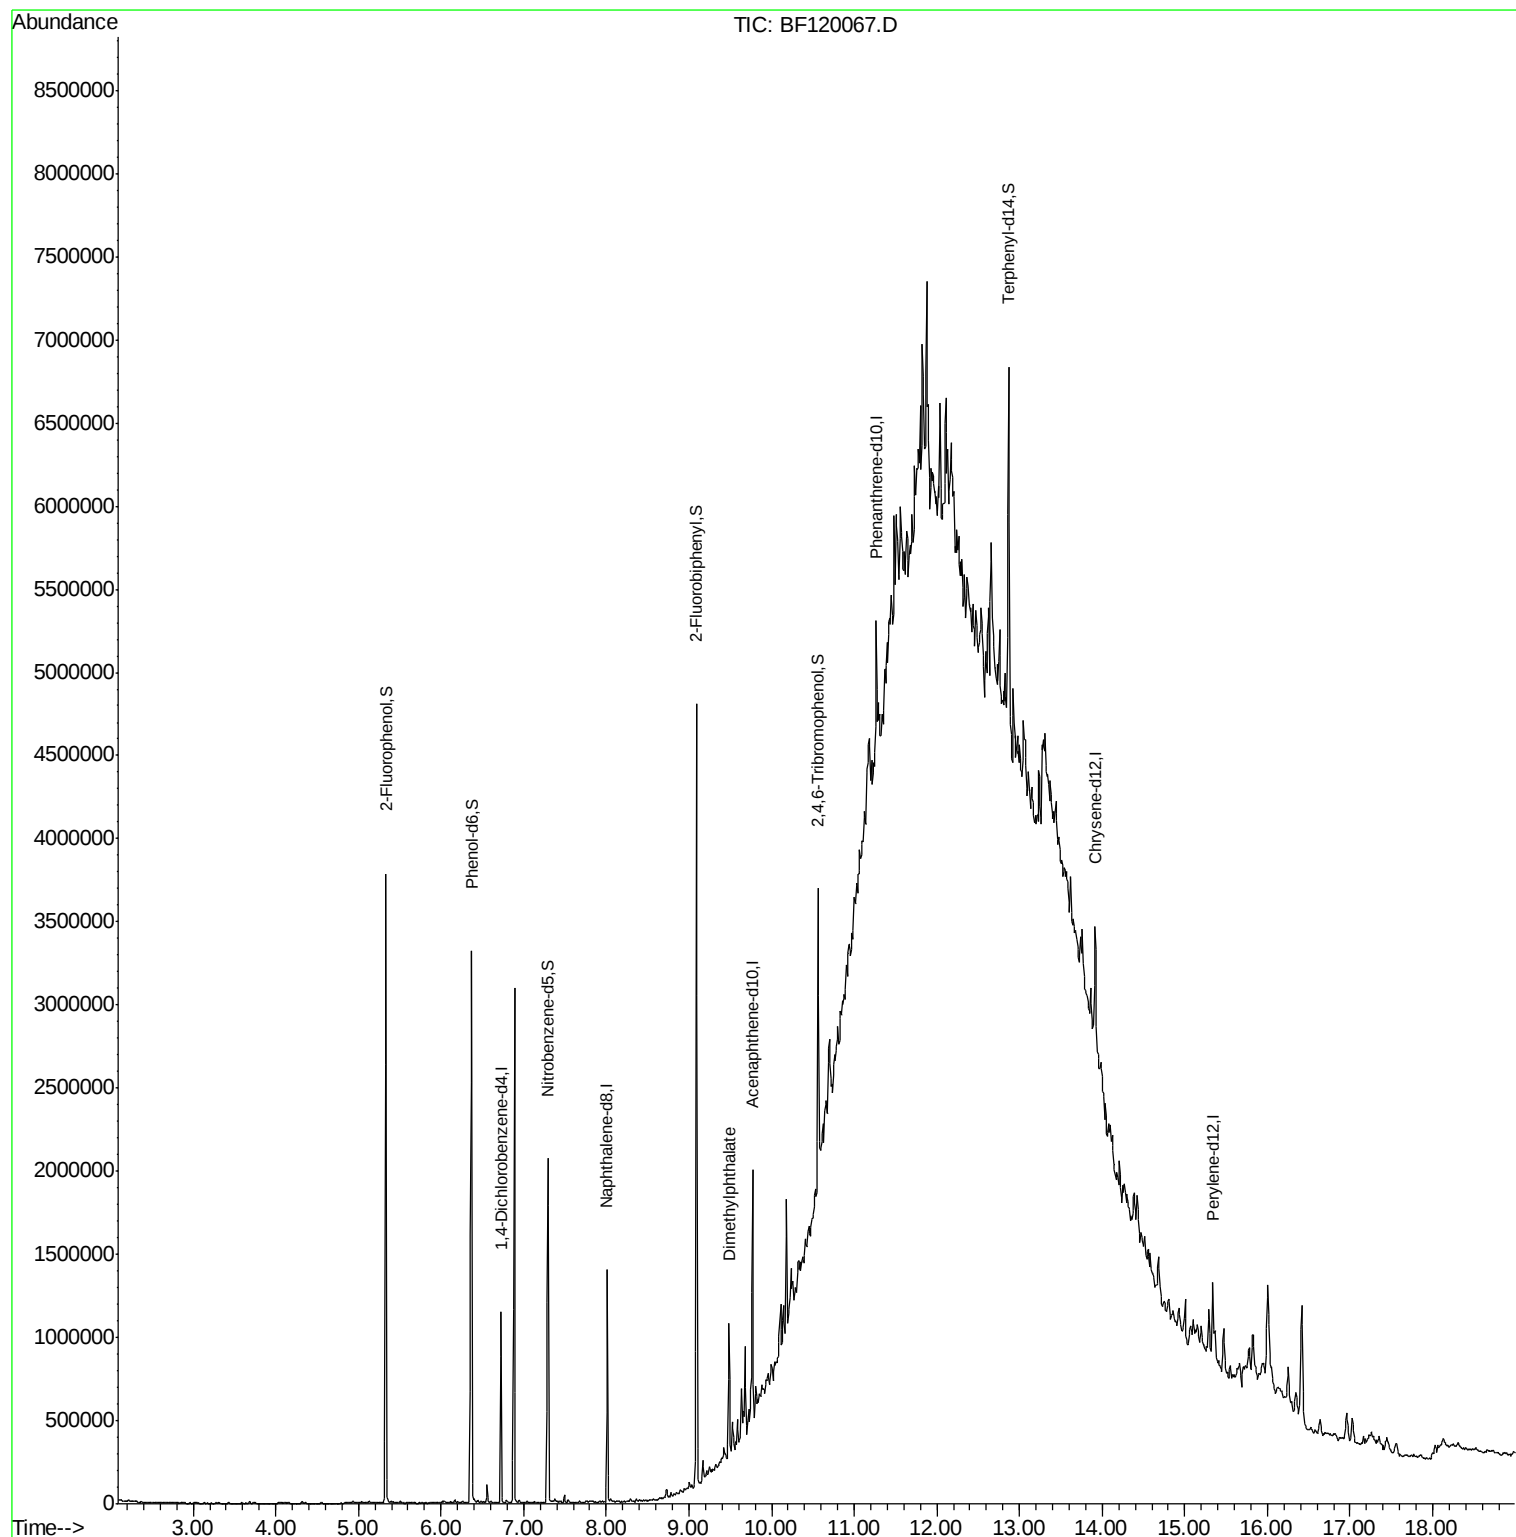

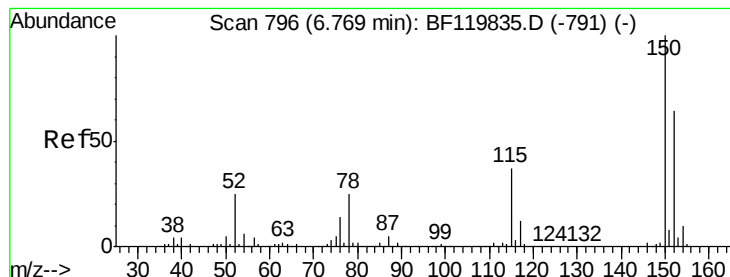


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. 0.00 min
Lab File: BF120067.D
Acq: 17 Apr 2020 18:53

Instrument :
BNA_F
ClientSampleId :
OILY-STONE-REGULATORS

Tot Ion:152 Resp: 157654
Ion Ratio Lower Upper
152 100
150 155.5 124.8 187.2
115 58.1 46.5 69.7

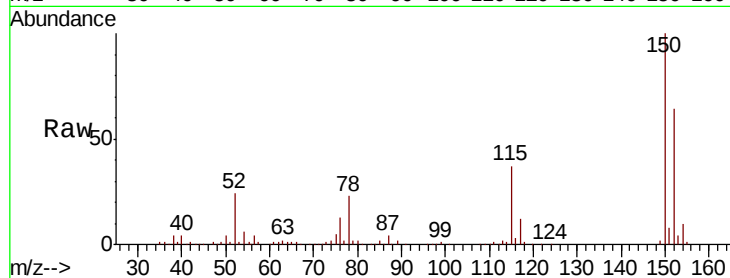


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

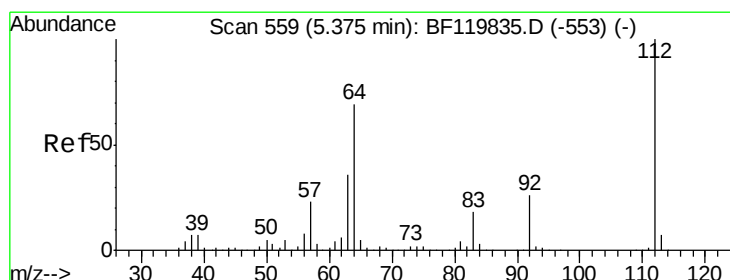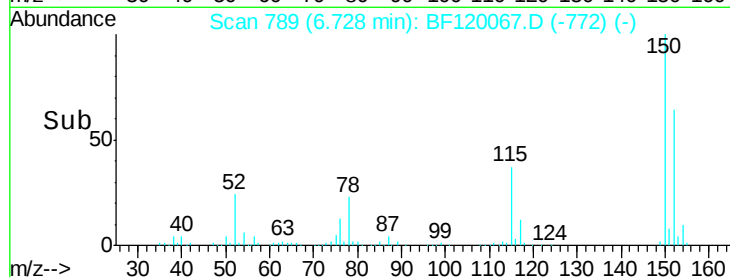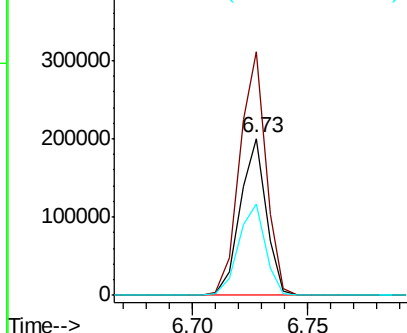



#5

2-Fluorophenol
Concen: 108.733 ng
RT: 5.33 min Scan# 552
Delta R.T. 0.01 min
Lab File: BF120067.D
Acq: 17 Apr 2020 18:53

Tgt Ion:112 Resp: 991919
Ion Ratio Lower Upper
112 100
64 69.2 55.5 83.3
63 35.8 29.1 43.7

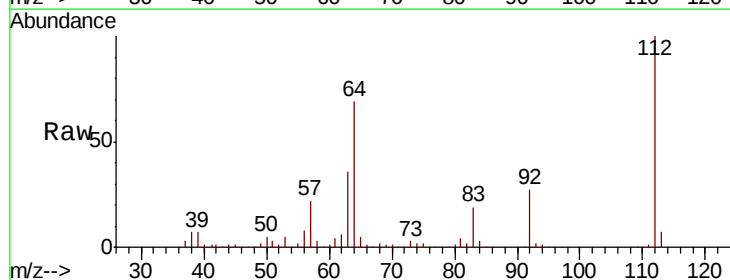

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

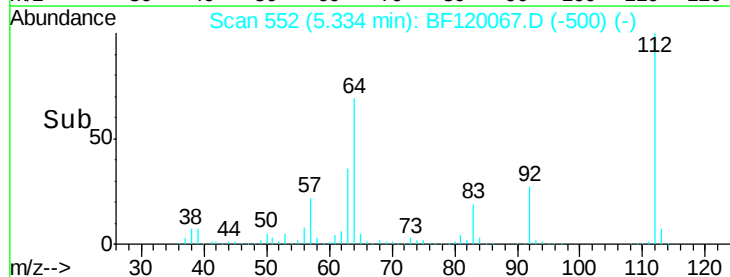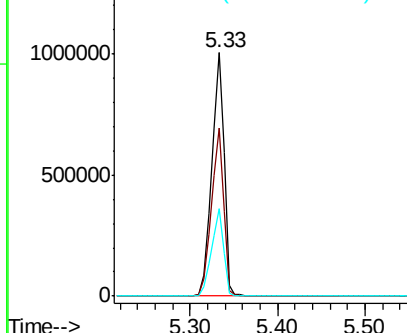



#7

Phenol-d6

Concen: 106.053 ng

RT: 6.37 min Scan# 728

Delta R.T. 0.00 min

Lab File: BF120067.D

Acq: 17 Apr 2020 18:53

Instrument :

BNA_F

ClientSampleId :

OILY-STONE-REGULATORS


Tot Ion: 99 Resp: 1246632

Ion Ratio Lower Upper




99 100

42 20.2 16.9 25.3

71 32.6 26.3 39.5

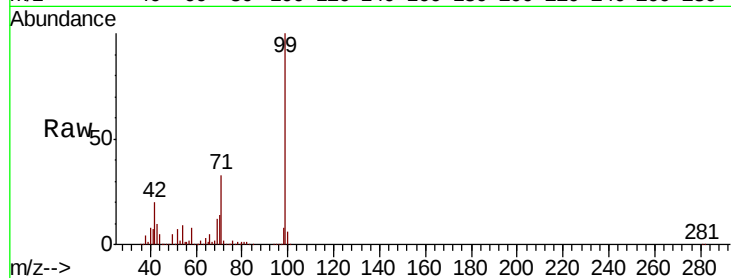

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

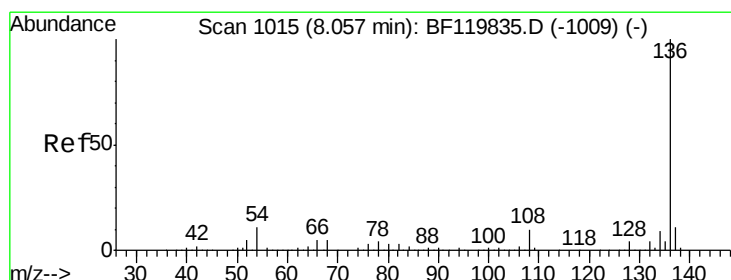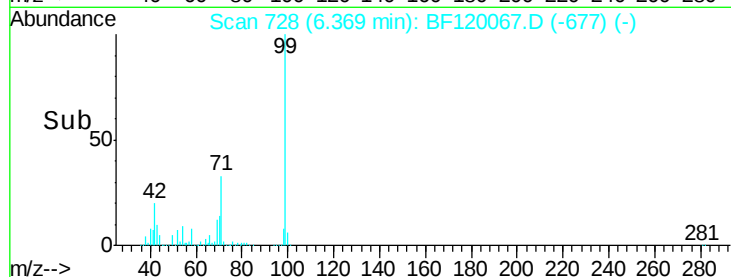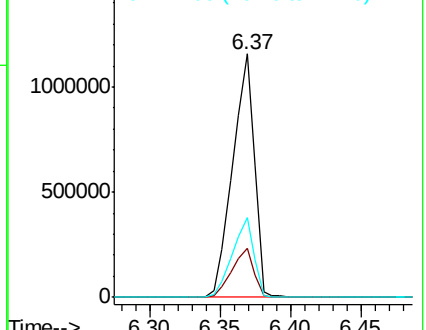

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007

Delta R.T. -0.01 min

Lab File: BF120067.D

Acq: 17 Apr 2020 18:53

Tgt Ion: 136 Resp: 566333


Ion Ratio Lower Upper

136 100



137 11.0 8.7 13.1


54 11.0 8.5 12.7

68 5.2 3.9 5.9

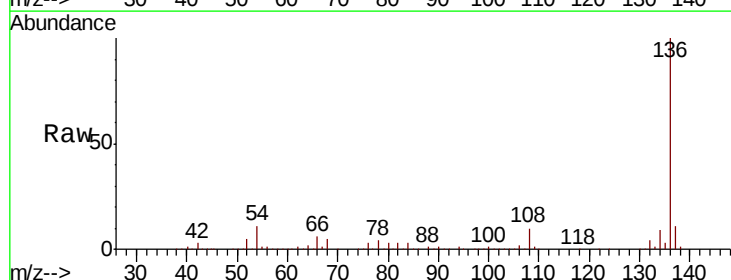

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



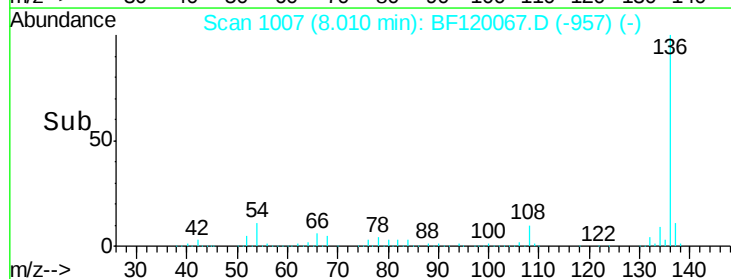
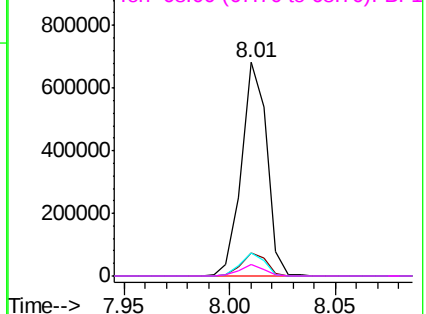


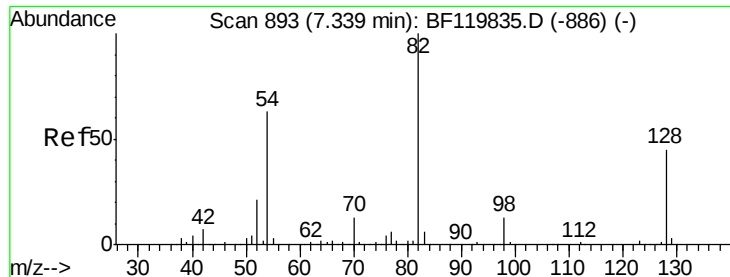

#23
Nitrobenzene-d5
Concen: 61.901 ng
RT: 7.29 min Scan# 885
Delta R.T. -0.01 min
Lab File: BF120067.D
Acq: 17 Apr 2020 18:53




Instrument :
BNA_F
ClientSampleId :
OILY-STONE-REGULATORS


Tot Ion: 82 Resp: 677635
Ion Ratio Lower Upper
82 100
128 43.5 36.2 54.4
54 65.4 50.4 75.6

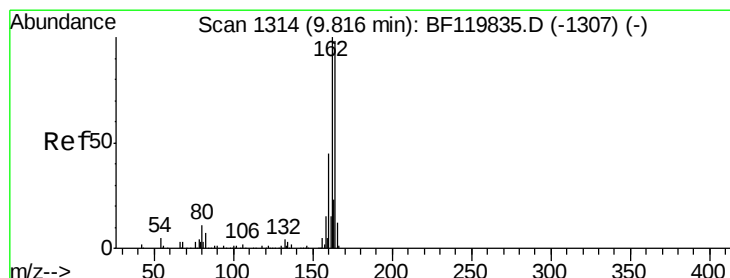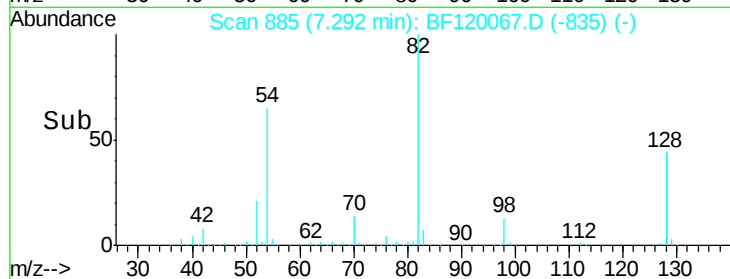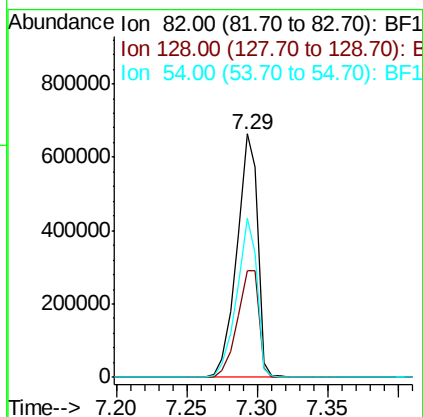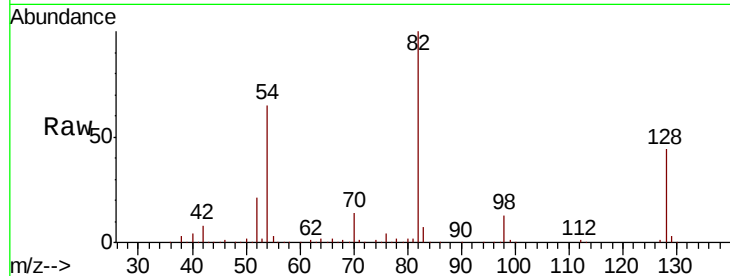

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.77 min Scan# 1306
Delta R.T. -0.01 min
Lab File: BF120067.D
Acq: 17 Apr 2020 18:53

Tgt Ion: 164 Resp: 244438
Ion Ratio Lower Upper
164 100
162 104.4 81.9 122.9
160 45.3 36.6 54.8


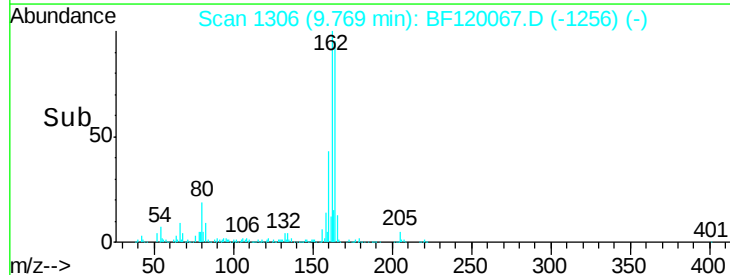
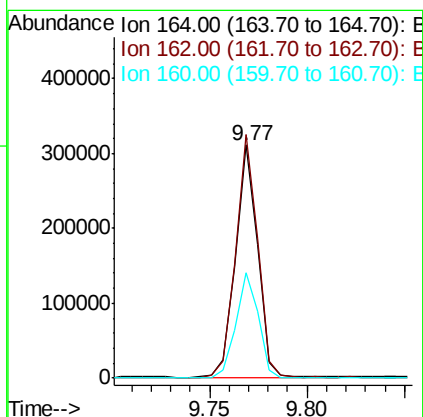
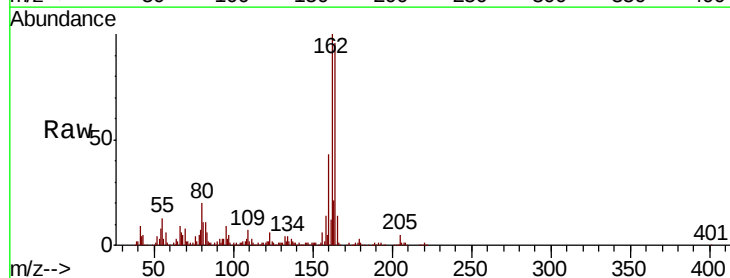


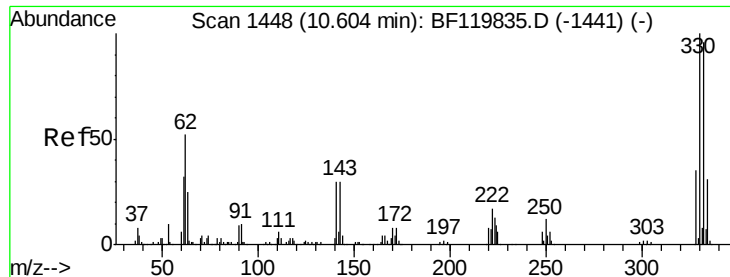

#42
 2,4,6-Tribromophenol
 Concen: 69.338 ng
 RT: 10.56 min Scan# 1441
 Delta R.T. -0.01 min
 Lab File: BF120067.D
 Acq: 17 Apr 2020 18:53




Instrument :
 BNA_F
 ClientSampleId :
 OILY-STONE-REGULATORS


Tot Ion:330 Resp: 207512
 Ion Ratio Lower Upper
 330 100
 332 98.1 76.8 115.2
 141 37.6 25.1 37.7

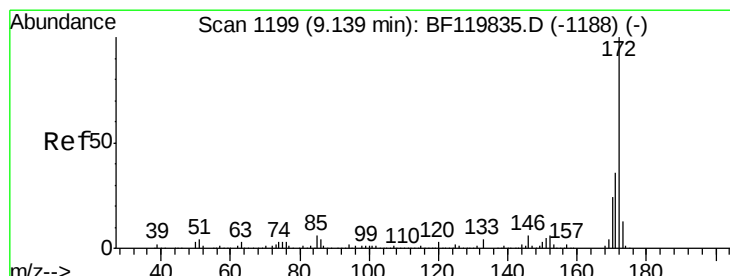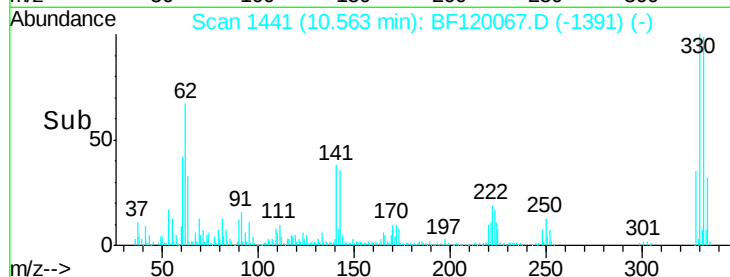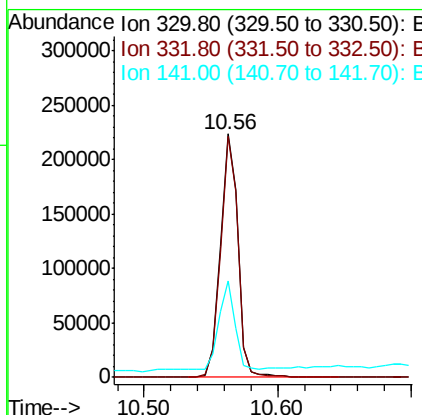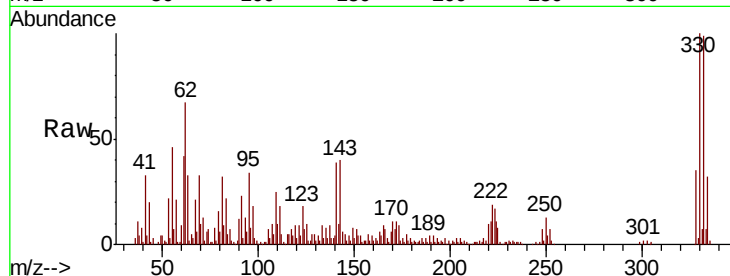

#45
 2-Fluorobiphenyl
 Concen: 81.435 ng
 RT: 9.09 min Scan# 1191
 Delta R.T. -0.01 min
 Lab File: BF120067.D
 Acq: 17 Apr 2020 18:53

Tgt Ion:172 Resp: 1402033
 Ion Ratio Lower Upper
 172 100
 171 36.5 28.9 43.3
 170 23.7 19.4 29.2


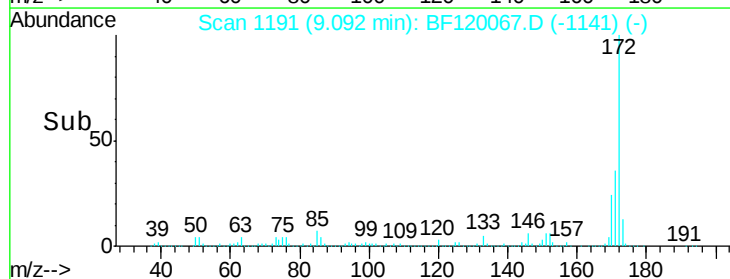
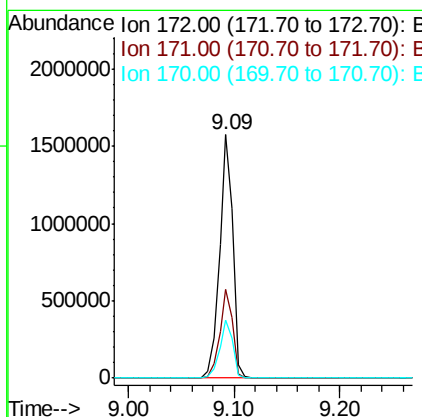
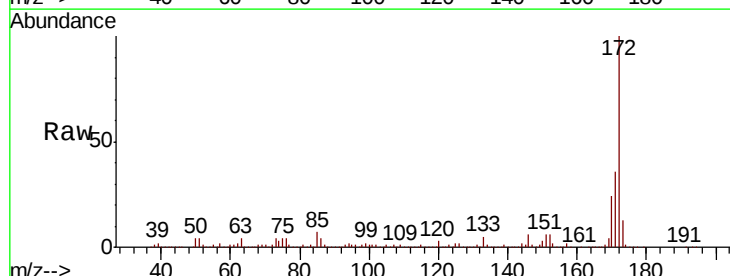


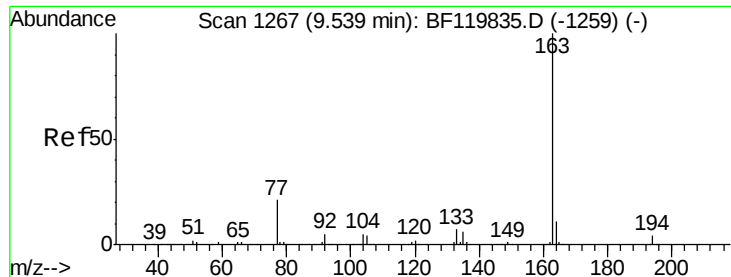

#50
Dimethylphthalate
Concen: 14.315 ng
RT: 9.49 min Scan# 1258
Delta R.T. -0.02 min
Lab File: BF120067.D
Acq: 17 Apr 2020 18:53




Instrument :
BNA_F
ClientSampleId :
OILY-STONE-REGULATORS


Tot Ion:163	Resp:	270662
Ion Ratio	Lower	Upper
163	100	
194	4.2	3.0 4.4
164	10.6	8.4 12.6

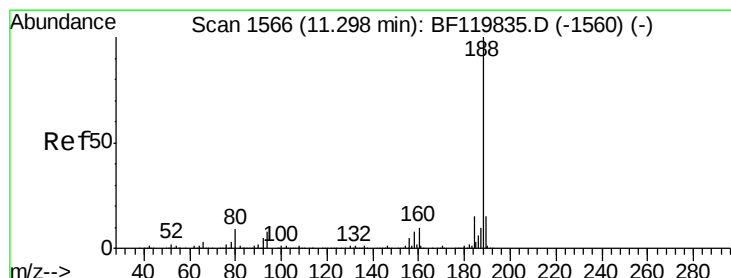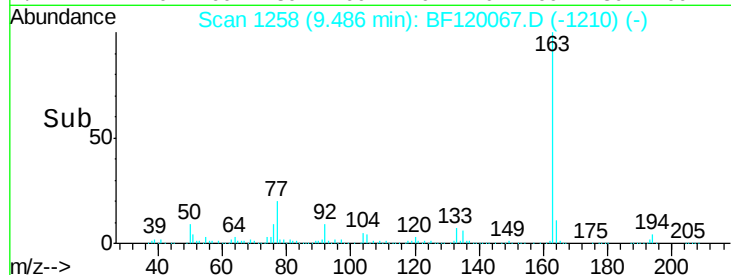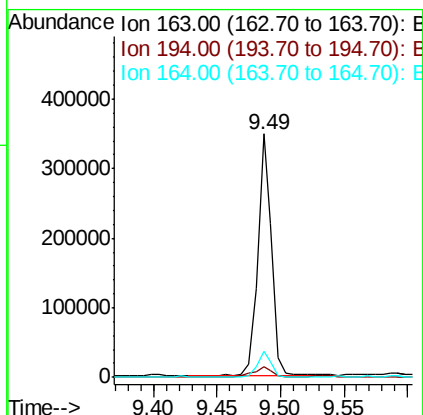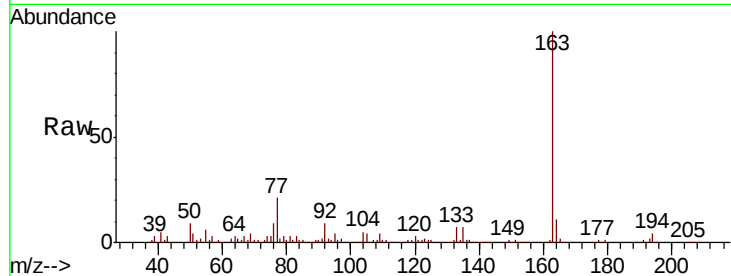

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.27 min Scan# 1561
Delta R.T. 0.01 min
Lab File: BF120067.D
Acq: 17 Apr 2020 18:53

Tgt Ion:188	Resp:	311670
Ion Ratio	Lower	Upper
188	100	
94	17.3	6.7 10.1#
80	14.5	7.4 11.2#

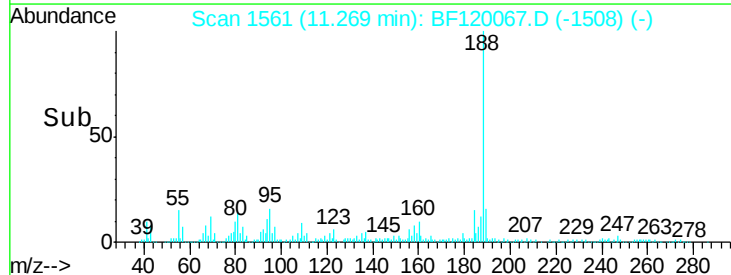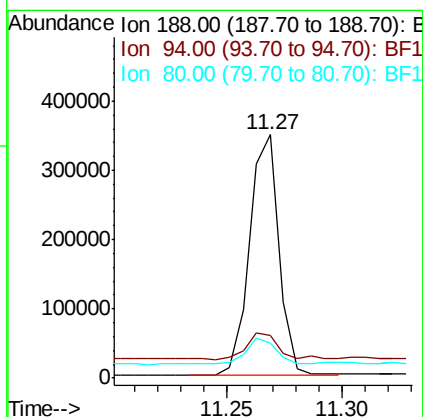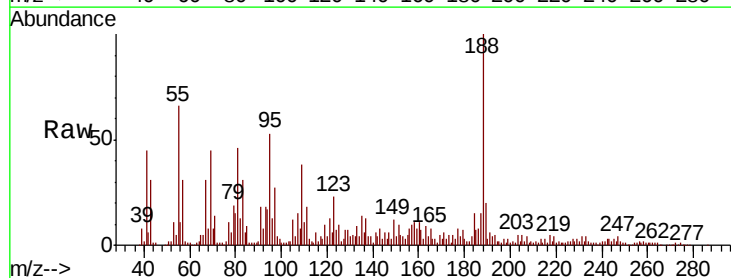

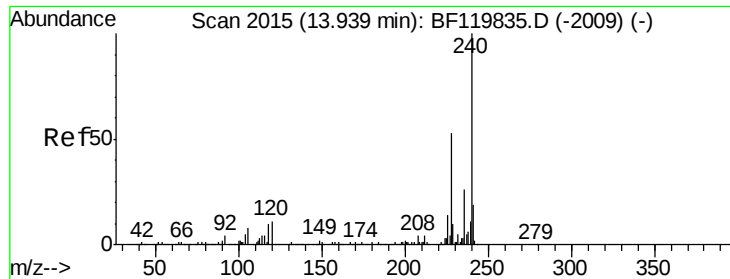

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.92 min Scan# 2011

Delta R.T. 0.01 min

Lab File: BF120067.D

Acq: 17 Apr 2020 18:53

Instrument :

BNA_F

ClientSampleId :

OILY-STONE-REGULATORS


Tot Ion:240 Resp: 249450

Ion Ratio Lower Upper

240 100

120 14.4 9.0 13.6#




236 26.0 20.7 31.1

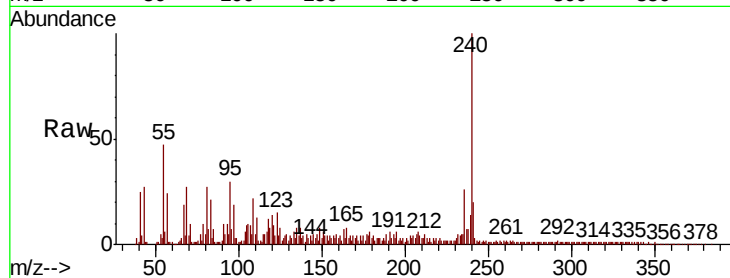

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

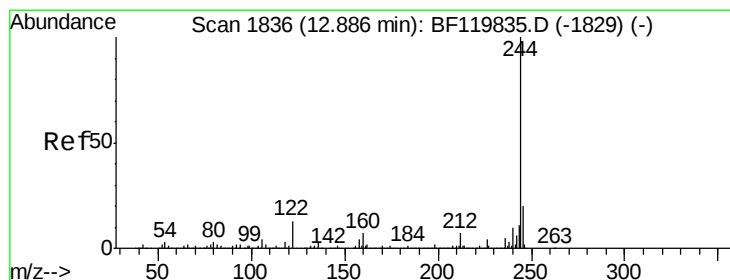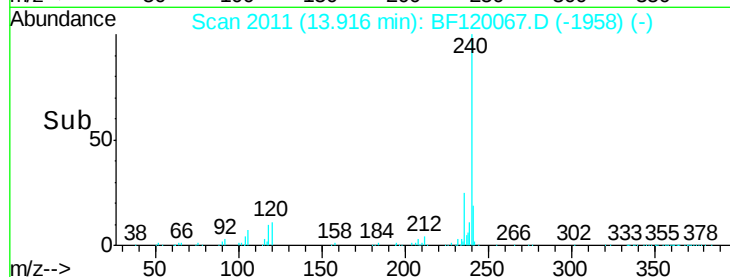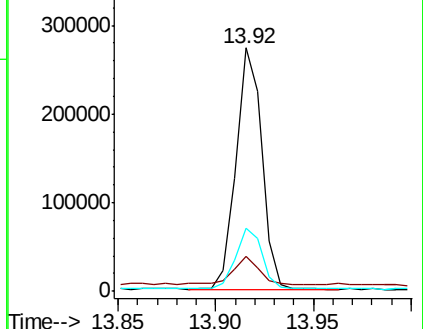

#79

Terphenyl-d14

Concen: 51.631 ng

RT: 12.87 min Scan# 1833

Delta R.T. 0.02 min

Lab File: BF120067.D

Acq: 17 Apr 2020 18:53


Tgt Ion:244 Resp: 765416

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0



122 15.0 10.3 15.5

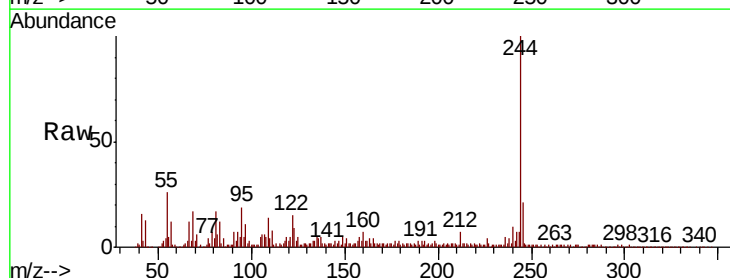


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

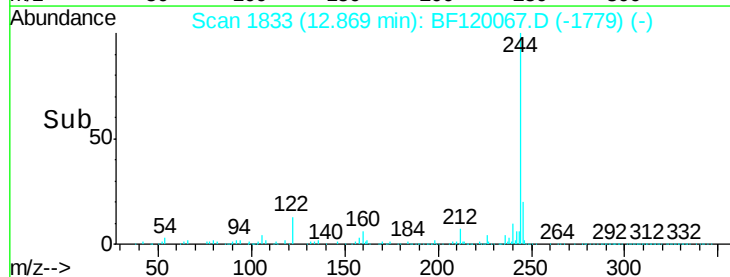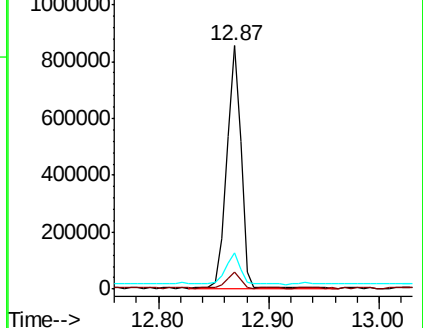

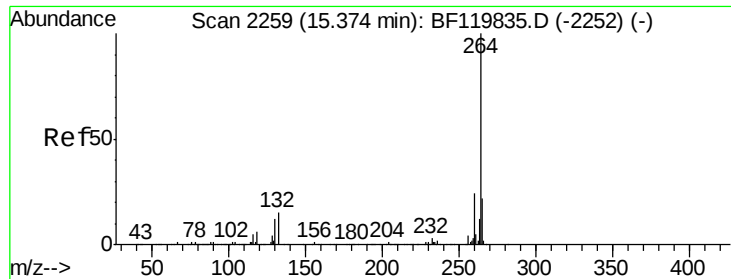

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.34 min Scan# 2253
Delta R.T. 0.01 min
Lab File: BF120067.D
Acq: 17 Apr 2020 18:53

Instrument :
BNA_F
ClientSampleId :
OILY-STONE-REGULATORS

Tot Ion	Ion	Ratio	Lower	Upper
264	100			
260	23.4	19.3	28.9	
265	22.4	17.6	26.4	

