


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041720\
 Data File : BF120046.D
 Acq On : 17 Apr 2020 9:24
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 17 10:51:37 2020

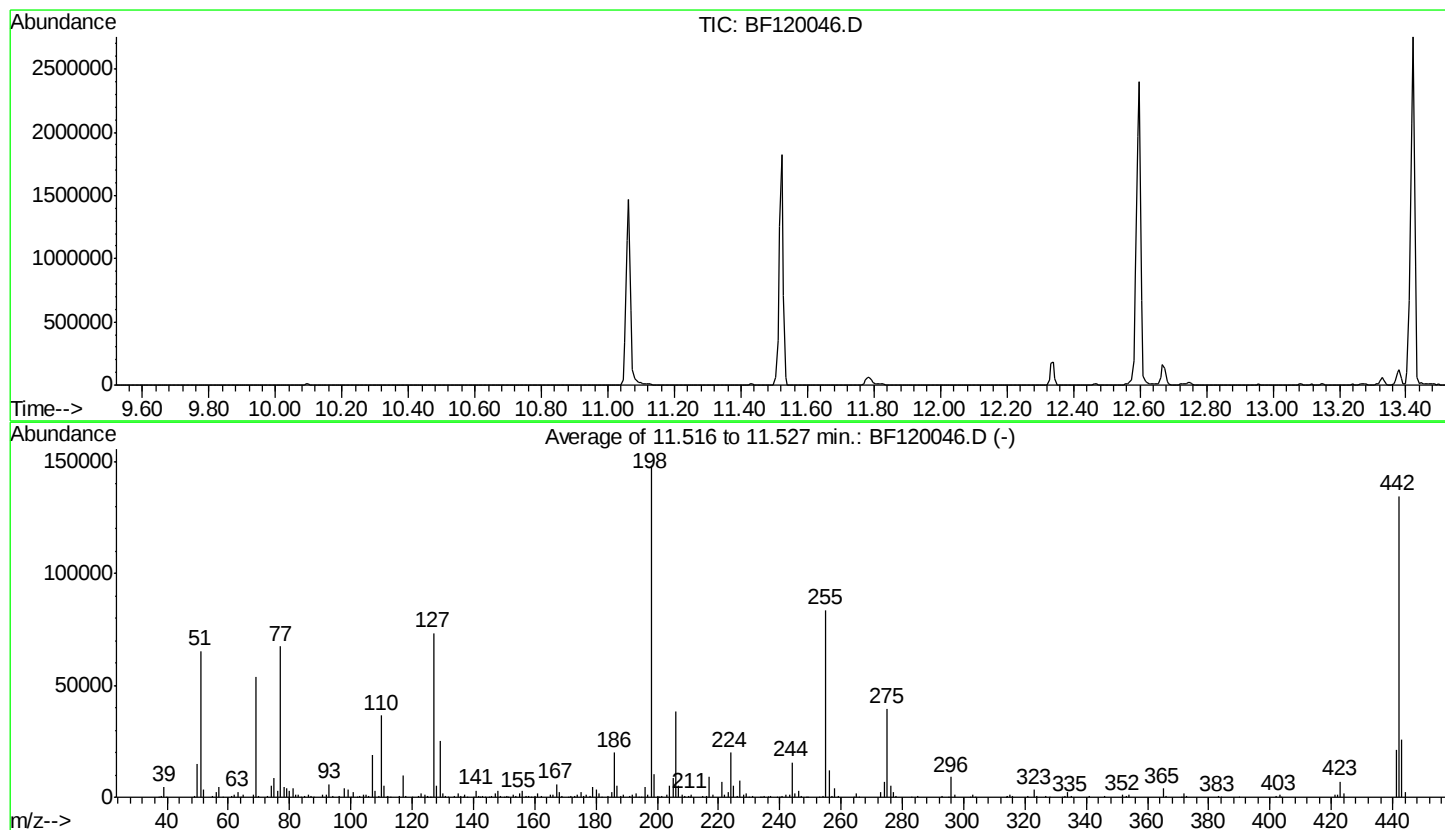

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	65277	PASS
68	69	0.00	2	1.7	907	PASS
69	198	0.00	100	36.5	54005	PASS
70	69	0.00	2	0.6	307	PASS
127	198	10	80	49.5	73306	PASS
197	198	0.00	2	0.6	901	PASS
198	198	100	100	100.0	148066	PASS
199	198	5	9	6.9	10202	PASS
275	198	10	60	26.7	39517	PASS
365	198	1	100	2.7	4005	PASS
441	198	0.01	100	14.3	21169	PASS
442	198	50	100	90.9	134621	PASS
443	442	15	24	19.0	25568	PASS