

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041819\
 Data File : BF113827.D
 Acq On : 18 Apr 2019 20:02
 Operator : JU/SJ
 Sample : K2436-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 19 02:07:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF041819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 13:55:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	169740	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	587221	20.00	ng	0.00
39) Acenaphthene-d10	9.93	164	259937	20.00	ng	0.00
64) Phenanthrene-d10	11.41	188	461032	20.00	ng	0.00
76) Chrysene-d12	14.04	240	511463	20.00	ng	0.00
87) Perylene-d12	15.51	264	591284	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.51	112	752879	73.75	ng	0.00
7) Phenol-d6	6.51	99	930538	73.10	ng	0.00
23) Nitrobenzene-d5	7.45	82	528622	54.82	ng	-0.01
42) 2,4,6-Tribromophenol	10.71	330	208801	72.71	ng	0.00
45) 2-Fluorobiphenyl	9.25	172	1005356	58.98	ng	0.00
79) Terphenyl-d14	12.99	244	1100095	45.10	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.51	77	1451	Below Cal	#	3
19) n-Nitroso-di-n-propylamine	7.45	70	71149	8.373	ng	# 78
25) Isophorone	7.45	82	528493	26.470	ng	# 65
50) Dimethylphthalate	9.64	163	100574	5.529	ng	# 98
51) 2,6-Dinitrotoluene	9.93	165	33842	8.430	ng	# 33
57) 2,4-Dinitrotoluene	9.93	165	33842	6.795	ng	# 29
65) 4,6-Dinitro-2-methylphenol	10.71	198	345	7.082	ng	# 1
67) 4-Bromophenyl-phenylether	10.71	248	12830	2.370	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF041819\
Data File : BF113827.D
Acq On : 18 Apr 2019 20:02
Operator : JU/SJ
Sample : K2436-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 19 02:07:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 13:55:51 2019
Response via : Initial Calibration

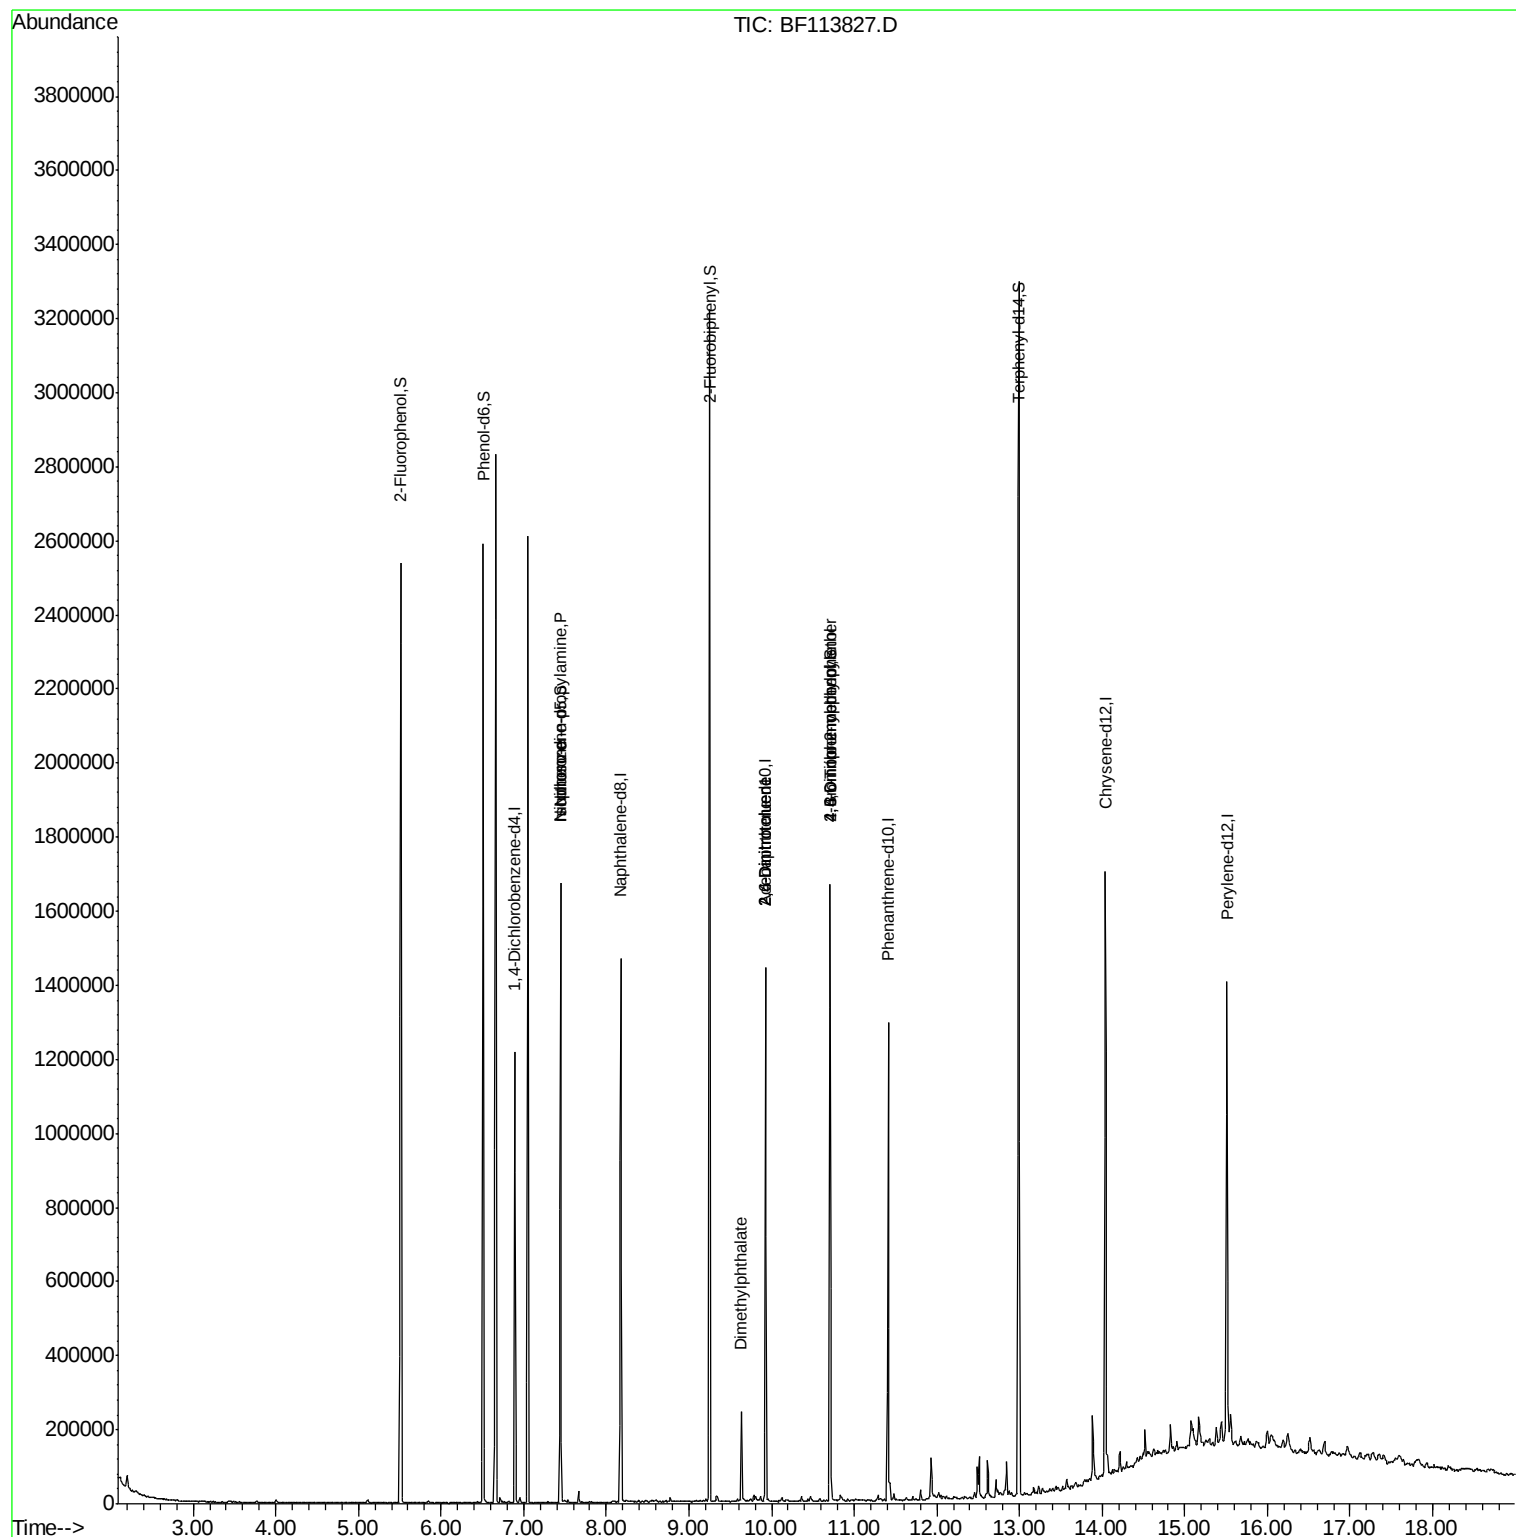

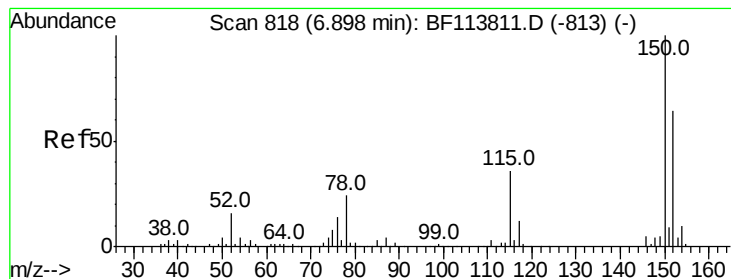


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.89 min Scan# 817
Delta R.T. -0.01 min
Lab File: BF113827.D
Acq: 18 Apr 2019 20:02

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 169740
Ion Ratio Lower Upper
152 100
150 154.9 125.9 188.9
115 58.9 45.9 68.9

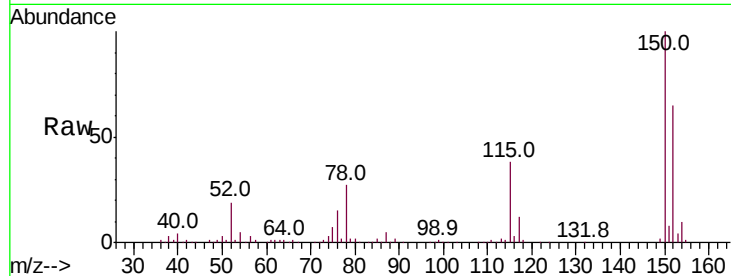


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

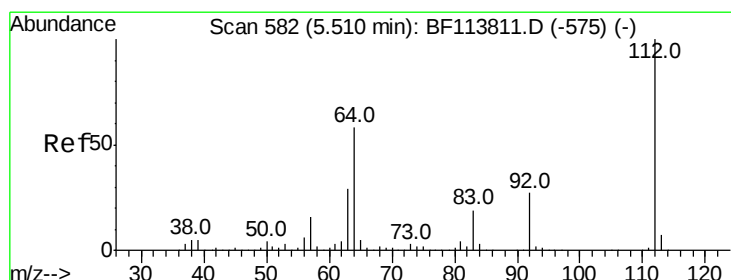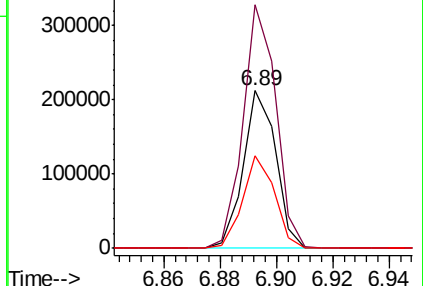



#5


2-Fluorophenol
Concen: 73.752 ng
RT: 5.51 min Scan# 582
Delta R.T. -0.00 min
Lab File: BF113827.D
Acq: 18 Apr 2019 20:02

Tgt Ion:112 Resp: 752879
Ion Ratio Lower Upper
112 100
64 59.3 46.6 69.8
63 29.5 23.1 34.7



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

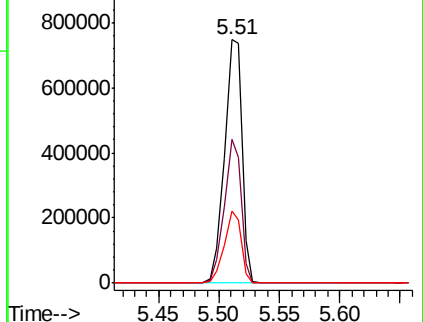

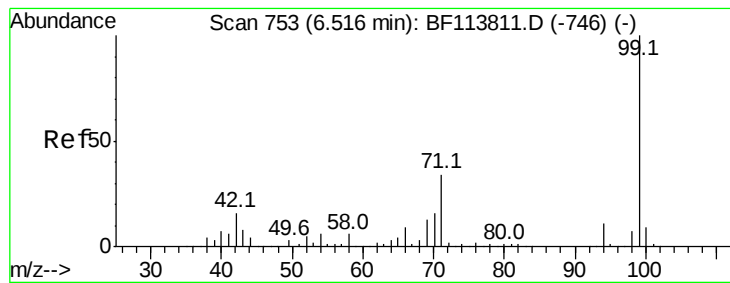

#7

Phenol-d6

Concen: 73.096 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.01 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 930538

Ion Ratio Lower Upper




99 100

42 15.8 12.5 18.7

71 33.3 26.9 40.3

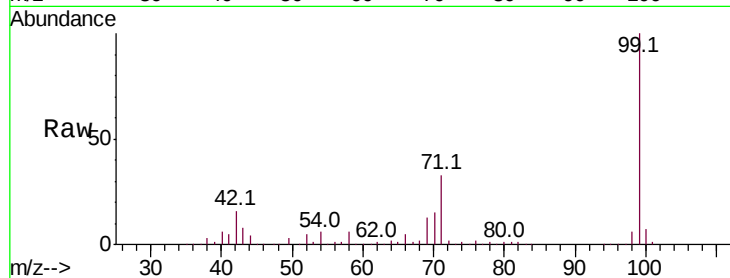

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

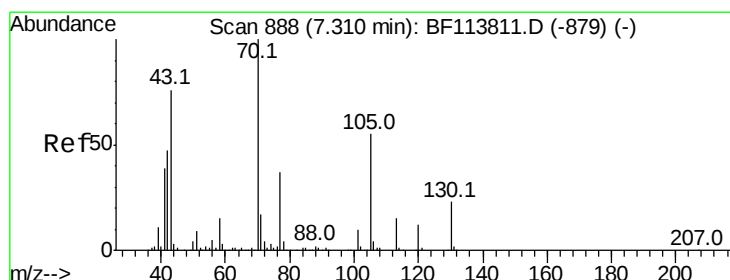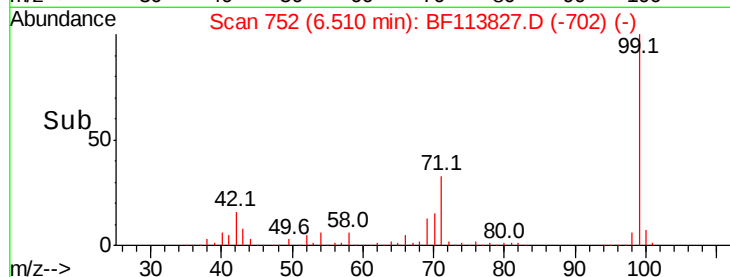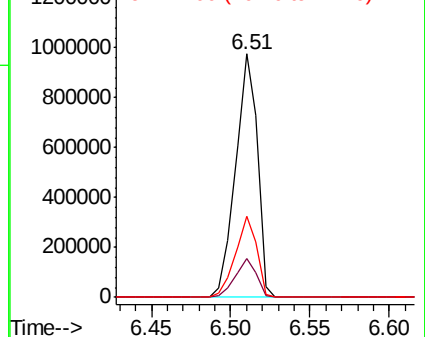

#19

n-Nitroso-di-n-propylamine

Concen: 8.373 ng

RT: 7.45 min Scan# 911

Delta R.T. 0.14 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02

Tgt Ion: 70 Resp: 71149


Ion Ratio Lower Upper

70 100



42 39.8 37.3 55.9


101 0.0 7.8 11.8#

130 2.0 18.2 27.2#

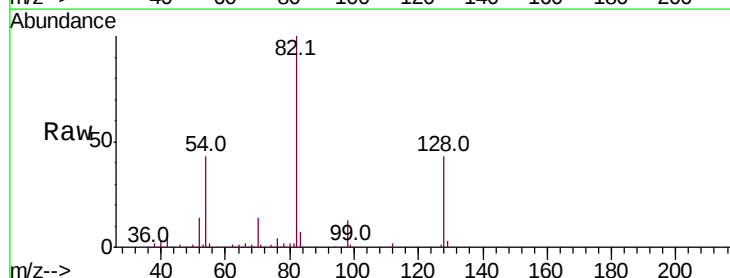

Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1

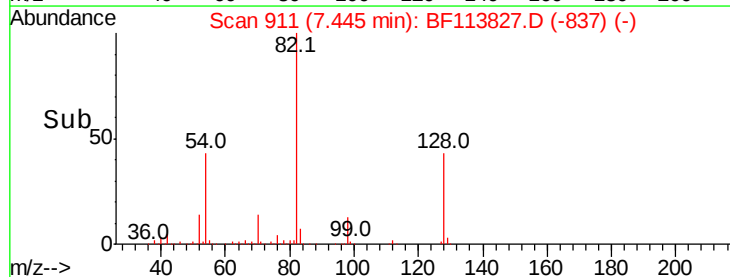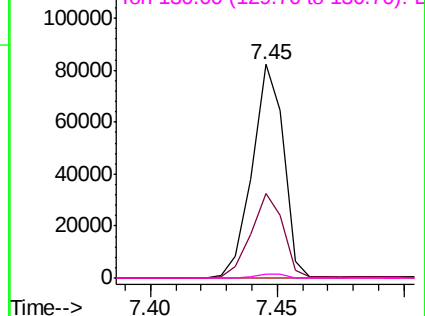



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.17 min Scan# 1035

Delta R.T. -0.01 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 587221


Ion Ratio Lower Upper

136 100

137 11.0 8.6 12.8

54 6.7 5.0 7.6

68 6.5 4.9 7.3



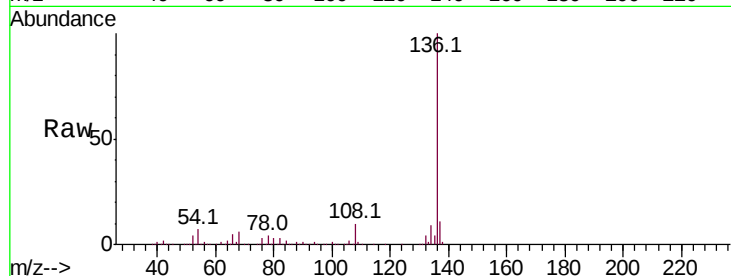


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

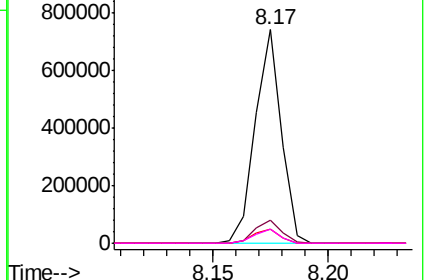

#23

Nitrobenzene-d5

Concen: 54.820 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.01 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02


Tgt Ion: 82 Resp: 528622

Ion Ratio Lower Upper

82 100

128 43.0 36.8 55.2



54 43.4 33.8 50.6




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

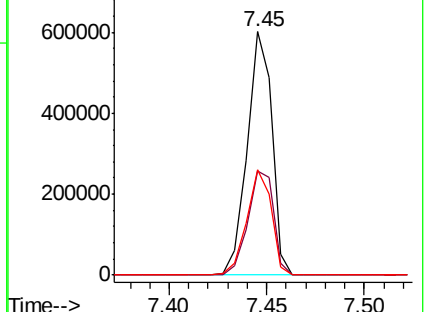

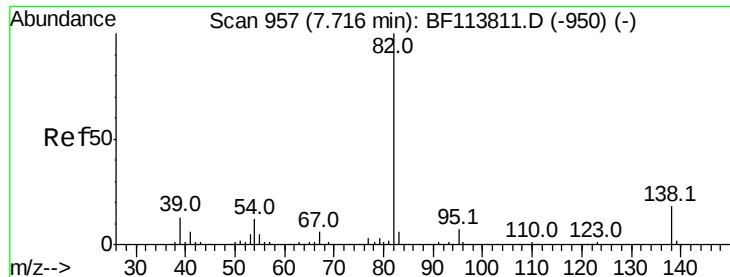

#25

Isophorone

Concen: 26.470 ng

RT: 7.45 min Scan# 911

Delta R.T. -0.27 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 528493

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.2#




138 0.0 14.6 22.0#

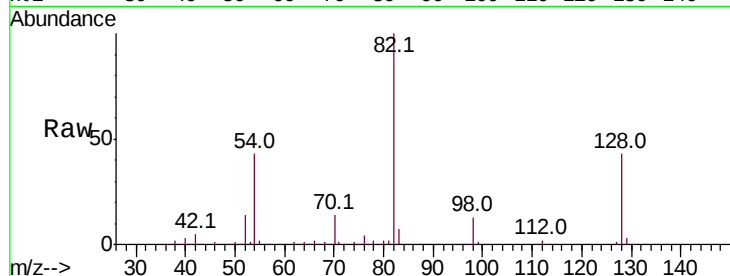

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

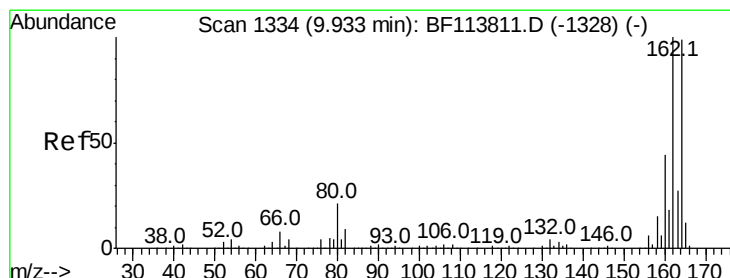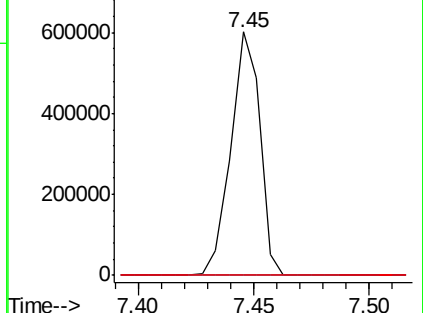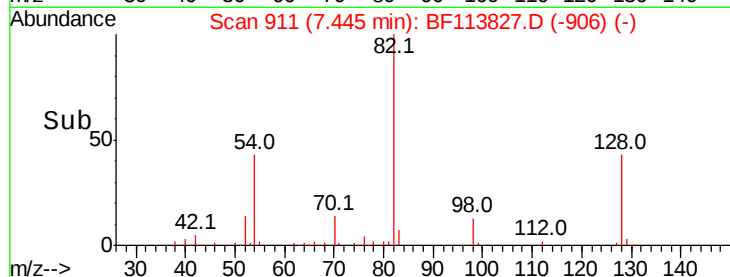

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.93 min Scan# 1333

Delta R.T. -0.01 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02


Tgt Ion:164 Resp: 259937

Ion Ratio Lower Upper

164 100

162 104.1 81.1 121.7



160 46.1 35.8 53.6

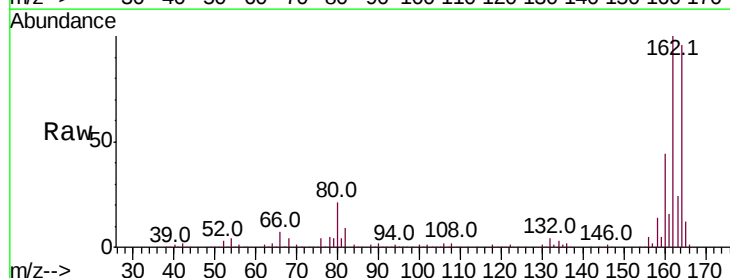


Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1

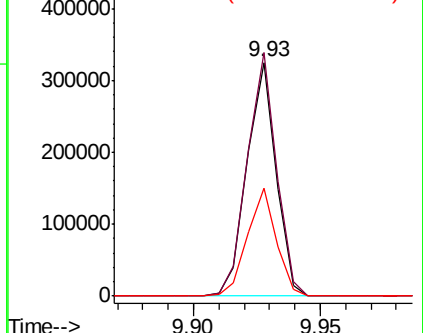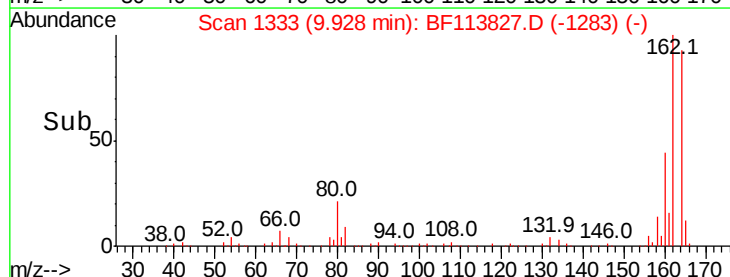



#42

2,4,6-Tribromophenol

Concen: 72.707 ng

RT: 10.71 min Scan# 1466

Delta R.T. -0.01 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02

Instrument :

BNA_F

ClientSampleId :


Tot Ion:330 Resp: 208801

Ion Ratio Lower Upper

330 100

332 95.0 77.5 116.3




141 27.7 22.2 33.2

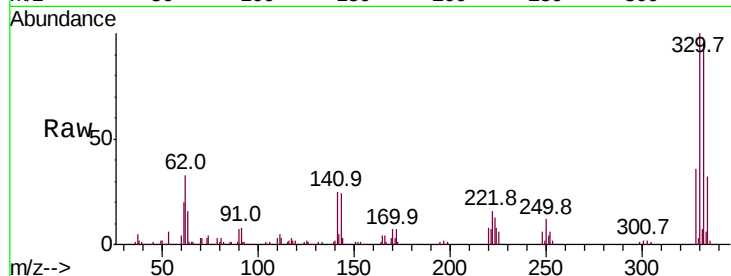

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

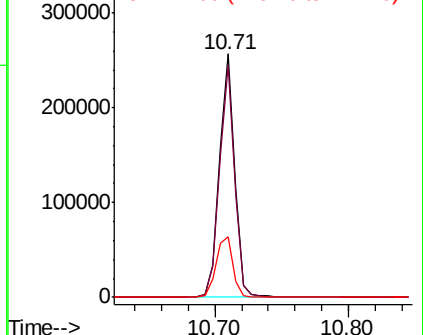

#45

2-Fluorobiphenyl

Concen: 58.984 ng

RT: 9.25 min Scan# 1218

Delta R.T. -0.00 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02


Tgt Ion:172 Resp: 1005356

Ion Ratio Lower Upper

172 100

171 36.0 29.4 44.0



170 23.7 19.9 29.9




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

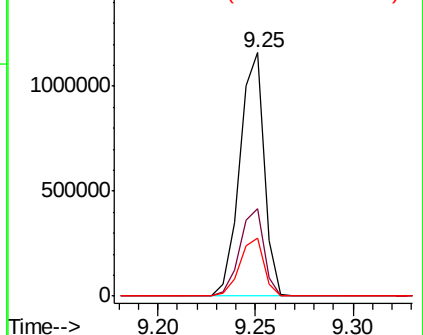



#50

Dimethylphthalate

Concen: 5.529 ng

RT: 9.64 min Scan# 1284

Delta R.T. -0.01 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 100574

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2




164 9.8 8.5 12.7



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

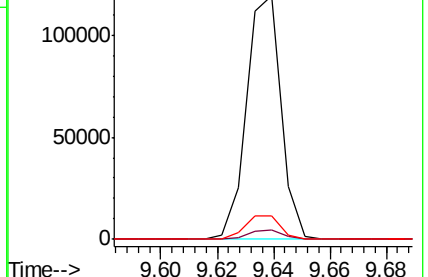

#51

2,6-Dinitrotoluene

Concen: 8.430 ng

RT: 9.93 min Scan# 1333

Delta R.T. 0.22 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02


Tgt Ion:165 Resp: 33842

Ion Ratio Lower Upper

165 100

63 1.2 33.8 50.8#



89 1.0 38.2 57.2#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1



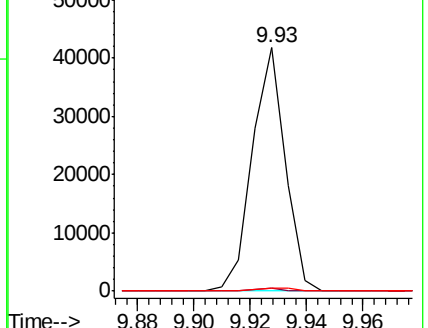
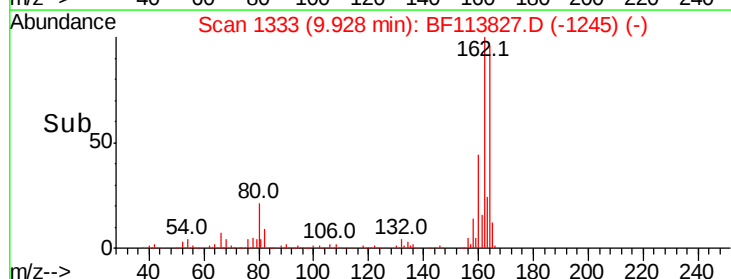




#57
 2,4-Dinitrotoluene
 Concen: 6.795 ng
 RT: 9.93 min Scan# 1333
 Delta R.T. -0.18 min
 Lab File: BF113827.D
 Acq: 18 Apr 2019 20:02




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:165	Resp: 33842
Ion Ratio	Lower Upper
165 100	
63 1.2	27.4 41.0#
89 1.0	51.8 77.6#
182 0.0	2.2 3.2#

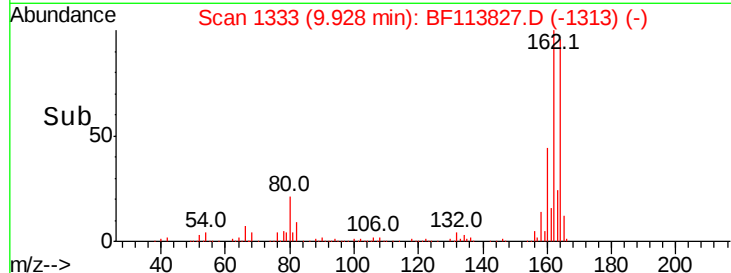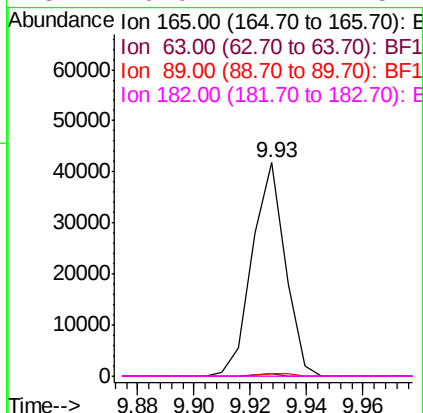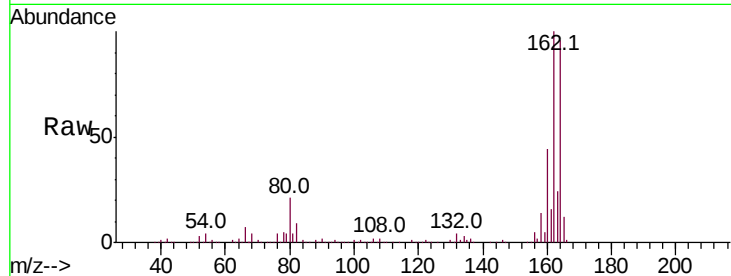

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.41 min Scan# 1585
 Delta R.T. -0.00 min
 Lab File: BF113827.D
 Acq: 18 Apr 2019 20:02

Tgt	Ion:188	Resp:	461032
Ion	Ratio	Lower	Upper
188	100		
94	9.0	8.2	12.4
80	9.5	9.0	13.6

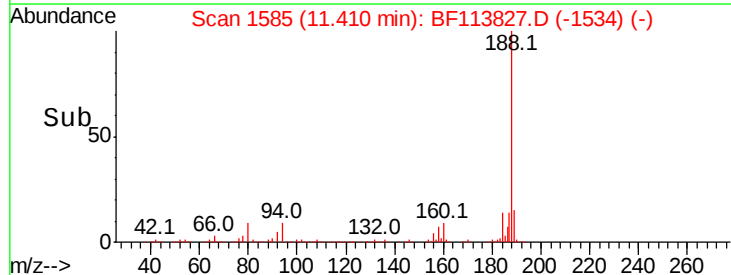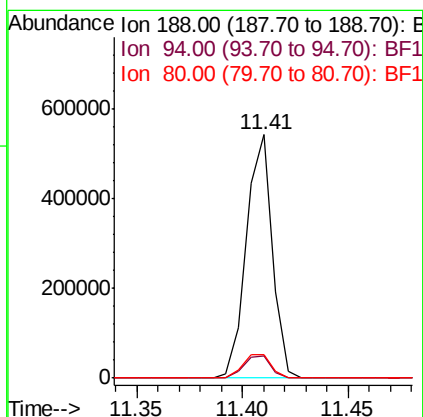

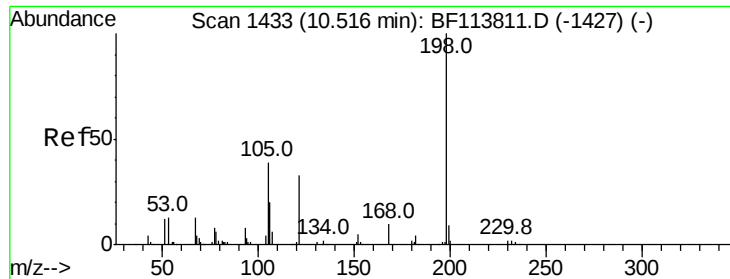

#65

4,6-Dinitro-2-methylphenol

Concen: 7.082 ng

RT: 10.71 min Scan# 1466

Delta R.T. 0.19 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02

Instrument :

BNA_F

ClientSampleId :


Tot Ion:198 Resp: 345

Ion Ratio Lower Upper

198 100

51 207.5 11.1 51.1#




105 234.4 20.7 60.7#

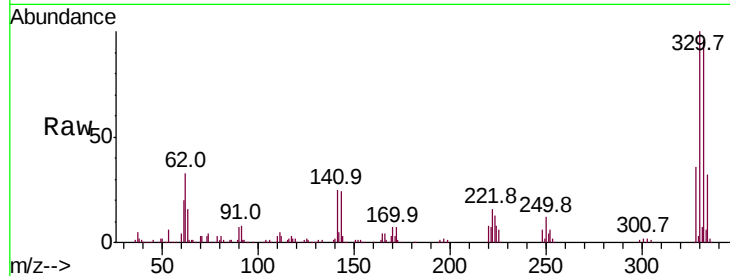

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

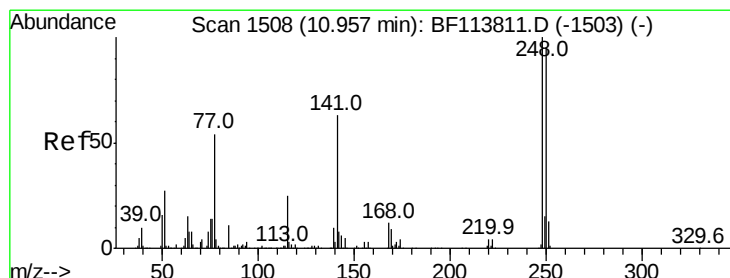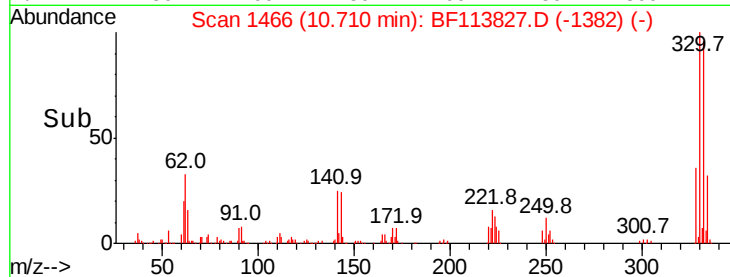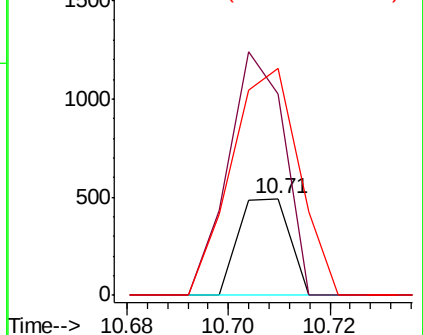

#67

4-Bromophenyl-phenylether

Concen: 2.370 ng

RT: 10.71 min Scan# 1466

Delta R.T. -0.25 min

Lab File: BF113827.D

Acq: 18 Apr 2019 20:02


Tgt Ion:248 Resp: 12830

Ion Ratio Lower Upper

248 100

250 202.2 75.8 113.6#



141 400.0 50.2 75.4#

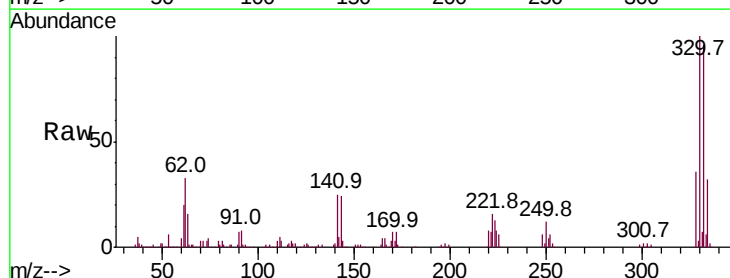


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E



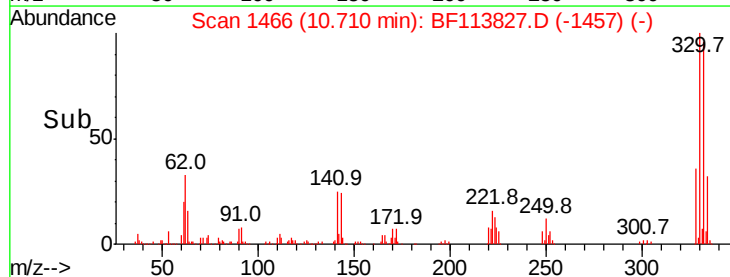
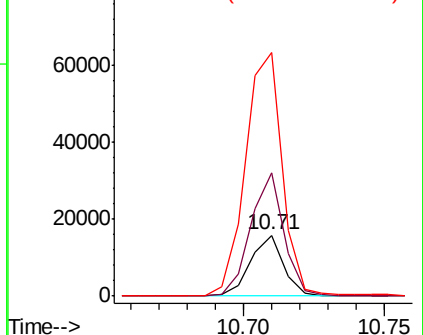




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.04 min Scan# 2032
Delta R.T. -0.01 min
Lab File: BF113827.D
Acq: 18 Apr 2019 20:02




Instrument :
BNA_F
ClientSampleId :


Tot Ion:240 Resp: 511463
Ion Ratio Lower Upper
240 100
120 10.7 9.3 13.9
236 25.8 21.2 31.8

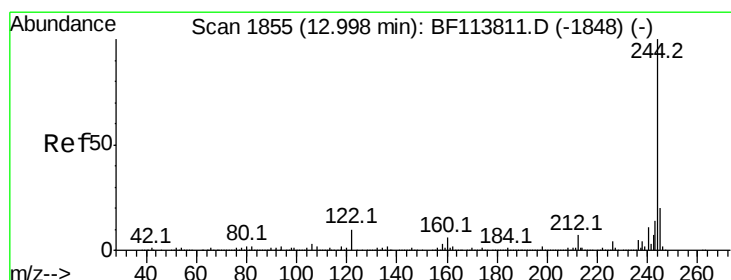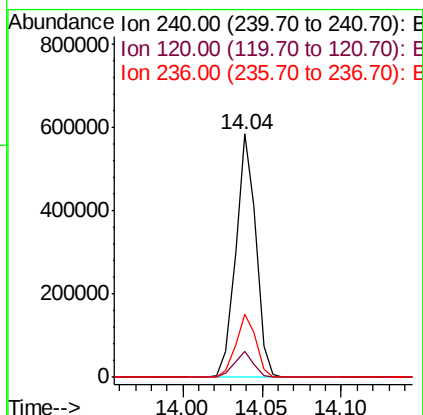

#79
Terphenyl-d14
Concen: 45.103 ng
RT: 12.99 min Scan# 1854
Delta R.T. -0.01 min
Lab File: BF113827.D
Acq: 18 Apr 2019 20:02

Tgt Ion:244 Resp: 1100095
Ion Ratio Lower Upper
244 100
212 6.4 5.4 8.2
122 9.3 7.6 11.4

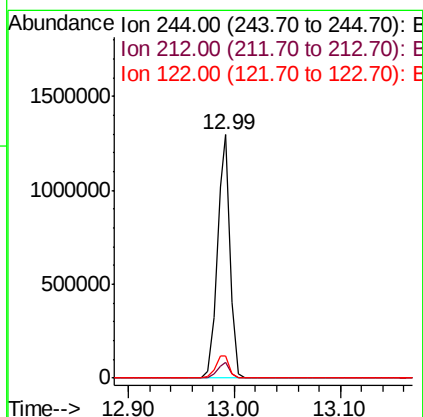


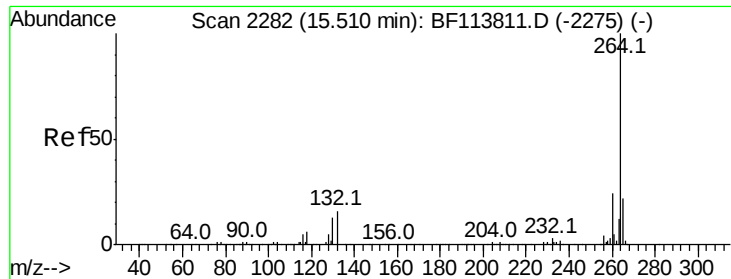

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.51 min Scan# 2282
 Delta R.T. -0.00 min
 Lab File: BF113827.D
 Acq: 18 Apr 2019 20:02

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.1	18.9	28.3
265	22.0	17.3	25.9



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

