




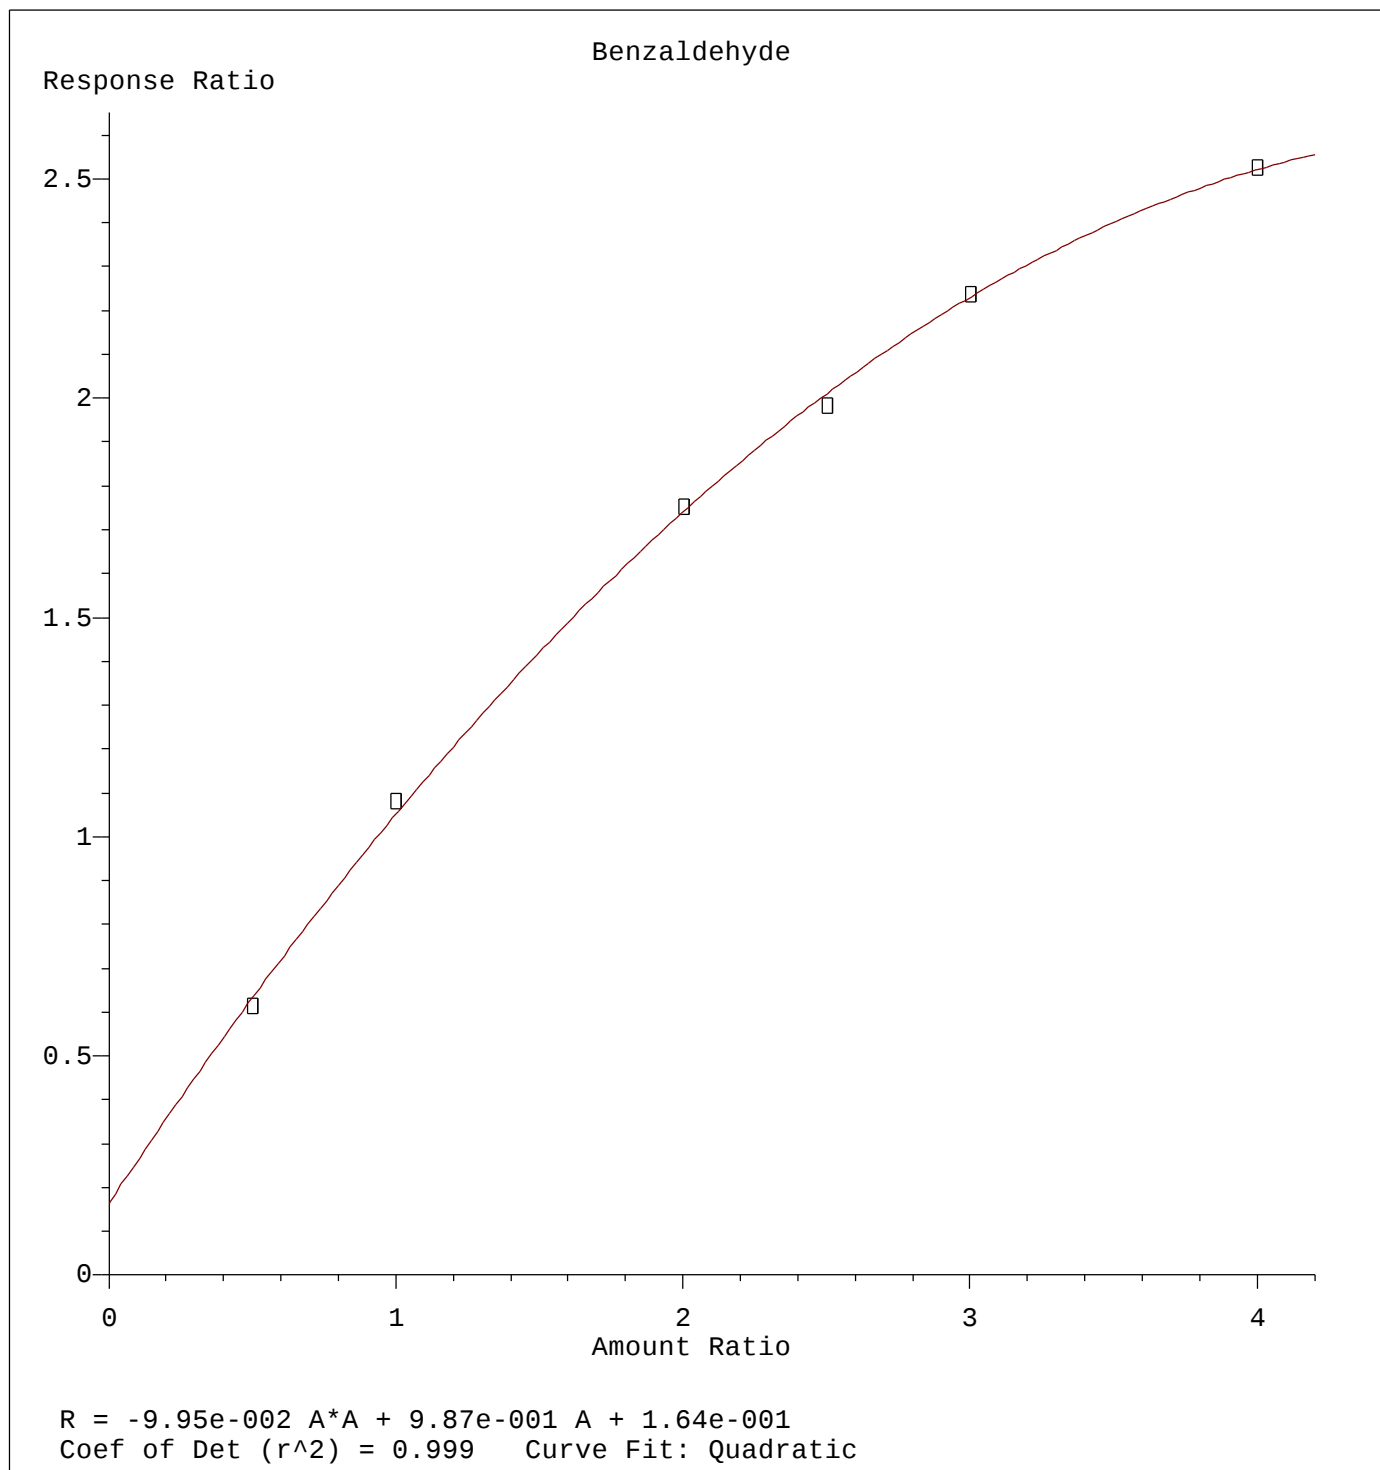

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Calibration Table Last Updated: Thu Apr 18 13:55:51 2019

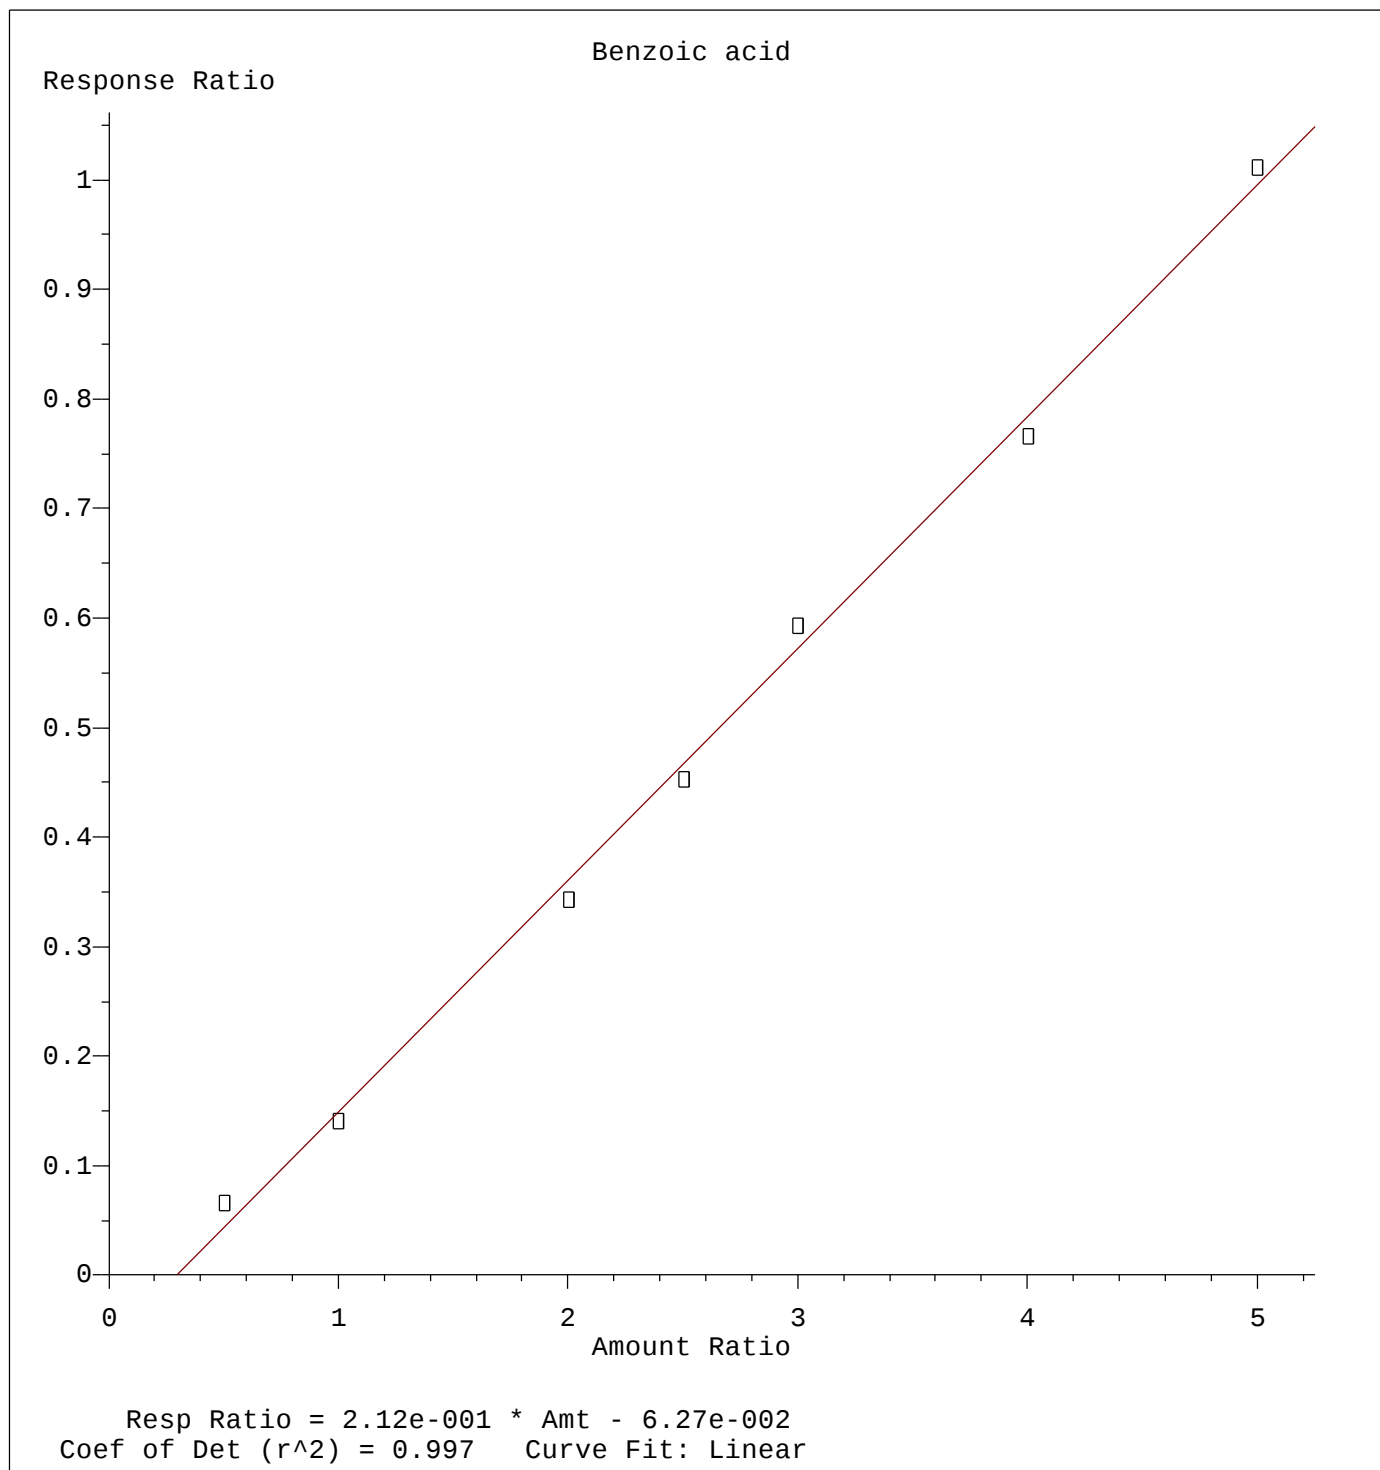


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Calibration Table Last Updated: Thu Apr 18 13:55:51 2019

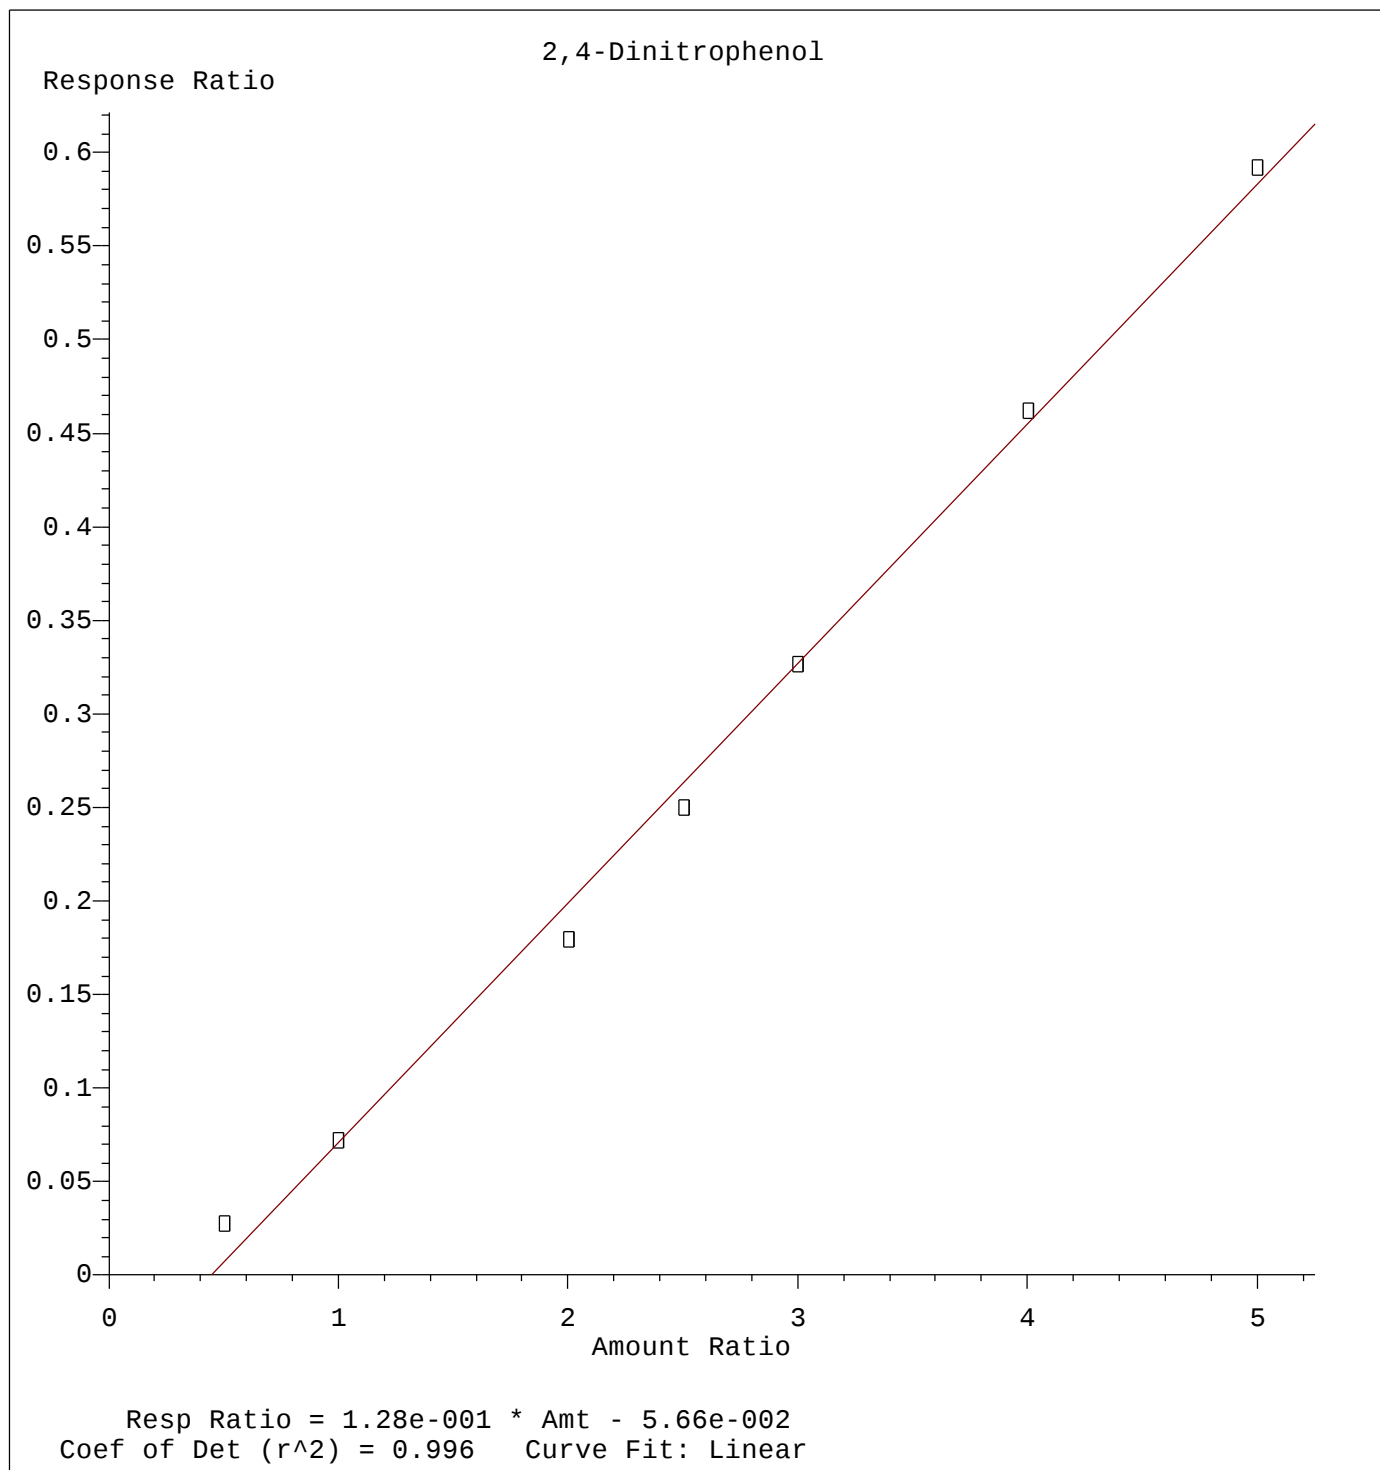


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Calibration Table Last Updated: Thu Apr 18 13:55:51 2019

4,6-Dinitro-2-methylphenol

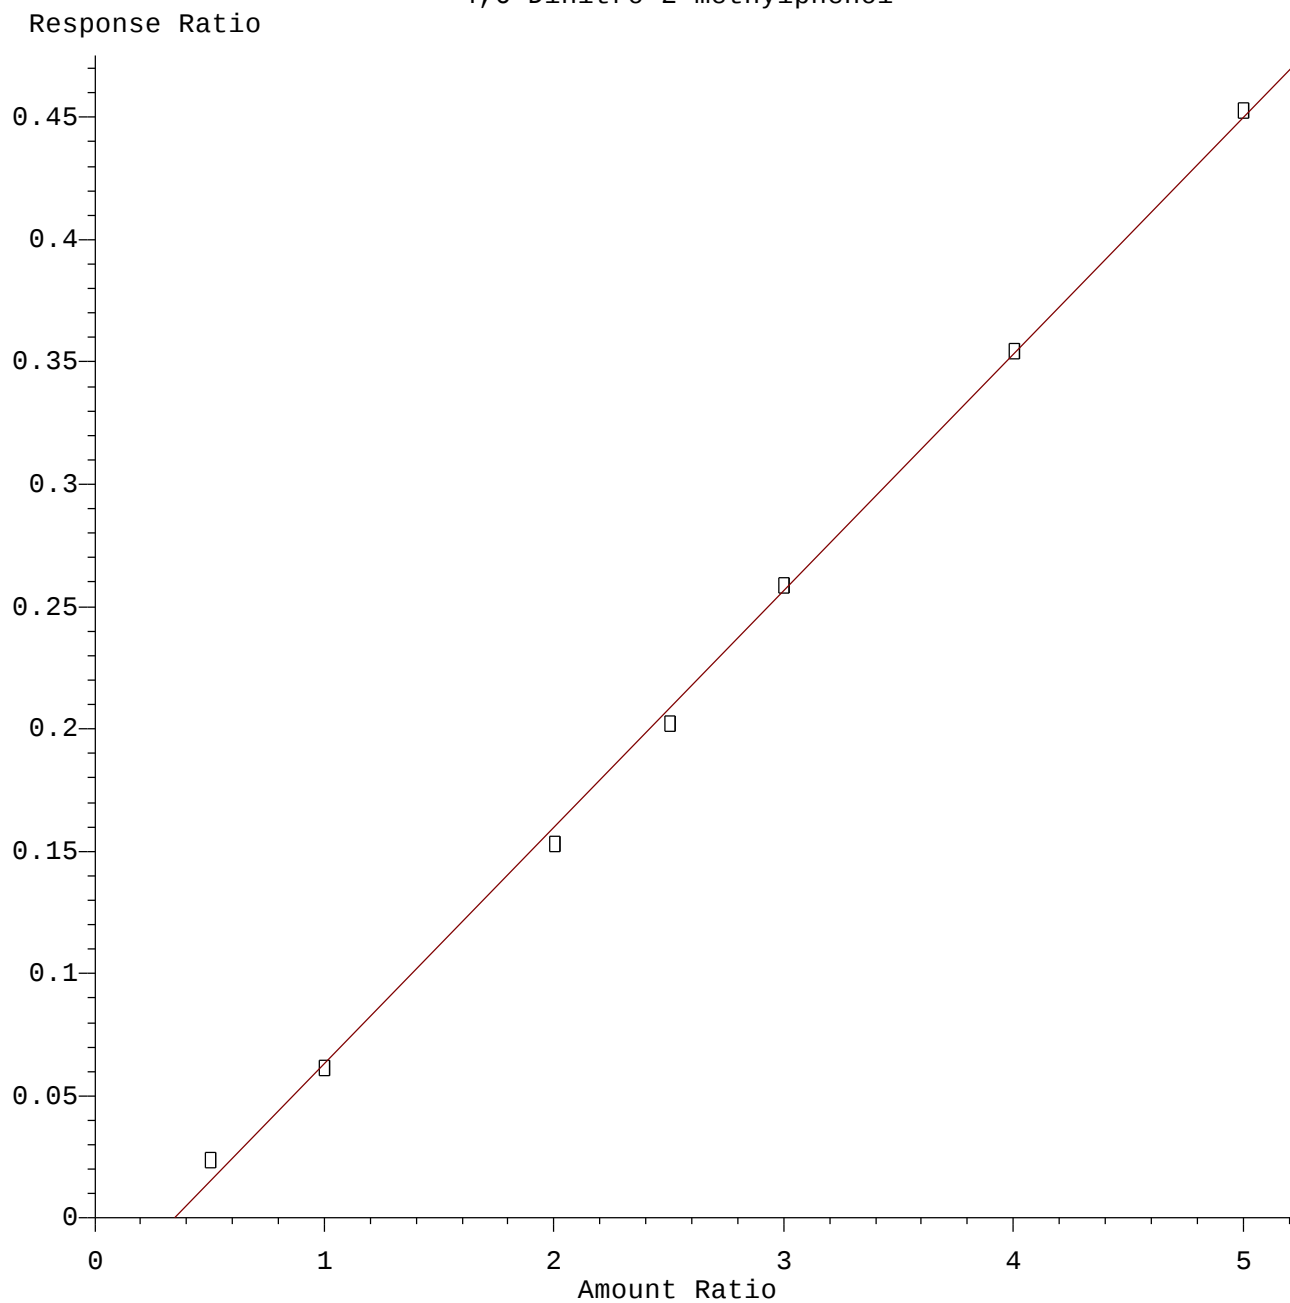

Resp Ratio = $9.66 \times 10^{-2} \times \text{Amt} - 3.35 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Calibration Table Last Updated: Thu Apr 18 13:55:51 2019

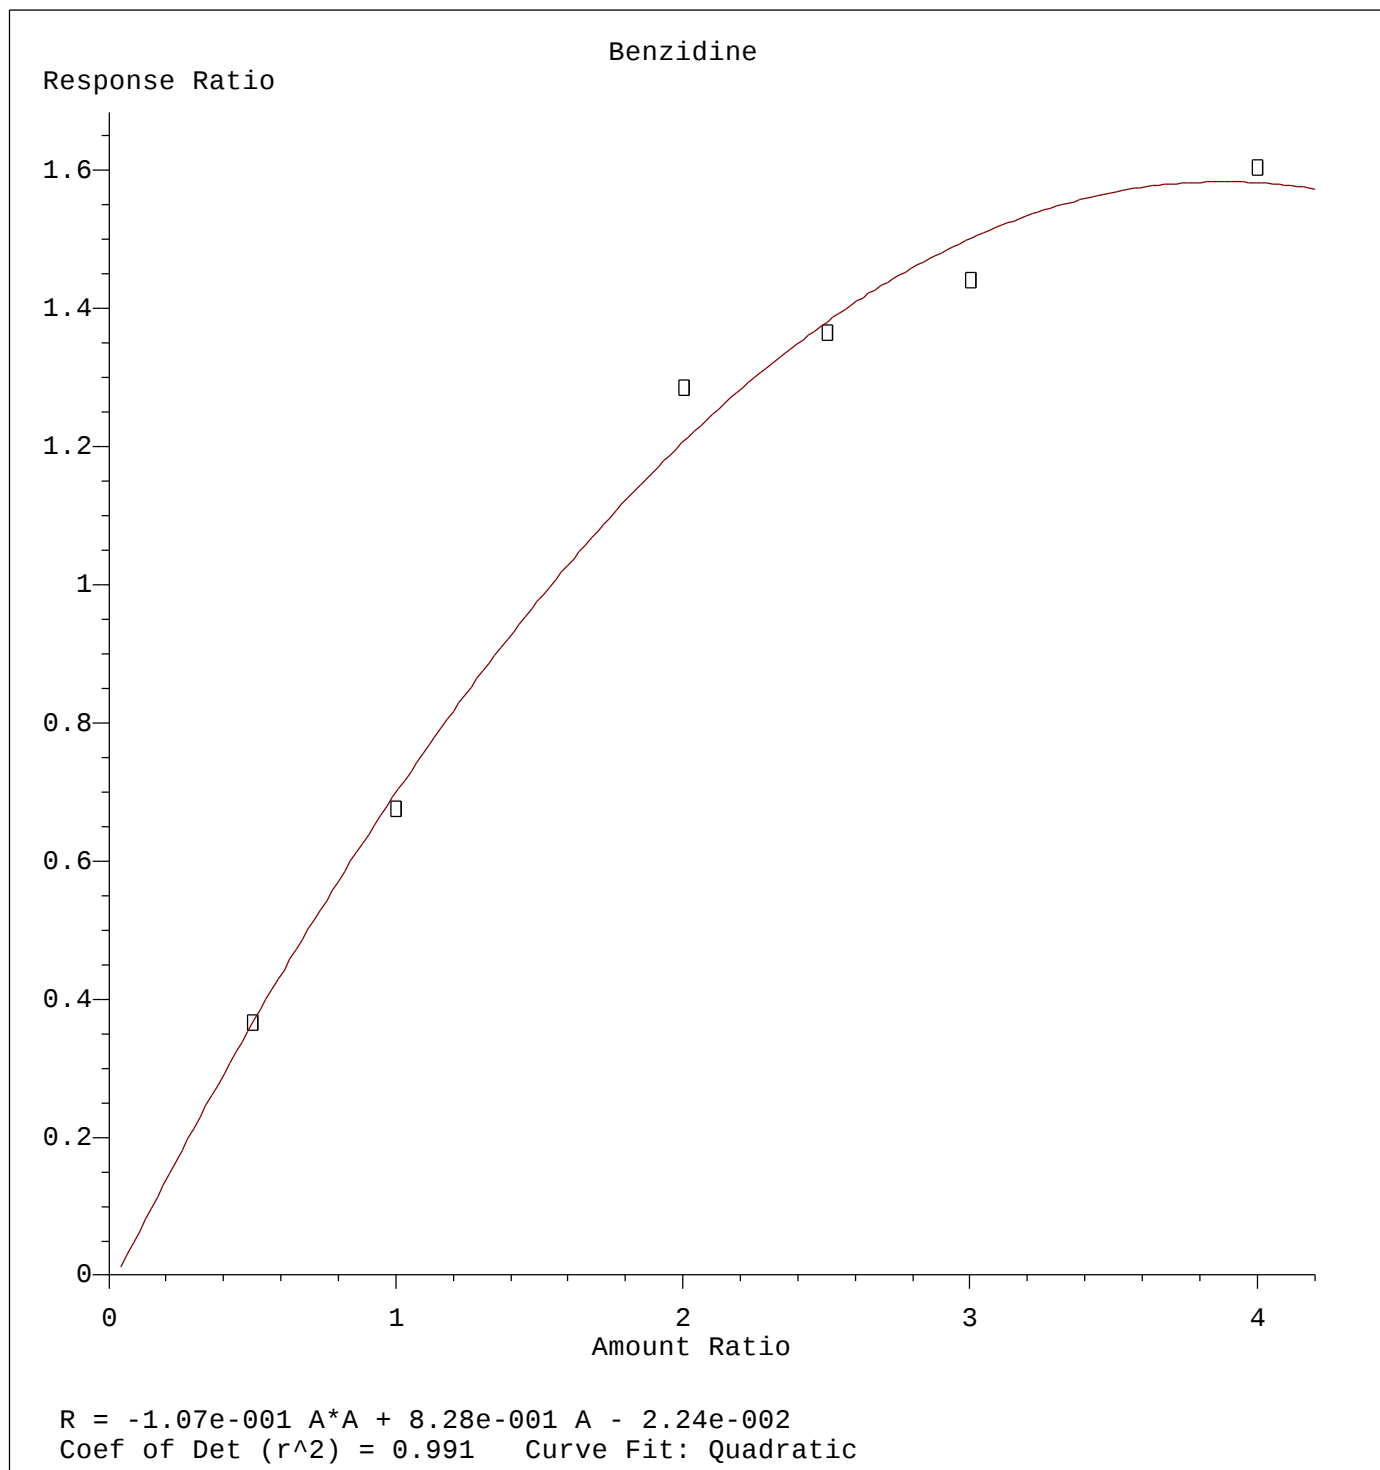

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Calibration Table Last Updated: Thu Apr 18 13:55:51 2019