
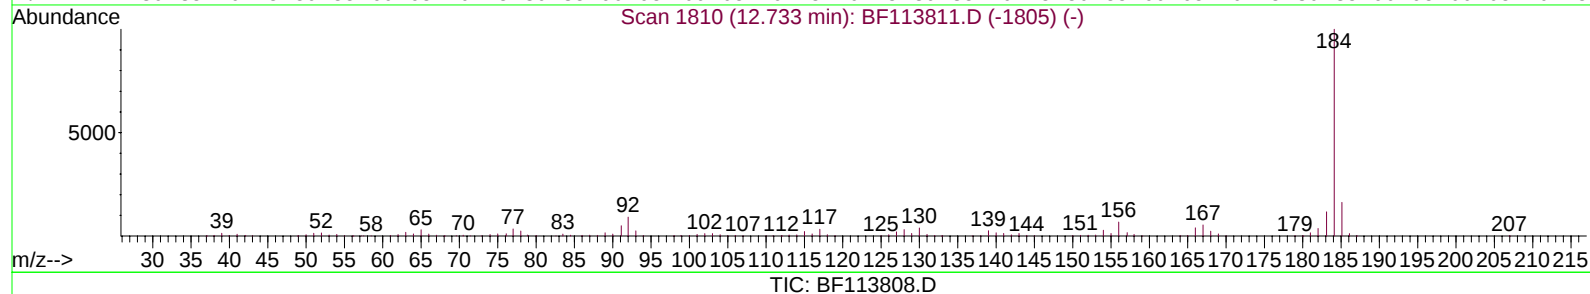
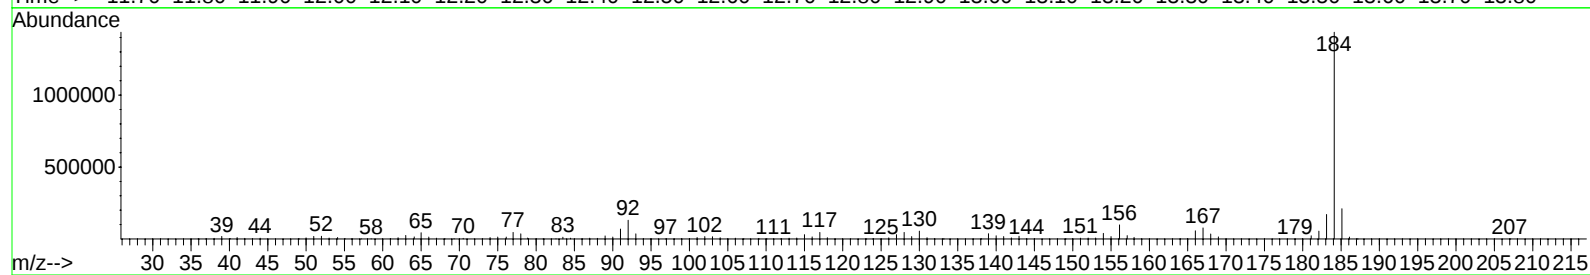


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF041819\
Data File : BF113808.D
Acq On : 18 Apr 2019 7:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 17:57:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 13:55:51 2019
Response via : Initial Calibration

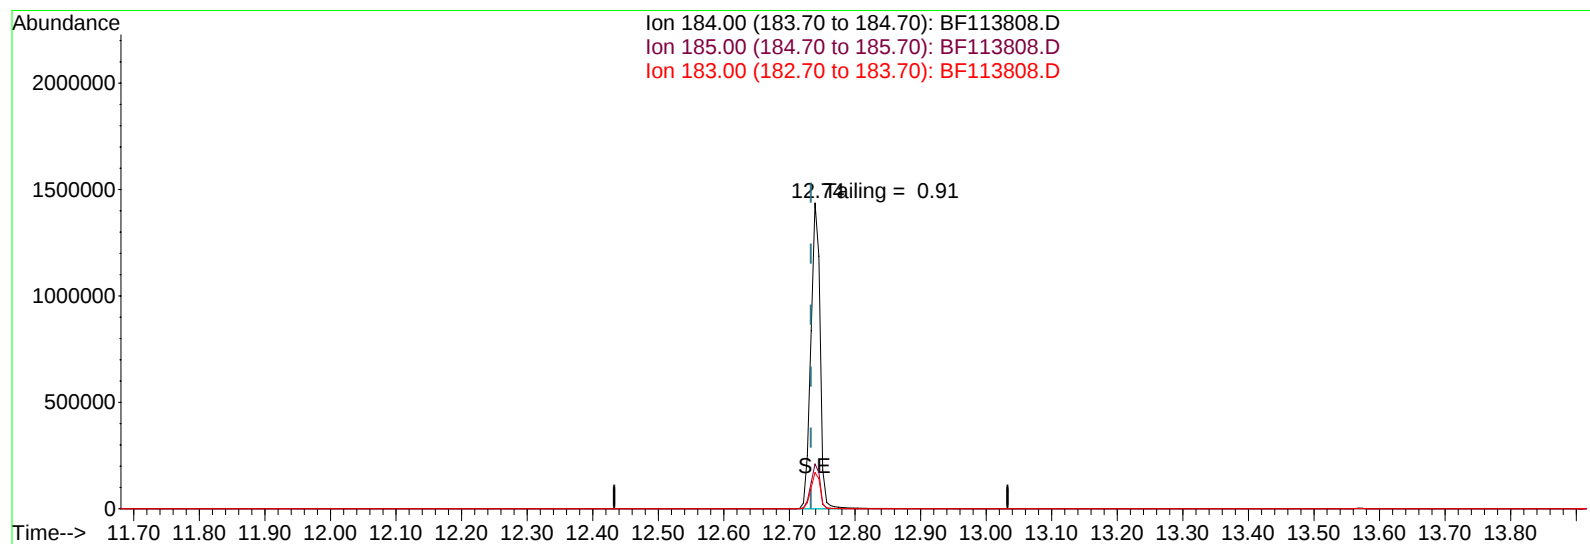

(77) Benzidine




12.739min (+0.006) -20.00ng

response 1422267

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.63
183.00	11.70	11.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF041819\
Data File : BF113808.D
Acq On : 18 Apr 2019 7:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 17:57:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 13:55:51 2019
Response via : Initial Calibration

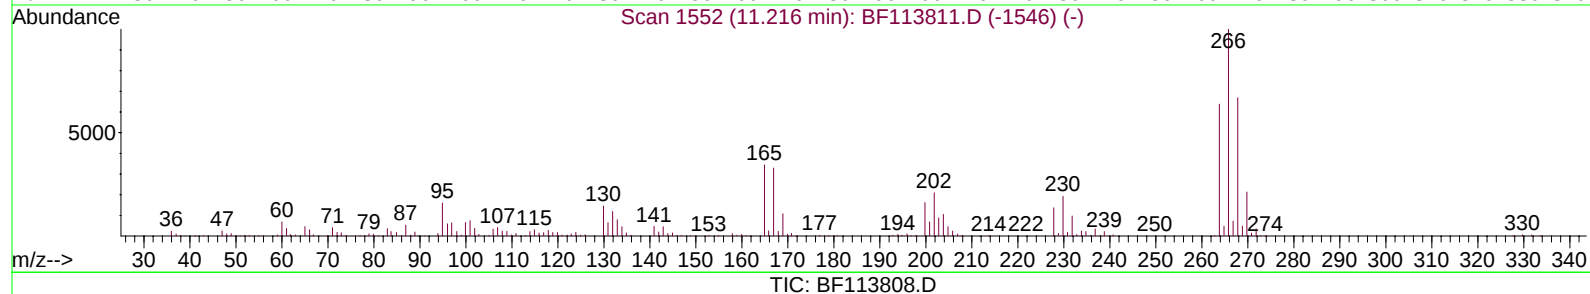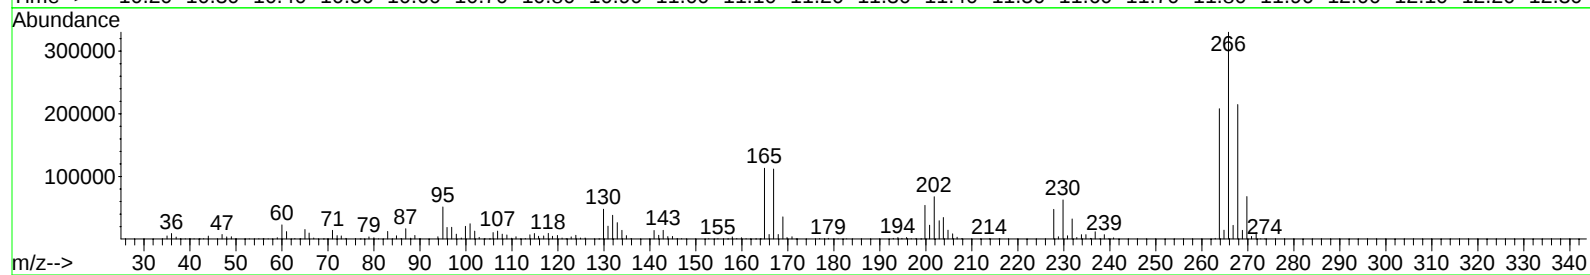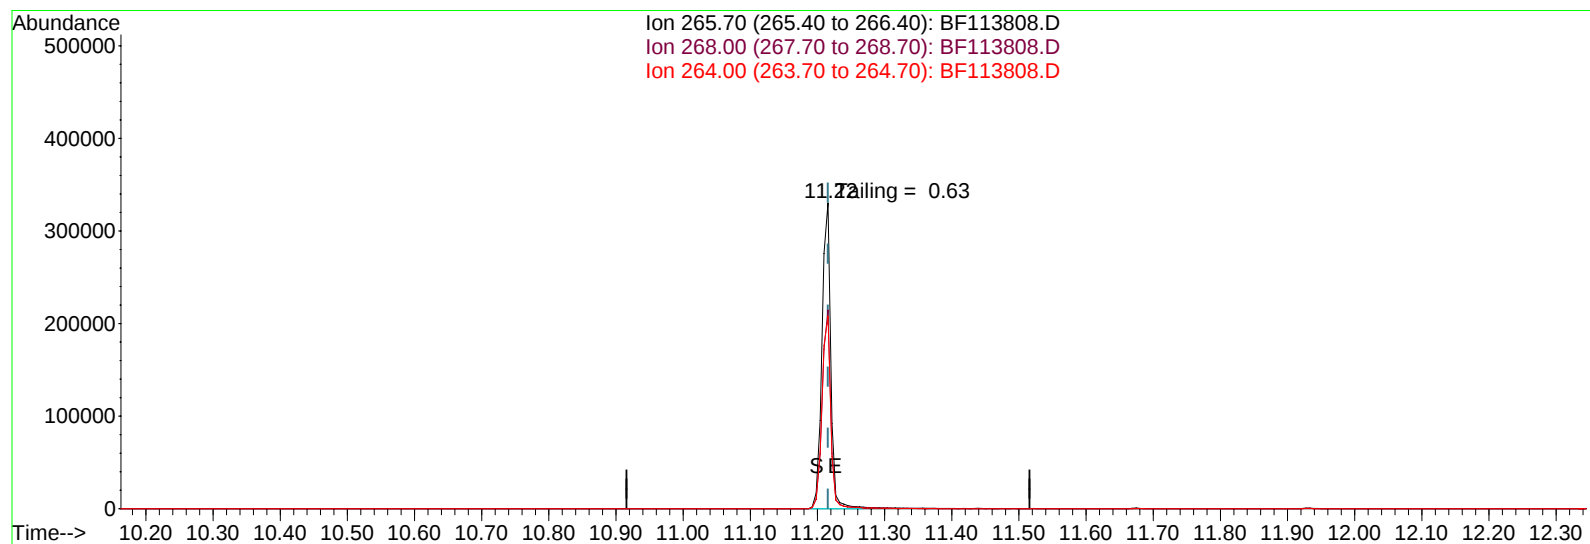

(70) Pentachlorophenol (C)

11.216min (-0.000) 83401.48ng

response 304078

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	65.02
264.00	63.80	63.00
0.00	0.00	0.00