


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041819\
 Data File : BF113808.D
 Acq On : 18 Apr 2019 7:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 18 13:55:51 2019

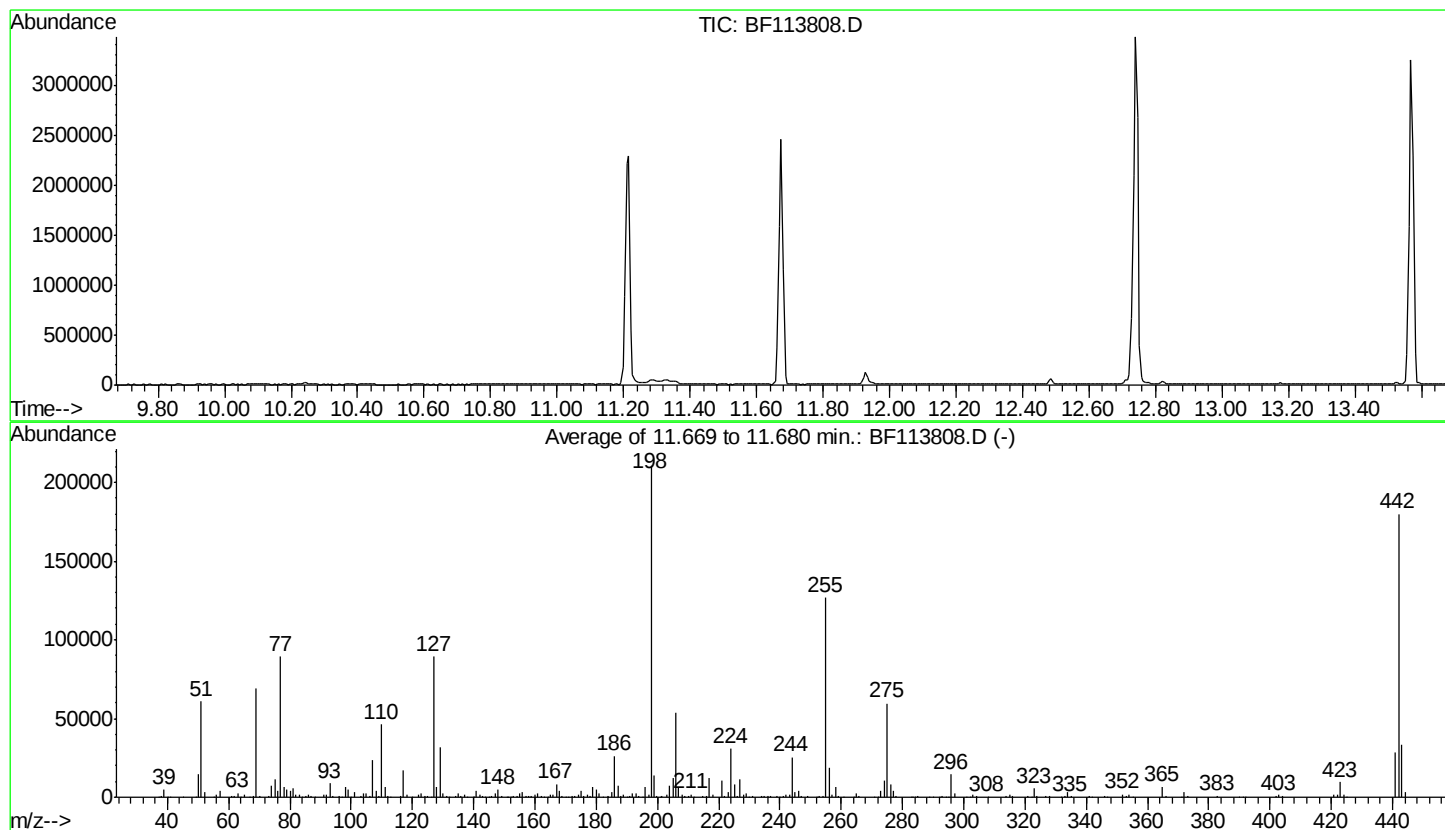

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	60672	PASS
68	69	0.00	2	1.8	1226	PASS
69	198	0.00	100	32.9	69401	PASS
70	69	0.00	2	0.8	554	PASS
127	198	10	80	42.4	89301	PASS
197	198	0.00	2	0.7	1381	PASS
198	198	100	100	100.0	210688	PASS
199	198	5	9	6.7	14032	PASS
275	198	10	60	28.2	59424	PASS
365	198	1	100	3.2	6714	PASS
441	198	0.01	100	13.4	28296	PASS
442	198	50	100	85.5	180077	PASS
443	442	15	24	18.5	33341	PASS