


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041819\
Data File : BF113817.D
Acq On : 18 Apr 2019 15:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 18 13:55:51 2019

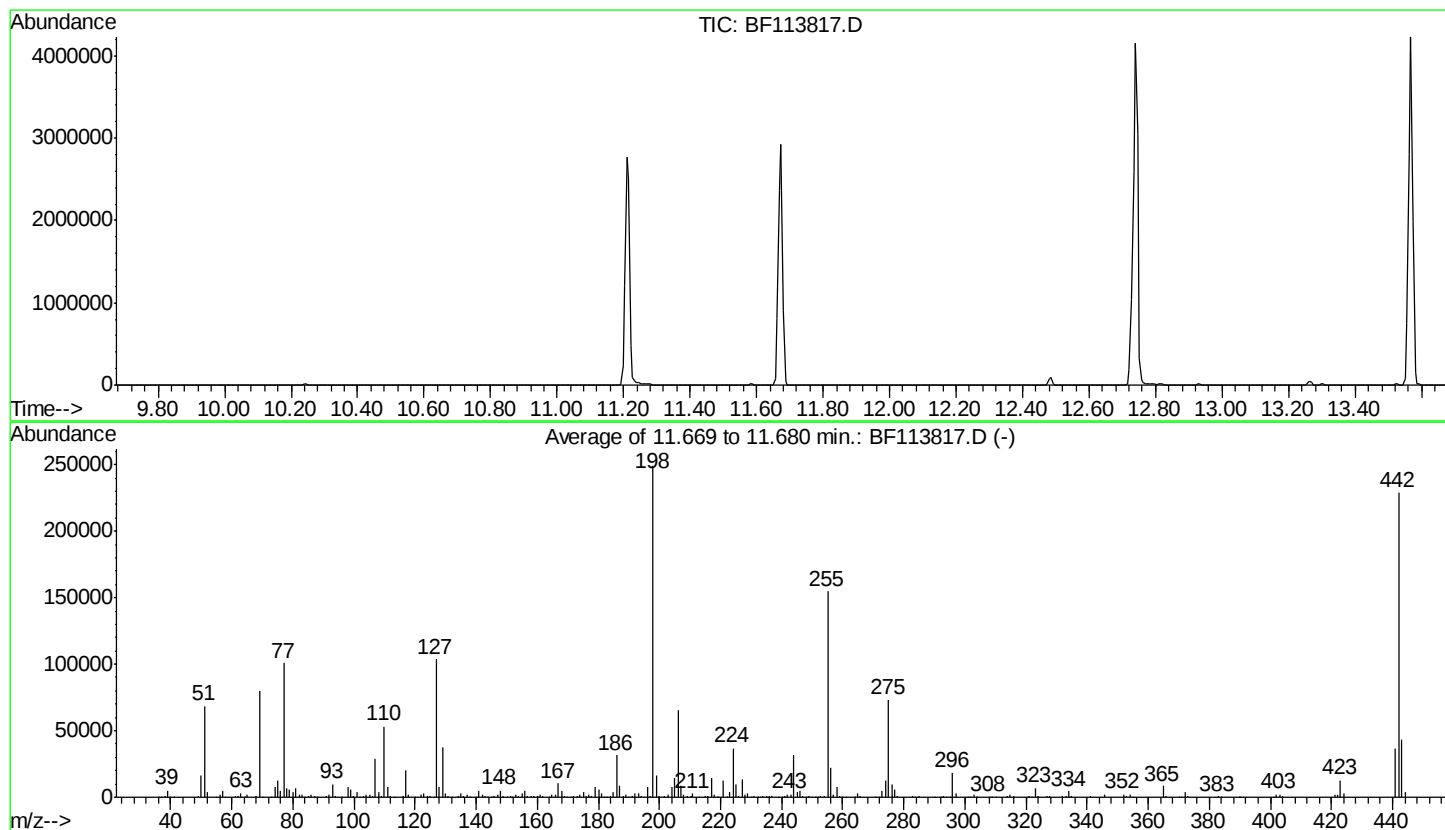

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	68563	PASS
68	69	0.00	2	1.7	1388	PASS
69	198	0.00	100	32.1	80053	PASS
70	69	0.00	2	0.5	388	PASS
127	198	10	80	41.6	103634	PASS
197	198	0.00	2	0.3	840	PASS
198	198	100	100	100.0	249240	PASS
199	198	5	9	6.6	16557	PASS
275	198	10	60	29.5	73586	PASS
365	198	1	100	3.4	8491	PASS
441	198	0.01	100	14.7	36645	PASS
442	198	50	100	91.8	228906	PASS
443	442	15	24	18.9	43354	PASS