

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041919\
 Data File : BF113866.D
 Acq On : 19 Apr 2019 18:39
 Operator : JU/SJ
 Sample : K2198-05 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-03-041719

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	579	583	595	rBV	702332	612561	48.16%	5.076%
2	6.516	749	753	756	rBV	770728	607857	47.79%	5.037%
3	6.540	756	757	763	rVB	33912	24348	1.91%	0.202%
4	6.669	775	779	782	rBV	737836	643879	50.62%	5.335%
5	6.904	815	819	822	rBV	1063432	920111	72.34%	7.624%
6	7.057	841	845	848	rBV	632879	487781	38.35%	4.042%
7	7.451	909	912	916	rVB	410394	314458	24.72%	2.606%
8	8.181	1032	1036	1040	rBV	1273897	1086694	85.44%	9.005%
9	9.257	1215	1219	1222	rBV	864074	659027	51.82%	5.461%
10	9.645	1282	1285	1288	rBV	60182	49765	3.91%	0.412%
11	9.939	1331	1335	1339	rBV	1373345	1124868	88.44%	9.321%
12	10.375	1405	1409	1414	rVB3	16127	14404	1.13%	0.119%
13	10.722	1464	1468	1473	rBV	472102	385588	30.32%	3.195%
14	10.845	1486	1489	1494	rBV3	23050	28834	2.27%	0.239%
15	11.298	1564	1566	1568	rBV2	24622	19732	1.55%	0.164%
16	11.328	1568	1571	1576	rVB2	17305	19534	1.54%	0.162%
17	11.428	1584	1588	1591	rBV	1476326	1261185	99.16%	10.451%
18	11.451	1591	1592	1595	rVV	85188	48115	3.78%	0.399%
19	11.504	1599	1601	1604	rVB	19726	17464	1.37%	0.145%
20	11.733	1637	1640	1643	rBV2	26039	22362	1.76%	0.185%
21	11.833	1653	1657	1659	rBV	24588	24518	1.93%	0.203%
22	11.945	1673	1676	1677	rBV	13923	14438	1.14%	0.120%
23	11.963	1677	1679	1684	rVB2	63728	64976	5.11%	0.538%
24	12.057	1692	1695	1697	rBV3	21800	22941	1.80%	0.190%
25	12.157	1709	1712	1714	rBV	26675	23574	1.85%	0.195%
26	12.386	1749	1751	1753	rBV3	15617	16346	1.29%	0.135%
27	12.463	1758	1764	1767	rBV7	15284	26557	2.09%	0.220%
28	12.522	1771	1774	1777	rBV2	26315	27619	2.17%	0.229%
29	12.557	1777	1780	1782	rBV	103559	109434	8.60%	0.907%
30	12.580	1782	1784	1787	rVB3	72219	62625	4.92%	0.519%
31	12.692	1800	1803	1807	rVB	89816	83254	6.55%	0.690%
32	12.804	1820	1822	1826	rBV5	16569	16710	1.31%	0.138%
33	12.945	1843	1846	1849	rVB	82123	68329	5.37%	0.566%
34	12.980	1850	1852	1857	rVB2	32430	30167	2.37%	0.250%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041919\
Data File : BF113866.D
Acq On : 19 Apr 2019 18:39
Operator : JU/SJ
Sample : K2198-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-041719

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.110	1870	1874	1882	rBV	838553	818009	64.32%	6.778%
36	13.392	1920	1922	1926	rVB	53207	52419	4.12%	0.434%
37	13.545	1946	1948	1950	rVB2	27913	21998	1.73%	0.182%
38	13.804	1989	1992	1995	rBV	49426	49949	3.93%	0.414%
39	14.363	2082	2087	2091	rBV	1176120	1271877	100.00%	10.539%
40	16.168	2390	2394	2402	rVB	714102	913578	71.83%	7.570%


Sum of corrected areas: 12067885

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041919\
Data File : BF113866.D
Acq On : 19 Apr 2019 18:39
Operator : JU/SJ
Sample : K2198-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-041719

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

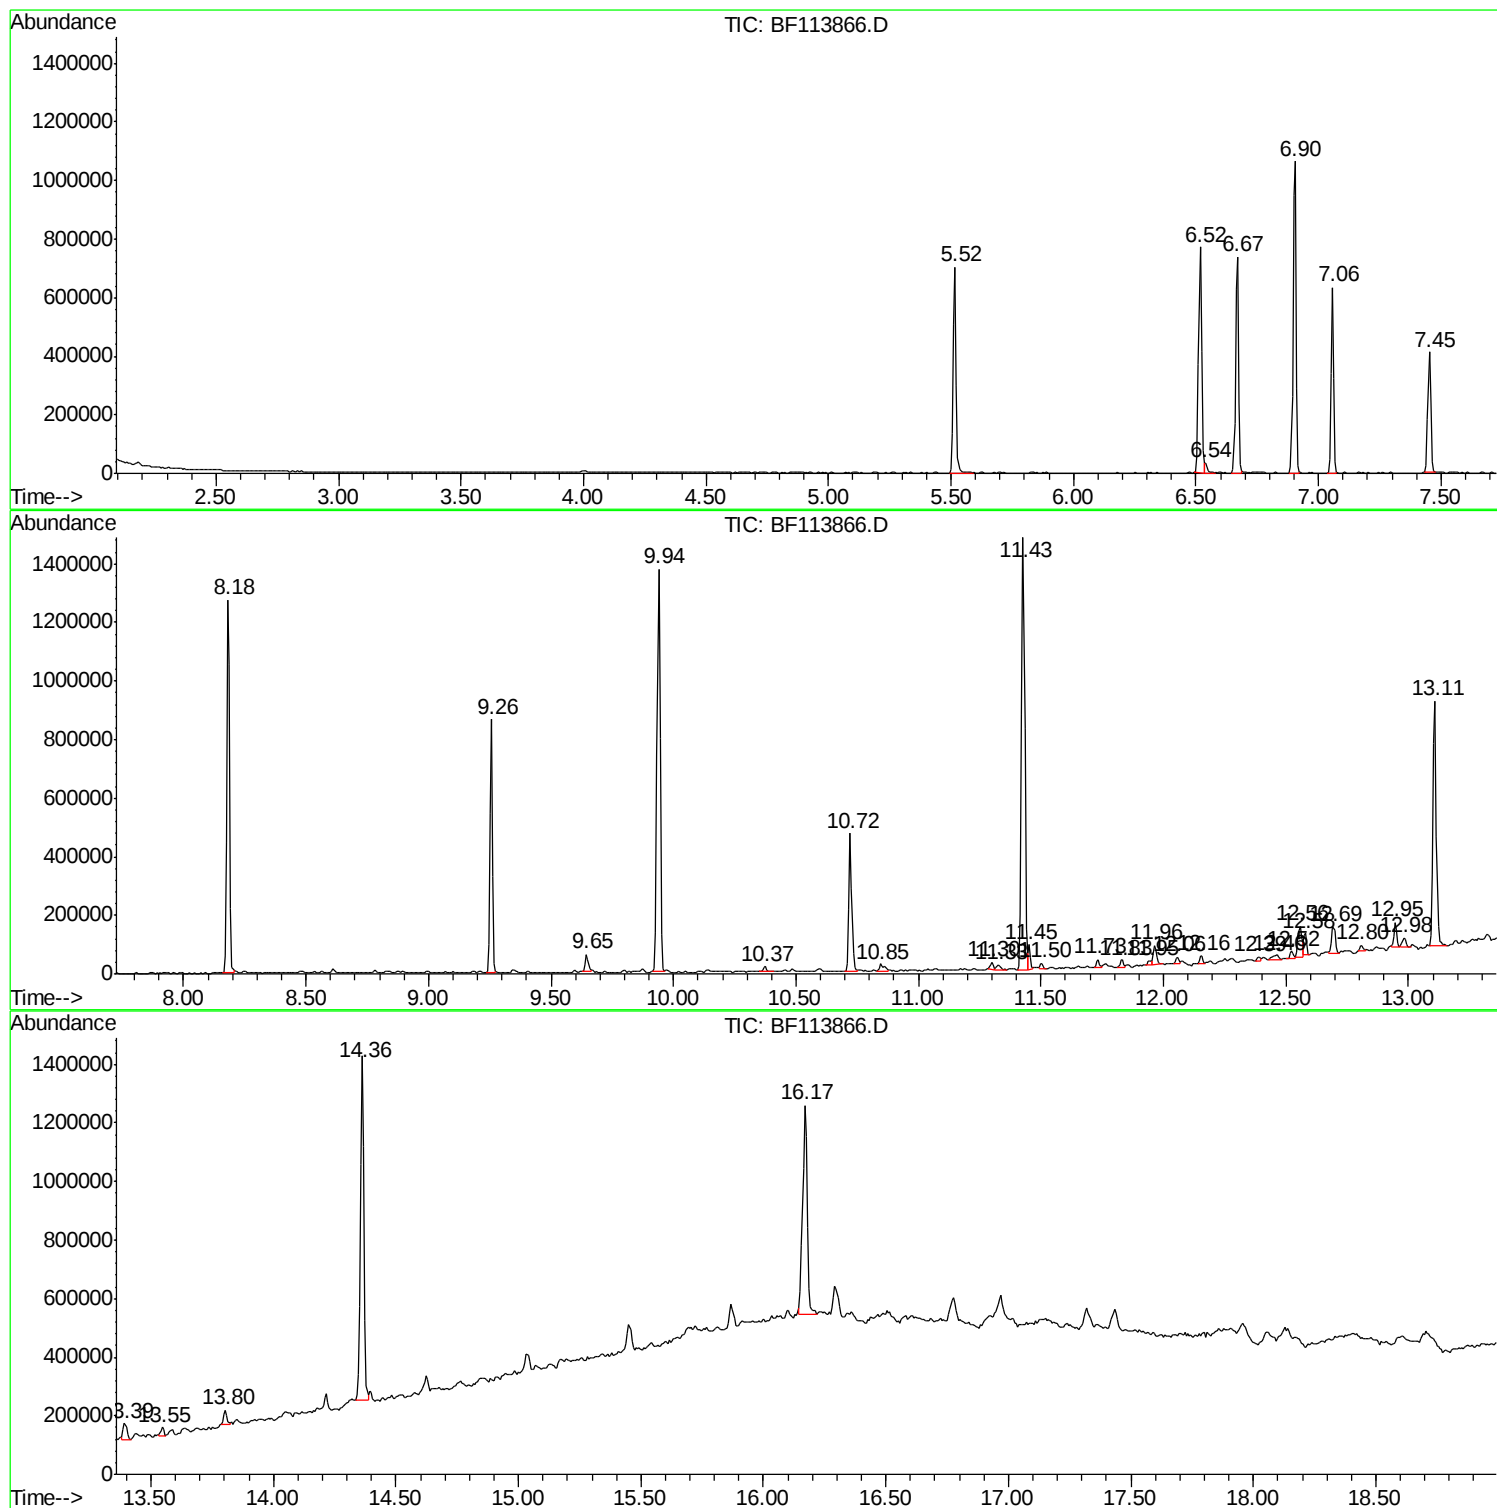

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041919\
Data File : BF113866.D
Acq On : 19 Apr 2019 18:39
Operator : JU/SJ
Sample : K2198-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-041719







Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.67	14.00 ng	643879	1,4-Dichlorobenzene-d4	6.90

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	16
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

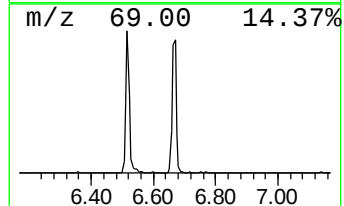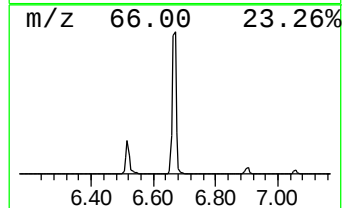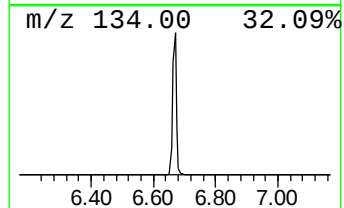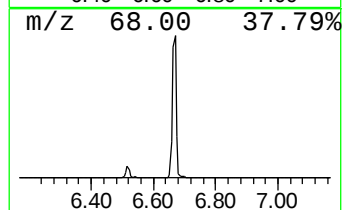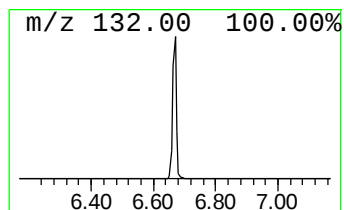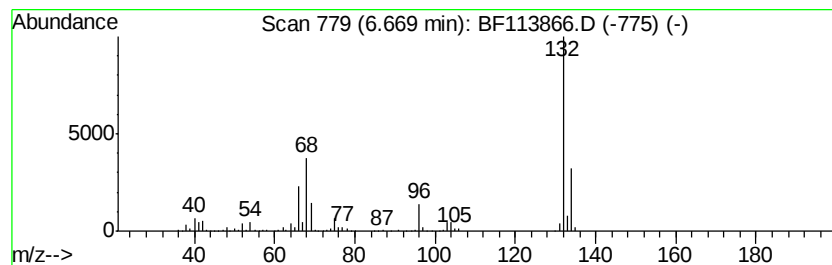

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041919\
Data File : BF113866.D
Acq On : 19 Apr 2019 18:39
Operator : JU/SJ
Sample : K2198-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-041719

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.67	6.67	14.0	ng	643879	1	6.90	920111	20.0