


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF041919\
 Data File : BF113849.D
 Acq On : 19 Apr 2019 10:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 18 13:55:51 2019

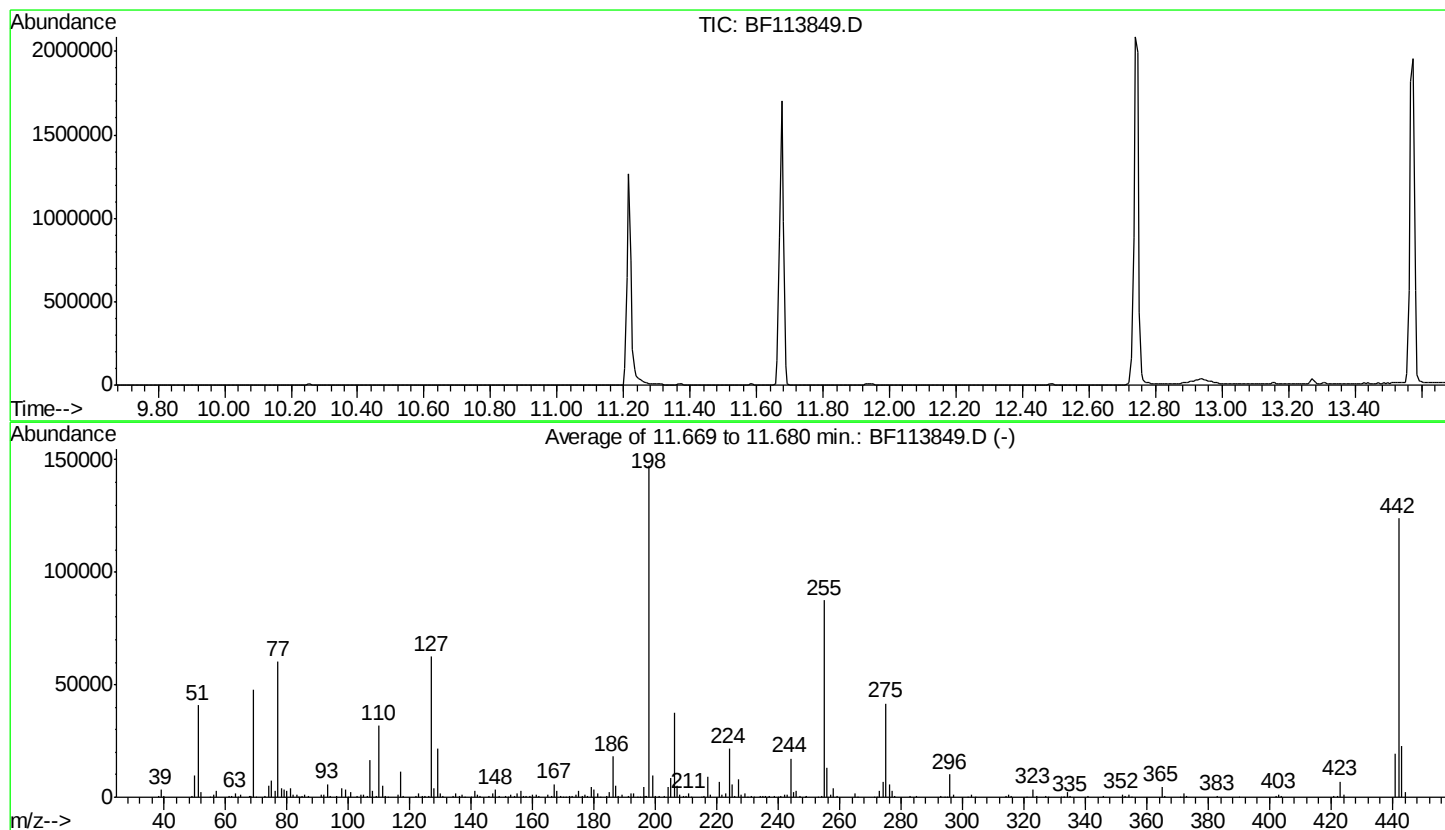

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.7	40880	PASS
68	69	0.00	2	1.0	468	PASS
69	198	0.00	100	32.5	47848	PASS
70	69	0.00	2	0.2	101	PASS
127	198	10	80	42.3	62418	PASS
197	198	0.00	2	0.4	595	PASS
198	198	100	100	100.0	147394	PASS
199	198	5	9	6.7	9825	PASS
275	198	10	60	28.2	41557	PASS
365	198	1	100	3.2	4674	PASS
441	198	0.01	100	13.2	19529	PASS
442	198	50	100	84.1	124032	PASS
443	442	15	24	18.3	22690	PASS