

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041922\
 Data File : BF127845.D
 Acq On : 19 Apr 2022 17:17
 Operator : CG\JU
 Sample : PB144218BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144218BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.581	554	560	563	rBV	3317119	3581176	57.36%	12.093%
2	6.569	721	728	731	rBV	2593094	3330275	53.34%	11.246%
3	6.940	787	791	795	rBB	716343	605340	9.70%	2.044%
4	7.510	881	888	891	rBV	2050405	2455655	39.33%	8.293%
5	8.222	1004	1009	1013	rBV	796505	841011	13.47%	2.840%
6	9.304	1186	1193	1196	rBV	4002702	4110541	65.84%	13.881%
7	9.986	1303	1309	1312	rBV	1338453	1247020	19.97%	4.211%
8	10.780	1437	1444	1447	rBV	3792411	3813206	61.08%	12.877%
9	11.480	1556	1563	1566	rBV	1832782	1674837	26.83%	5.656%
10	13.074	1828	1834	1837	rBV	5929020	6243236	100.00%	21.083%
11	14.121	2008	2012	2016	rBV	1357109	1144684	18.33%	3.866%
12	15.639	2265	2270	2278	rBV	436857	565452	9.06%	1.910%




Sum of corrected areas: 29612433

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041922\
Data File : BF127845.D
Acq On : 19 Apr 2022 17:17
Operator : CG\JU
Sample : PB144218BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144218BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

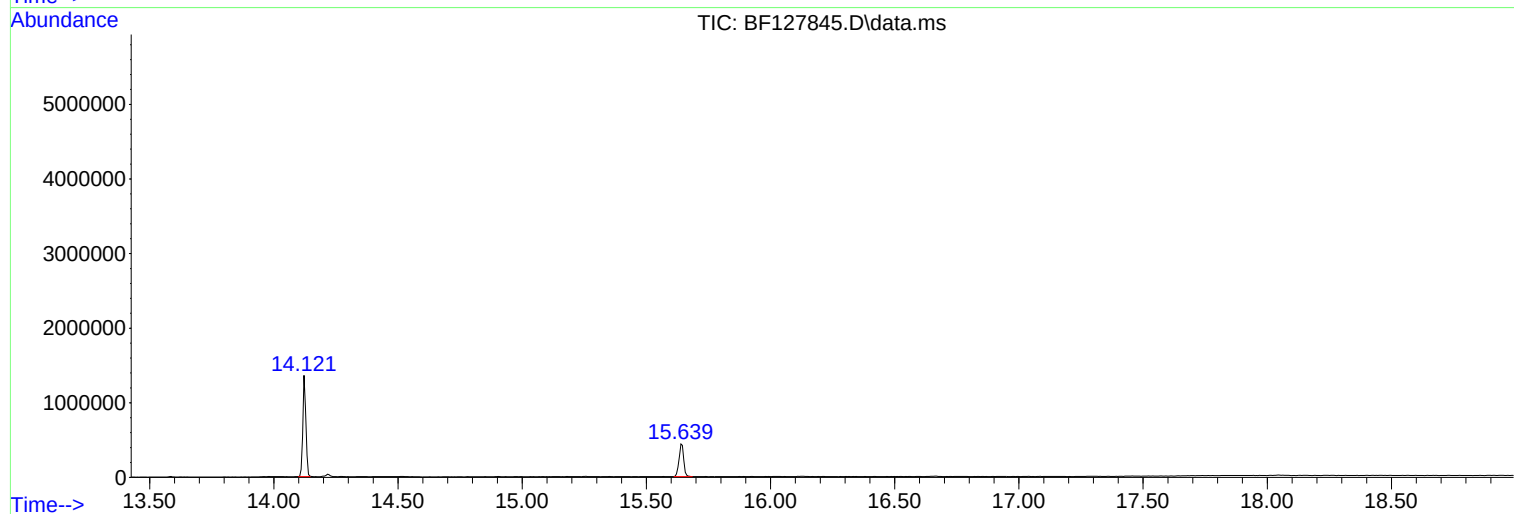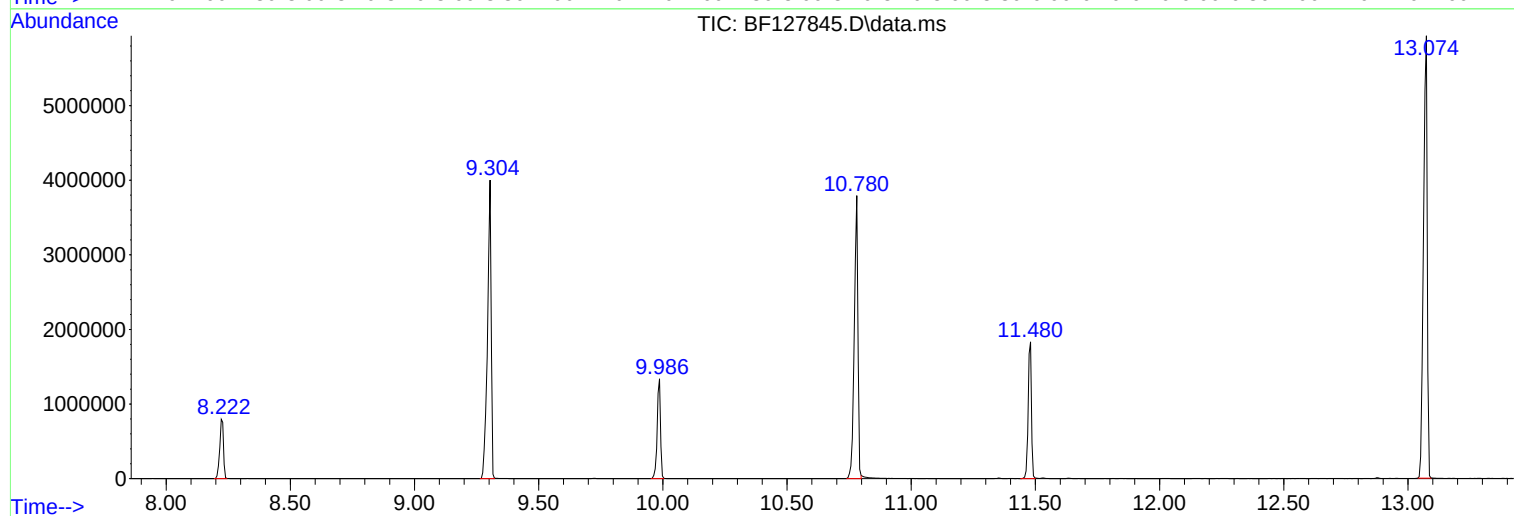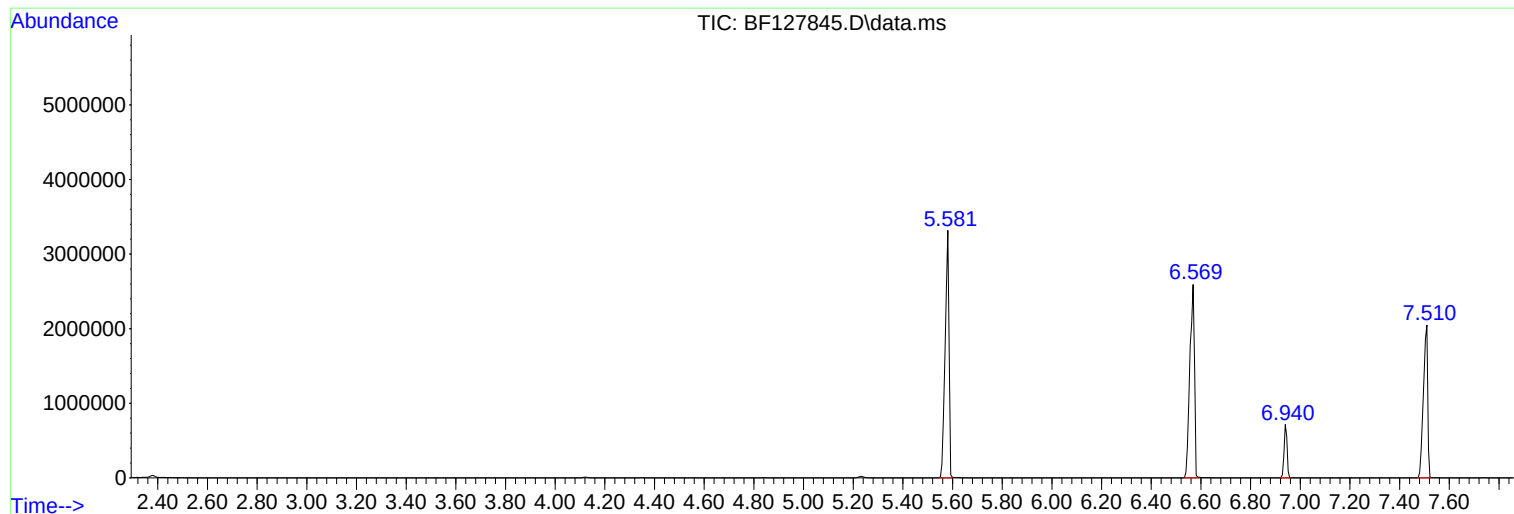

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041922\
Data File : BF127845.D
Acq On : 19 Apr 2022 17:17
Operator : CG\JU
Sample : PB144218BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144218BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041922\
Data File : BF127845.D
Acq On : 19 Apr 2022 17:17
Operator : CG\JU
Sample : PB144218BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144218BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------