


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041922\
 Data File : BF127834.D
 Acq On : 19 Apr 2022 10:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 19 17:31:18 2022

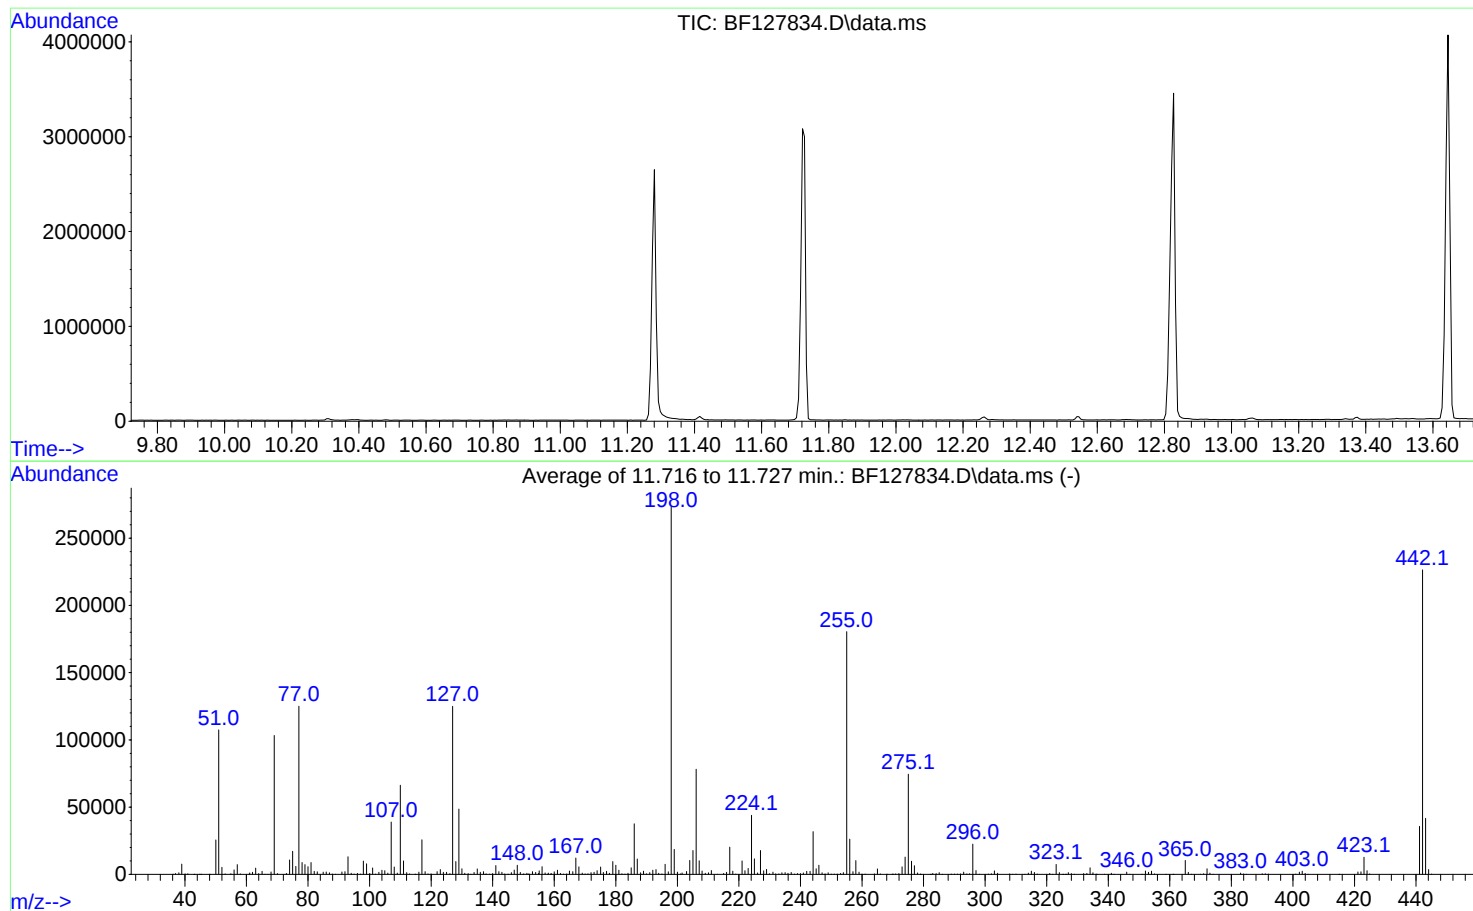




AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	107494	PASS
68	69	0.00	2	1.7	1750	PASS
69	198	0.00	100	37.8	103339	PASS
70	69	0.00	2	0.6	605	PASS
127	198	10	80	45.7	124949	PASS
197	198	0.00	2	0.7	1883	PASS
198	198	100	100	100.0	273536	PASS
199	198	5	9	6.8	18609	PASS
275	198	10	60	27.2	74453	PASS
365	198	1	100	3.8	10309	PASS
441	198	0.01	100	13.0	35659	PASS
442	442	50	100	100.0	226432	PASS
443	442	15	24	18.4	41608	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041922\
 Data File : BF127834.D
 Acq On : 19 Apr 2022 10:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 19 13:33:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 19 13:24:29 2022
 Response via : Initial Calibration

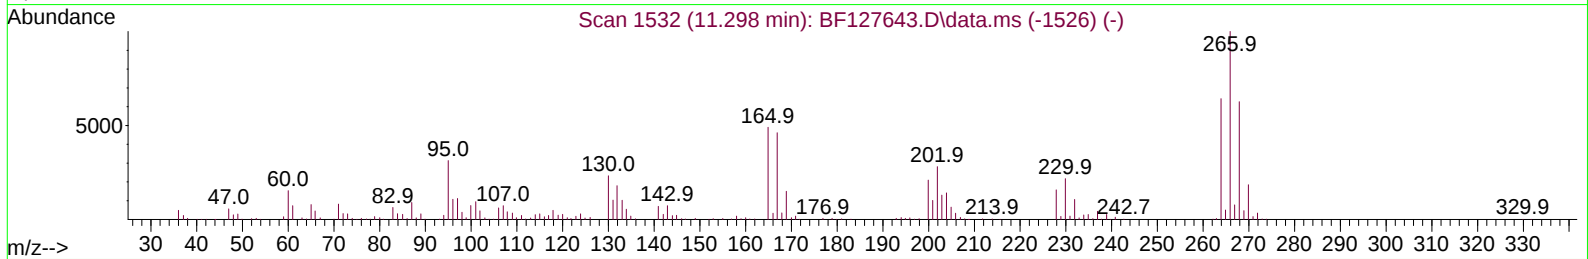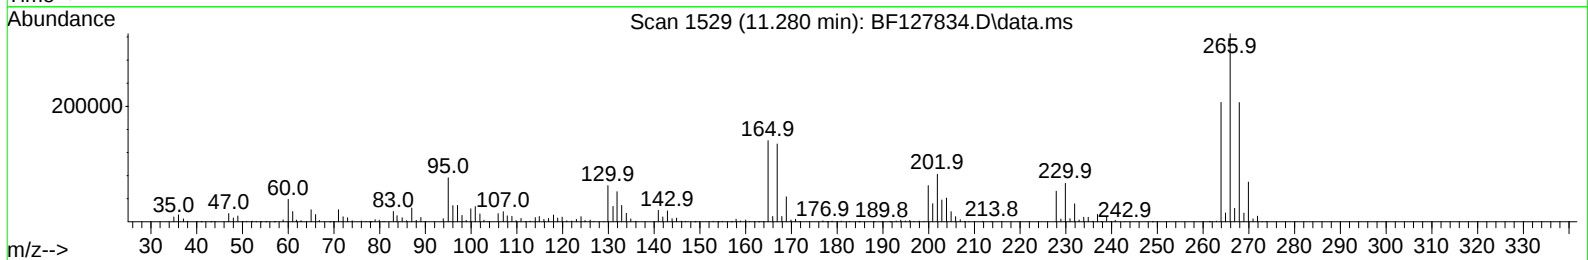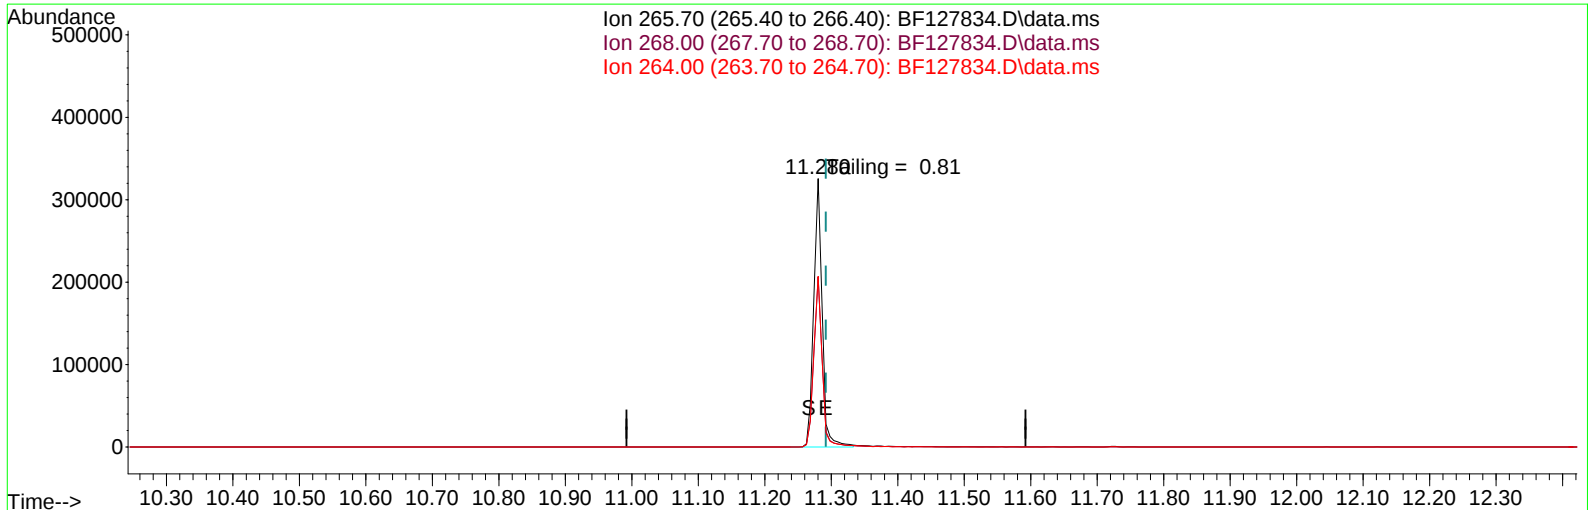

TIC: BF127834.D\data.ms

(70) Pentachlorophenol (C)

11.280min (-0.012) 228315.74 ng




response 293075

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.38
264.00	60.60	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041922\
Data File : BF127834.D
Acq On : 19 Apr 2022 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 19 13:33:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 19 13:24:29 2022
Response via : Initial Calibration

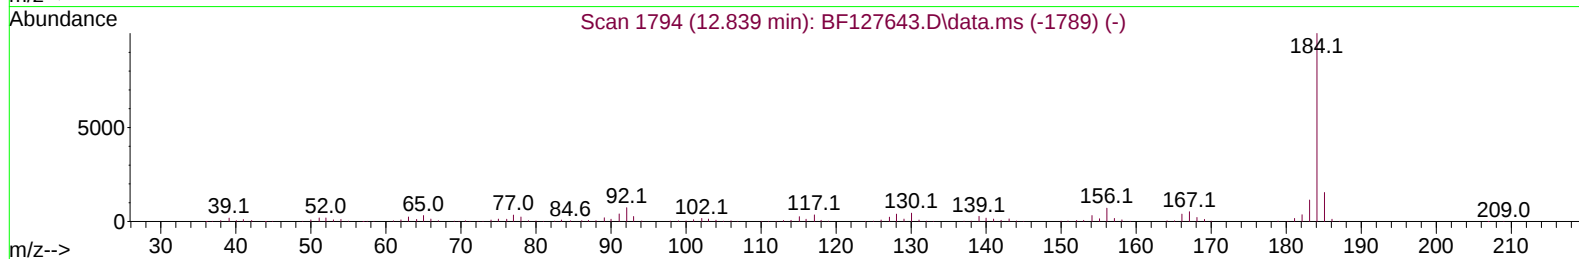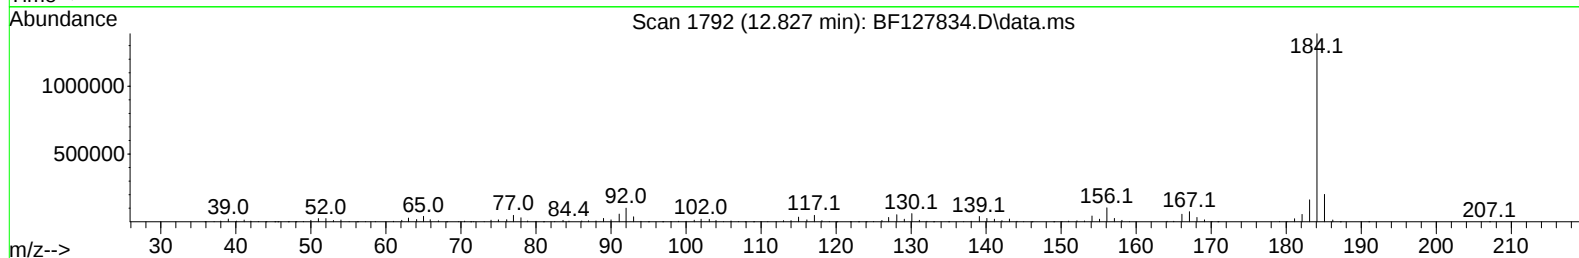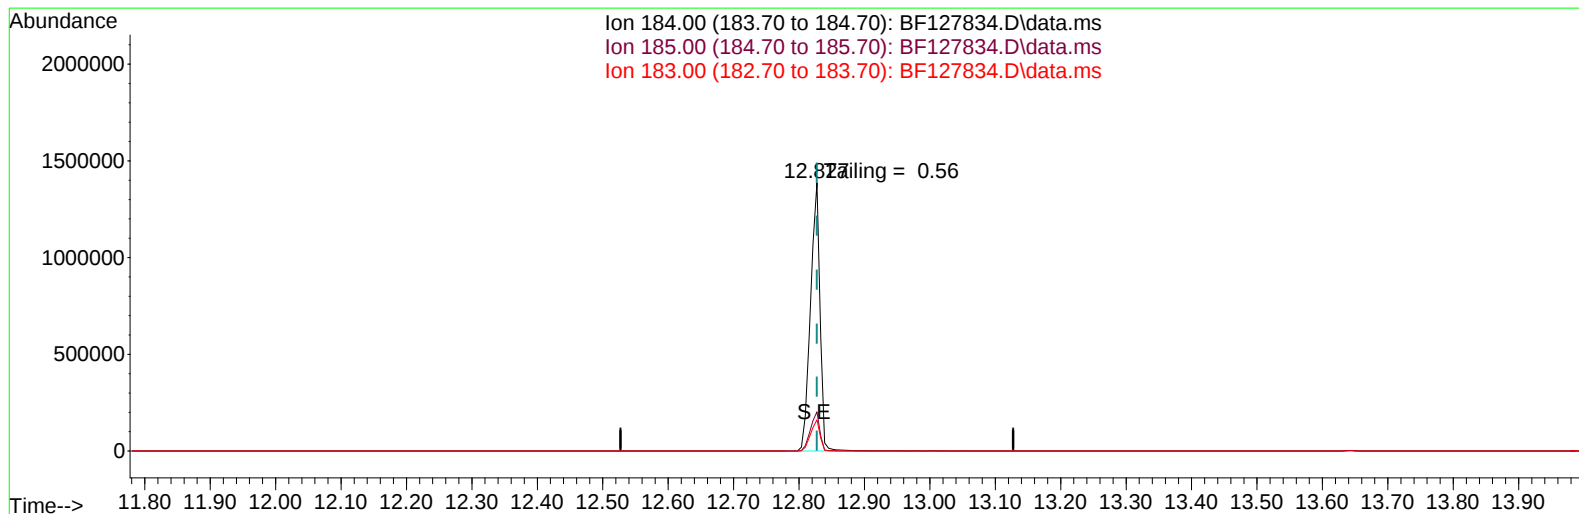

TIC: BF127834.D\data.ms

(77) Benzidine

12.827min (-0.000) 24897.60 ng

response 1388718

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.60
183.00	11.70	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/19/2022	BNA_F	<u>BF127834.D</u>
Compound Name	Response	Retention Time
DDT	700009	13.64
DDD	1524	13.33
DDE	318	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1842	701851	0.26

Instrument :
BNA_F
ClientSampleId :
DFTPP